

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111121\
 Data File : BG051010.D
 Acq On : 12 Nov 2021 22:48
 Operator : CG/JU
 Sample : M4542-02
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BGGE8

Quant Time: Nov 15 01:03:17 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110321.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Nov 15 00:27:19 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.235	152	51876	20.000	ng/ul	0.00
20) Naphthalene-d8	11.061	136	233138	20.000	ng/ul	-0.01
38) Acenaphthene-d10	14.862	164	152160	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.606	188	314097	20.000	ng/ul	-0.01
79) Chrysene-d12	21.907	240	246918	20.000	ng/ul	-0.01
88) Perylene-d12	25.326	264	247401	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.599	96	6266	3.898	ng/uL	0.00
4) Pyridine-d5	4.046	84	37052	7.706	ng/ul	-0.02
7) Phenol-d5	7.383	99	34174	6.175	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.553	67	104272	29.167	ng/ul	0.00
11) 2-Chlorophenol-d4	7.765	132	90771	23.667	ng/ul	0.00
15) 4-Methylphenol-d8	8.940	113	66425	15.246	ng/ul	0.00
21) Nitrobenzene-d5	9.410	128	65140	32.879	ng/ul	-0.01
24) 2-Nitrophenol-d4	10.138	143	70728	32.106	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.679	165	108043	29.115	ng/ul	0.00
31) 4-Chloroaniline-d4	11.196	131	87789	15.622	ng/ul	-0.01
46) Dimethylphthalate-d6	14.257	166	416300	35.761	ng/ul	-0.01
49) Acenaphthylene-d8	14.563	160	493576	34.031	ng/ul	0.00
54) 4-Nitrophenol-d4	15.062	143	16440	7.789	ng/ul	0.00
60) Fluorene-d10	15.849	176	356424	34.562	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.967	200	65153	34.214	ng/ul	-0.01
73) Anthracene-d10	17.706	188	559344	37.666	ng/ul	0.00
81) Pyrene-d10	19.986	212	575905	36.111	ng/ul	0.00
92) Benzo(a)pyrene-d12	25.091	264	478099	34.957	ng/ul	-0.01
Target Compounds						
47) Dimethylphthalate	14.304	163	16458	1.414	ng/ul#	Qvalue 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111121\
Data File : BG051010.D
Acq On : 12 Nov 2021 22:48
Operator : CG/JU
Sample : M4542-02
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BGGE8

Quant Time: Nov 15 01:03:17 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110321.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Nov 15 00:27:19 2021
Response via : Initial Calibration

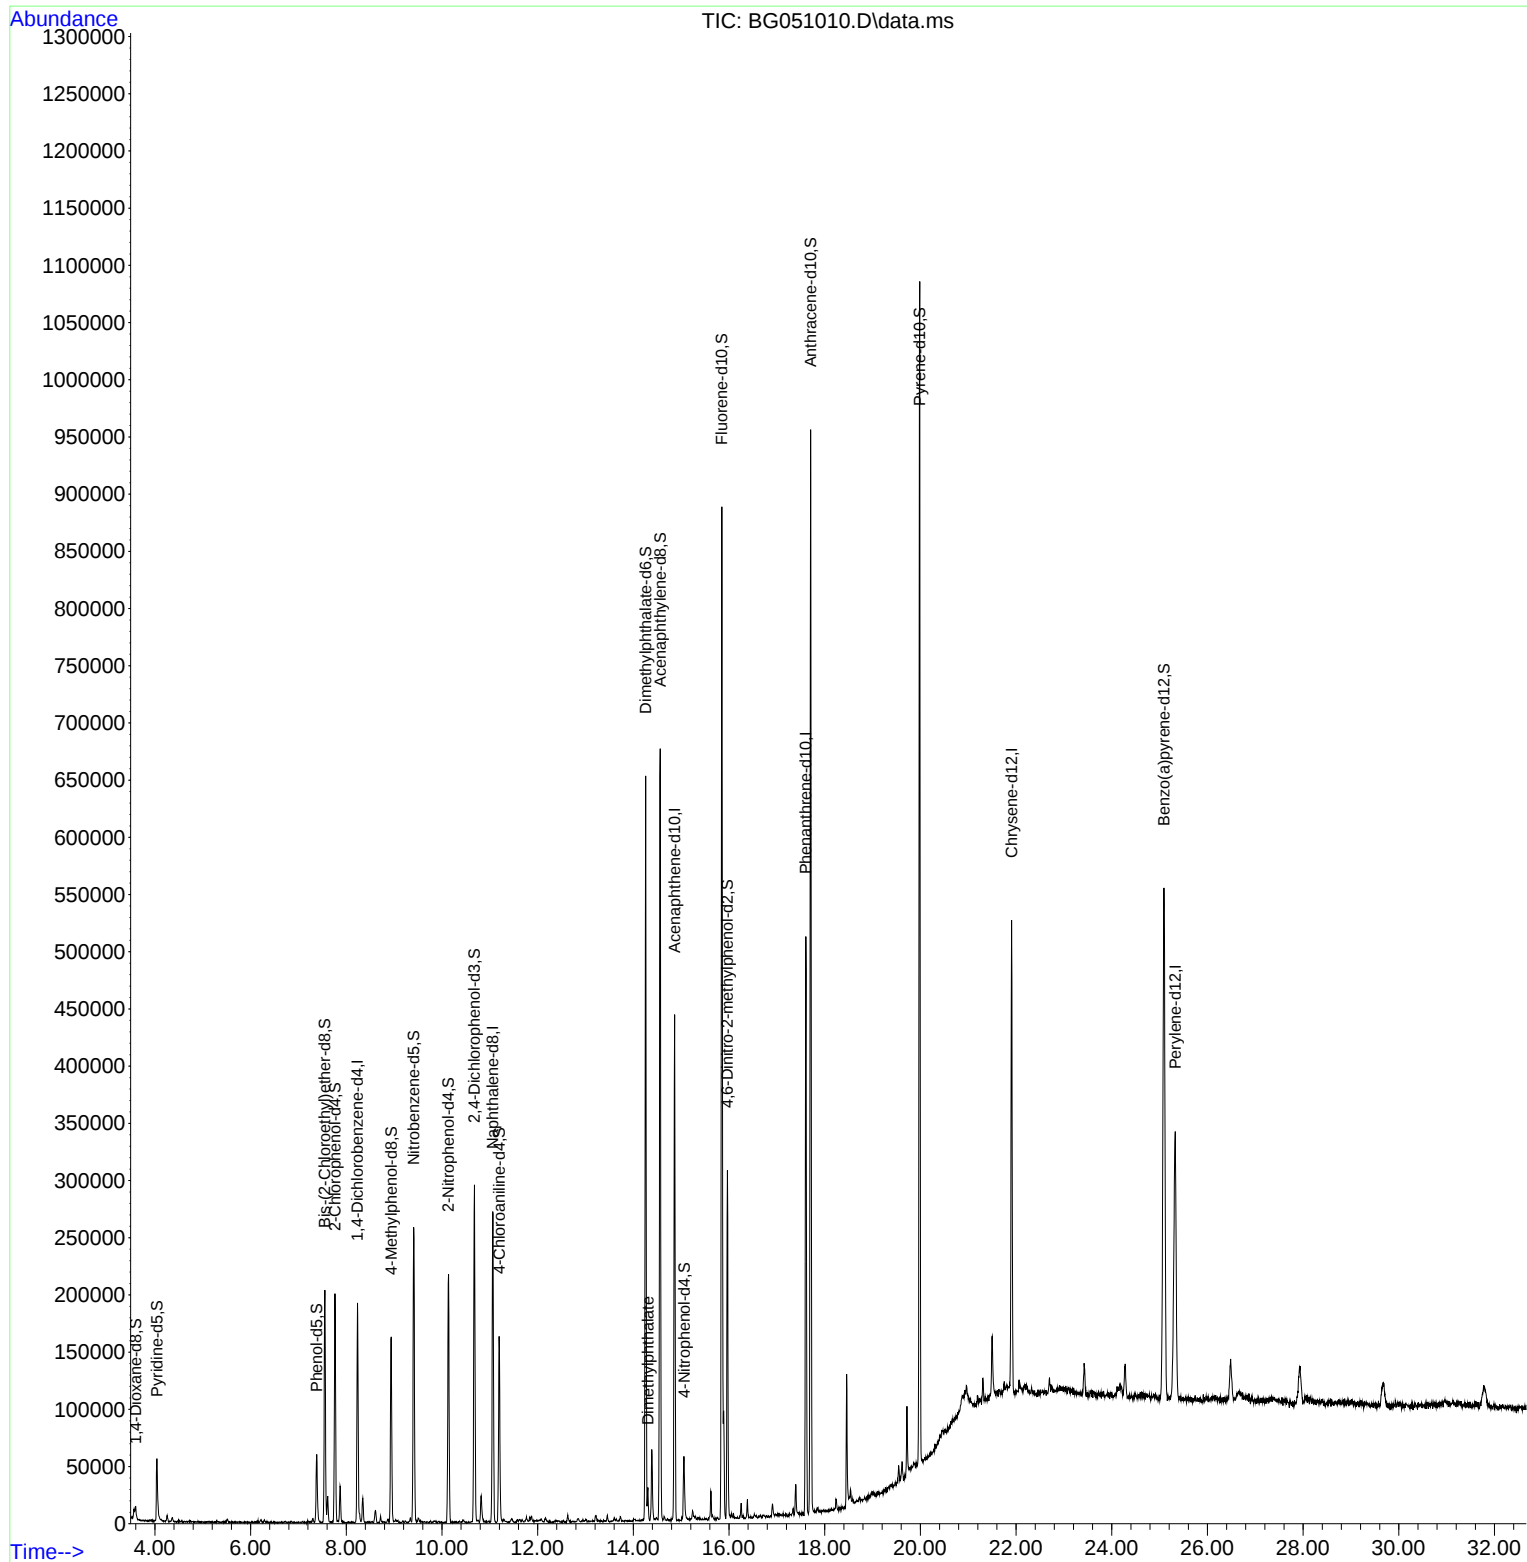

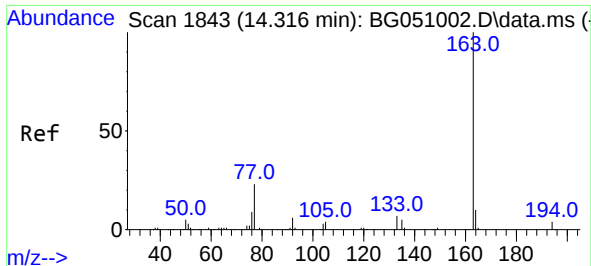

#47
Dimethylphthalate
Concen: 1.414 ng/ul
RT: 14.304 min Scan# 11
Delta R.T. -0.012 min
Lab File: BG051010.D
Acq: 12 Nov 2021 22:48

Instrument :
BNA_G
ClientSampleId :
BGGE8

Tgt Ion:163 Resp: 16458
Ion Ratio Lower Upper
163 100
194 4.5 3.0 4.4#
164 11.0 8.2 12.4

