

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111121\
 Data File : BG051012.D
 Acq On : 13 Nov 2021 00:10
 Operator : CG/JU
 Sample : M4542-03
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BGGE9

Quant Time: Nov 15 01:10:27 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110321.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Nov 15 00:27:19 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.235	152	45071	20.000	ng/u1	0.00
20) Naphthalene-d8	11.061	136	203393	20.000	ng/u1	-0.01
38) Acenaphthene-d10	14.863	164	132072	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.606	188	283007	20.000	ng/u1	-0.01
79) Chrysene-d12	21.907	240	222047	20.000	ng/u1	-0.01
88) Perylene-d12	25.321	264	220112	20.000	ng/u1	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.593	96	3409	2.441	ng/uL	0.00
4) Pyridine-d5	4.040	84	24814	5.940	ng/u1	-0.02
7) Phenol-d5	7.383	99	25361	5.274	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.548	67	77598	24.983	ng/u1	-0.01
11) 2-Chlorophenol-d4	7.765	132	66871	20.068	ng/u1	0.00
15) 4-Methylphenol-d8	8.934	113	48186	12.730	ng/u1	-0.01
21) Nitrobenzene-d5	9.410	128	48726	28.191	ng/u1	-0.01
24) 2-Nitrophenol-d4	10.139	143	51509	26.801	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.679	165	81229	25.091	ng/u1	0.00
31) 4-Chloroaniline-d4	11.196	131	67513	13.771	ng/u1	-0.01
46) Dimethylphthalate-d6	14.257	166	314297	31.105	ng/u1	-0.01
49) Acenaphthylene-d8	14.557	160	374045	29.712	ng/u1	-0.01
54) 4-Nitrophenol-d4	15.056	143	11692	6.382	ng/u1	0.00
60) Fluorene-d10	15.850	176	269887	30.151	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.967	200	50549	29.461	ng/u1	-0.01
73) Anthracene-d10	17.706	188	449321	33.581	ng/u1	0.00
81) Pyrene-d10	19.980	212	486351	33.912	ng/u1	-0.01
92) Benzo(a)pyrene-d12	25.086	264	393194	32.313	ng/u1	-0.02
Target Compounds						
47) Dimethylphthalate	14.304	163	15475	1.532	ng/u1	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111121\
Data File : BG051012.D
Acq On : 13 Nov 2021 00:10
Operator : CG/JU
Sample : M4542-03
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BGGE9

Quant Time: Nov 15 01:10:27 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110321.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Nov 15 00:27:19 2021
Response via : Initial Calibration

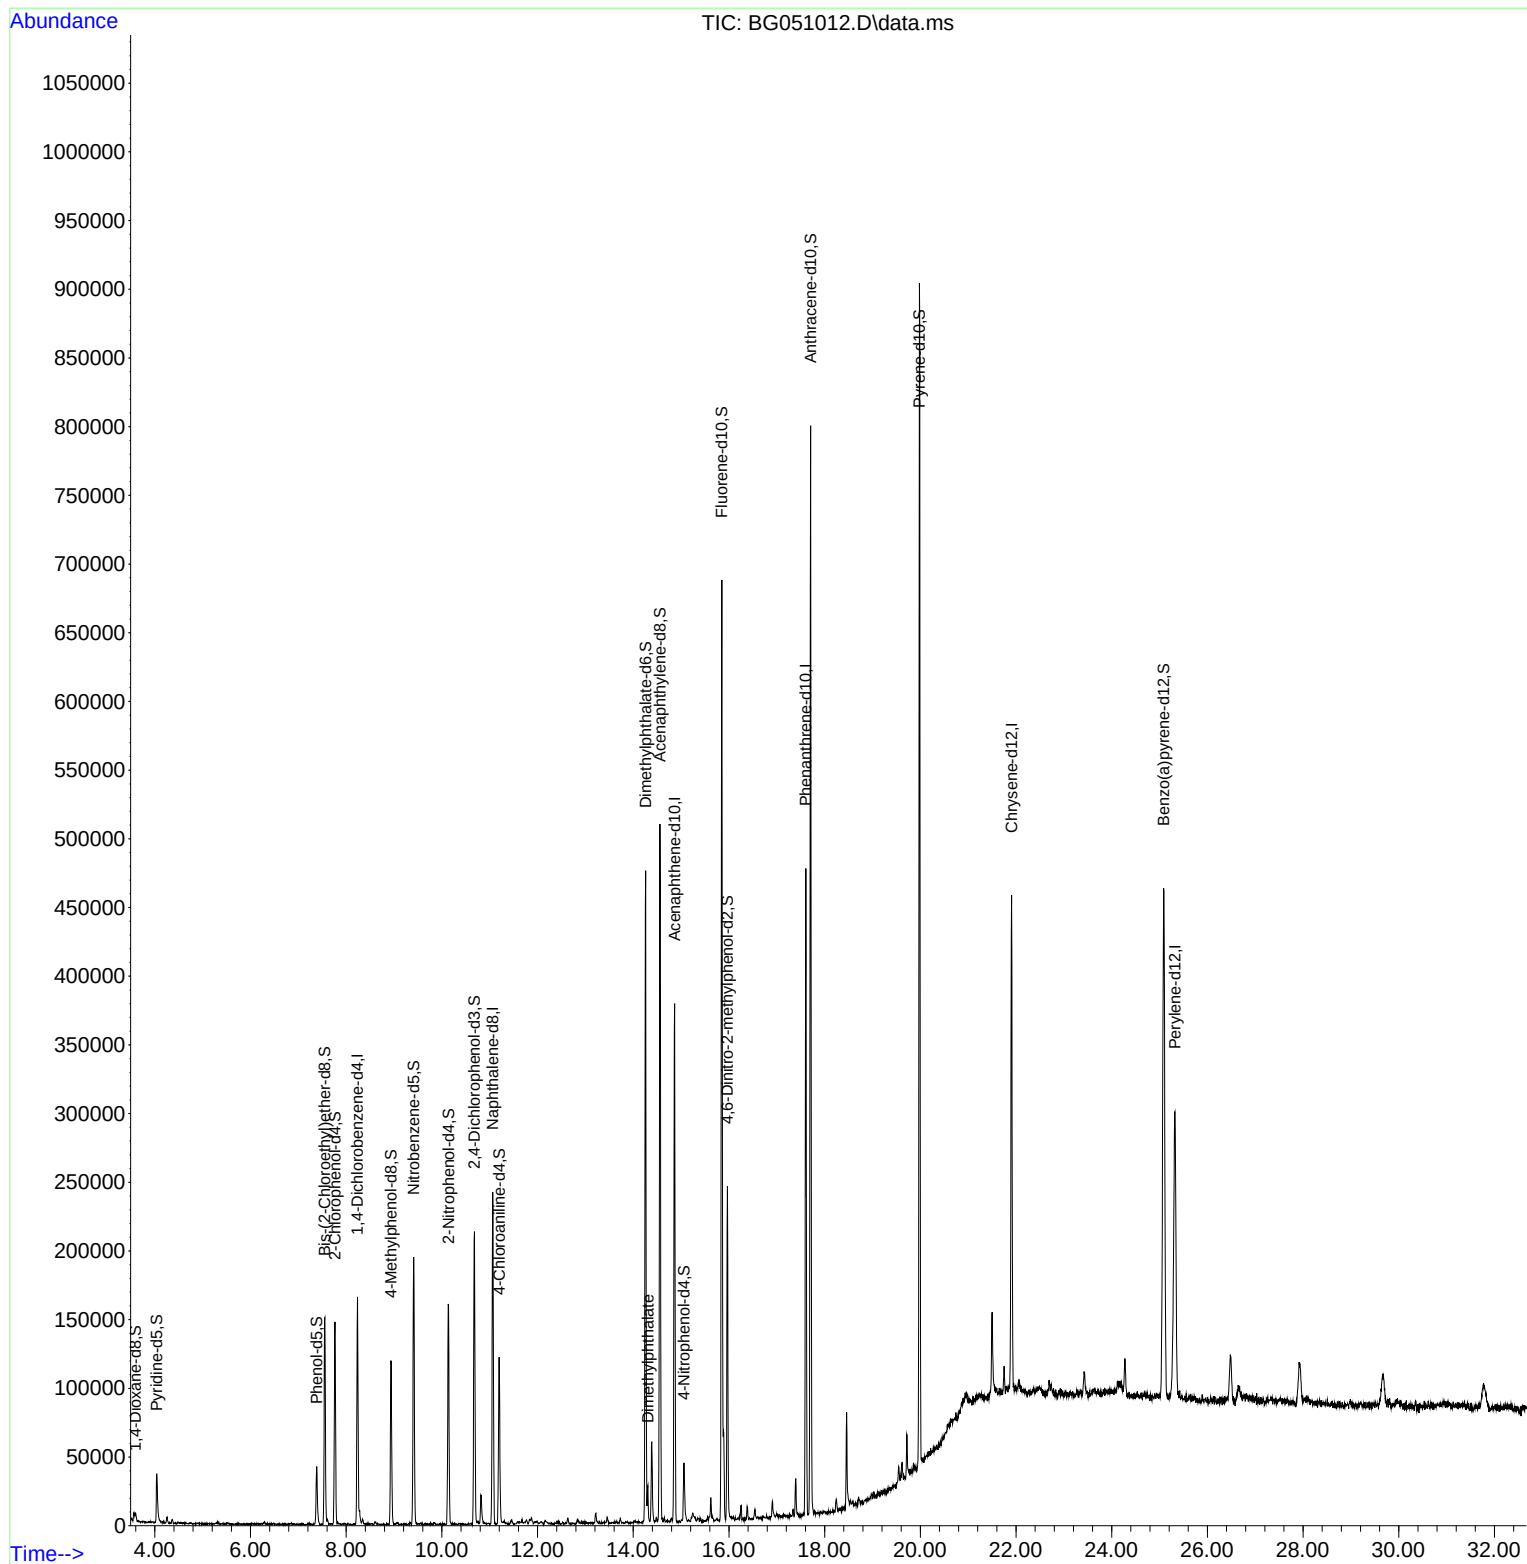

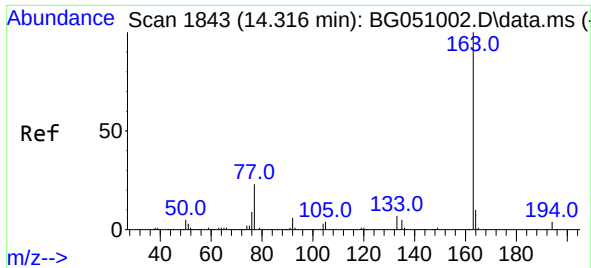

#47
 Dimethylphthalate
 Concen: 1.532 ng/ul
 RT: 14.304 min Scan# 11
 Delta R.T. -0.012 min
 Lab File: BG051012.D
 Acq: 13 Nov 2021 00:10

Instrument :
 BNA_G
 ClientSampleId :
 BGGE9

Tgt Ion:163 Resp: 15475
 Ion Ratio Lower Upper
 163 100
 194 3.3 3.0 4.4
 164 9.8 8.2 12.4

