

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111121\
 Data File : BG050964.D
 Acq On : 11 Nov 2021 11:58
 Operator : CG/JU
 Sample : PB140630BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK630

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110321.M
 Title : SVOA CALIBRATION

Signal : TIC: BG050964.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.587	13	17	28	rVB	13805	22658	1.64%	0.172%
2	4.015	85	90	109	rBV	168665	312731	22.67%	2.380%
3	4.356	145	148	155	rVB4	2404	3962	0.29%	0.030%
4	7.370	654	661	671	rVB	198534	356913	25.87%	2.716%
5	7.541	683	690	700	rBV	153505	272534	19.76%	2.074%
6	7.752	718	726	735	rBV	186011	329418	23.88%	2.507%
7	8.228	800	807	814	rBV	127818	220238	15.96%	1.676%
8	8.922	917	925	939	rBV	233392	412299	29.89%	3.138%
9	9.397	999	1006	1021	rBV	194785	350041	25.37%	2.664%
10	10.126	1122	1130	1139	rBV	155490	287622	20.85%	2.189%
11	10.667	1214	1222	1237	rBV	203611	392582	28.46%	2.988%
12	11.048	1277	1287	1296	rBV	178821	333278	24.16%	2.536%
13	11.184	1302	1310	1323	rBV	228354	434935	31.53%	3.310%
14	12.623	1551	1555	1561	rBV2	2861	4885	0.35%	0.037%
15	14.239	1824	1830	1838	rBV	456835	703355	50.99%	5.353%
16	14.544	1875	1882	1890	rBV	481024	784017	56.83%	5.967%
17	14.850	1927	1934	1942	rBV	298657	471842	34.20%	3.591%
18	15.032	1959	1965	1985	rBV	173287	329054	23.85%	2.504%
19	15.837	2095	2102	2112	rVB	645105	989821	71.75%	7.533%
20	15.954	2116	2122	2137	rVV	188976	305762	22.16%	2.327%
21	16.078	2140	2143	2146	rVB	2152	2340	0.17%	0.018%
22	17.376	2361	2364	2370	rBV3	1249	1911	0.14%	0.015%
23	17.594	2394	2401	2409	rBV	377910	589337	42.72%	4.485%
24	17.694	2411	2418	2428	rVV2	733325	1159767	84.07%	8.826%
25	19.533	2727	2731	2736	rBV2	10433	14289	1.04%	0.109%
26	19.603	2738	2743	2751	rVB	8862	13951	1.01%	0.106%
27	19.967	2798	2805	2815	rVB	964136	1379530	100.00%	10.499%
28	20.831	2949	2952	2954	rBV3	1649	2341	0.17%	0.018%
29	20.954	2971	2973	2978	rVB5	3878	4402	0.32%	0.034%
30	21.001	2978	2981	2983	rBV4	1970	2004	0.15%	0.015%
31	21.448	3055	3057	3059	rBV3	1624	1720	0.12%	0.013%
32	21.477	3059	3062	3066	rVB4	3757	4502	0.33%	0.034%
33	21.513	3066	3068	3069	rBV2	1805	1537	0.11%	0.012%
34	21.595	3077	3082	3087	rBV5	4226	7420	0.54%	0.056%
35	21.806	3116	3118	3122	rBV5	1830	2299	0.17%	0.017%
36	21.889	3125	3132	3142	rVB	361652	609834	44.21%	4.641%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111121\
 Data File : BG050964.D
 Acq On : 11 Nov 2021 11:58
 Operator : CG/JU
 Sample : PB140630BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK630

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110321.M
 Title : SVOA CALIBRATION

37	22.511	3235	3238	3240	rBV4	1513	1841	0.13%	0.014%
38	22.688	3264	3268	3271	rVV6	2583	4150	0.30%	0.032%
39	23.034	3326	3327	3330	rBV3	1218	1552	0.11%	0.012%
40	23.410	3386	3391	3395	rVB5	4708	8208	0.59%	0.062%
41	23.522	3409	3410	3412	rBV2	2194	1463	0.11%	0.011%
42	23.610	3419	3425	3432	rBV4	8452	17677	1.28%	0.135%
43	23.681	3435	3437	3439	rBV2	1431	1464	0.11%	0.011%
44	23.751	3445	3449	3450	rBV4	1404	1399	0.10%	0.011%
45	24.027	3494	3496	3498	rBV3	1603	1746	0.13%	0.013%
46	24.139	3513	3515	3520	rVB5	1451	2146	0.16%	0.016%
47	24.256	3529	3535	3542	rVB6	8207	17778	1.29%	0.135%
48	25.050	3658	3670	3682	rBV2	427144	1252664	90.80%	9.533%
49	25.279	3697	3709	3721	rBV2	197420	619070	44.88%	4.711%
50	25.843	3803	3805	3807	rVB3	3095	2401	0.17%	0.018%
51	25.860	3807	3808	3810	rBV2	2009	1699	0.12%	0.013%
52	26.160	3856	3859	3861	rBV2	1972	1715	0.12%	0.013%
53	26.448	3901	3908	3918	rVB8	10993	33715	2.44%	0.257%
54	26.730	3955	3956	3963	rBV6	1778	3252	0.24%	0.025%
55	27.882	4144	4152	4154	rBV4	9829	21576	1.56%	0.164%
56	28.017	4173	4175	4178	rBV4	1300	1910	0.14%	0.015%
57	28.117	4190	4192	4194	rBV3	1692	1534	0.11%	0.012%
58	28.328	4227	4228	4231	rBV3	1594	1895	0.14%	0.014%
59	28.381	4236	4237	4240	rVV2	2035	1417	0.10%	0.011%
60	28.598	4271	4274	4275	rBV3	1518	1695	0.12%	0.013%
61	28.739	4296	4298	4300	rBV3	1583	1713	0.12%	0.013%
62	29.609	4440	4446	4447	rBV6	5002	7690	0.56%	0.059%
63	30.056	4519	4522	4524	rBV3	1511	1955	0.14%	0.015%
64	30.138	4534	4536	4541	rBV6	1510	2037	0.15%	0.016%
65	30.443	4586	4588	4591	rBV4	1386	1397	0.10%	0.011%
66	31.654	4792	4794	4796	rBV3	1885	1682	0.12%	0.013%
67	31.707	4801	4803	4805	rVV3	2586	2490	0.18%	0.019%
68	32.165	4879	4881	4885	rVB5	1708	1895	0.14%	0.014%




Sum of corrected areas: 13139957

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111121\
Data File : BG050964.D
Acq On : 11 Nov 2021 11:58
Operator : CG/JU
Sample : PB140630BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK630

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110321.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

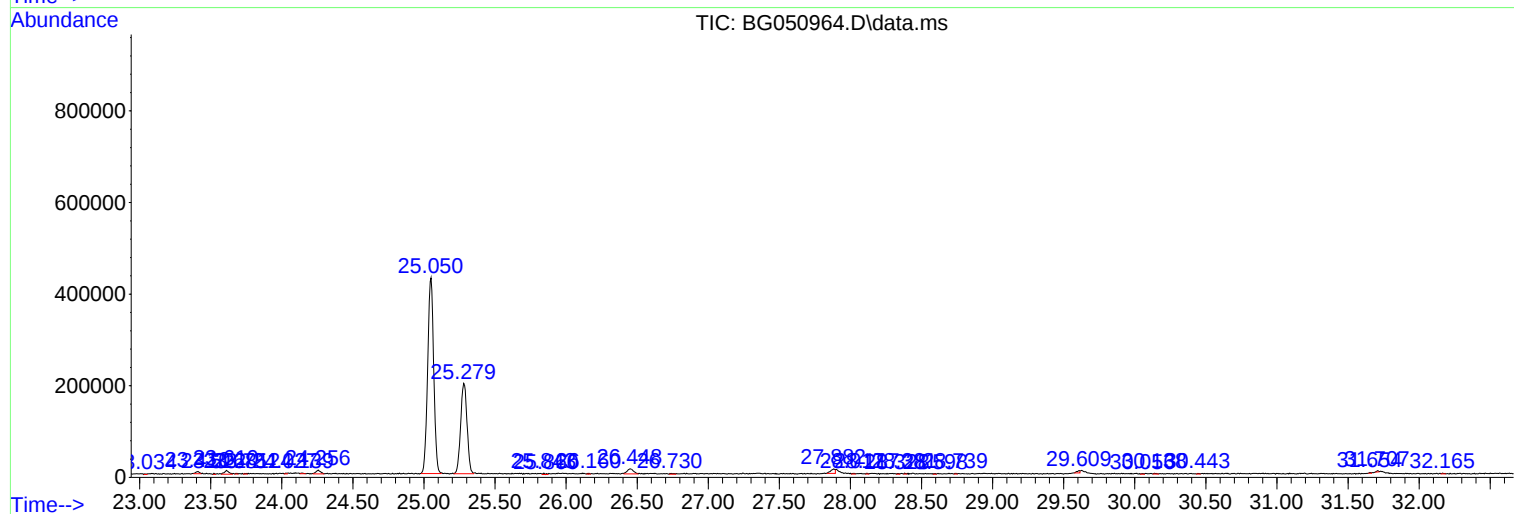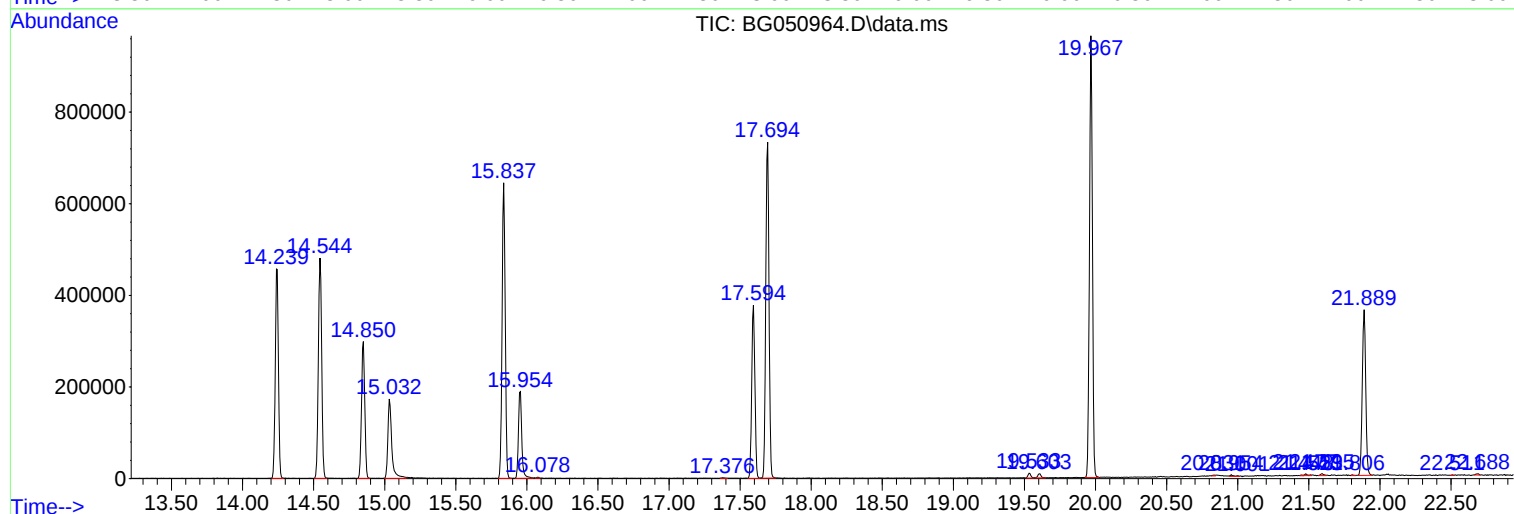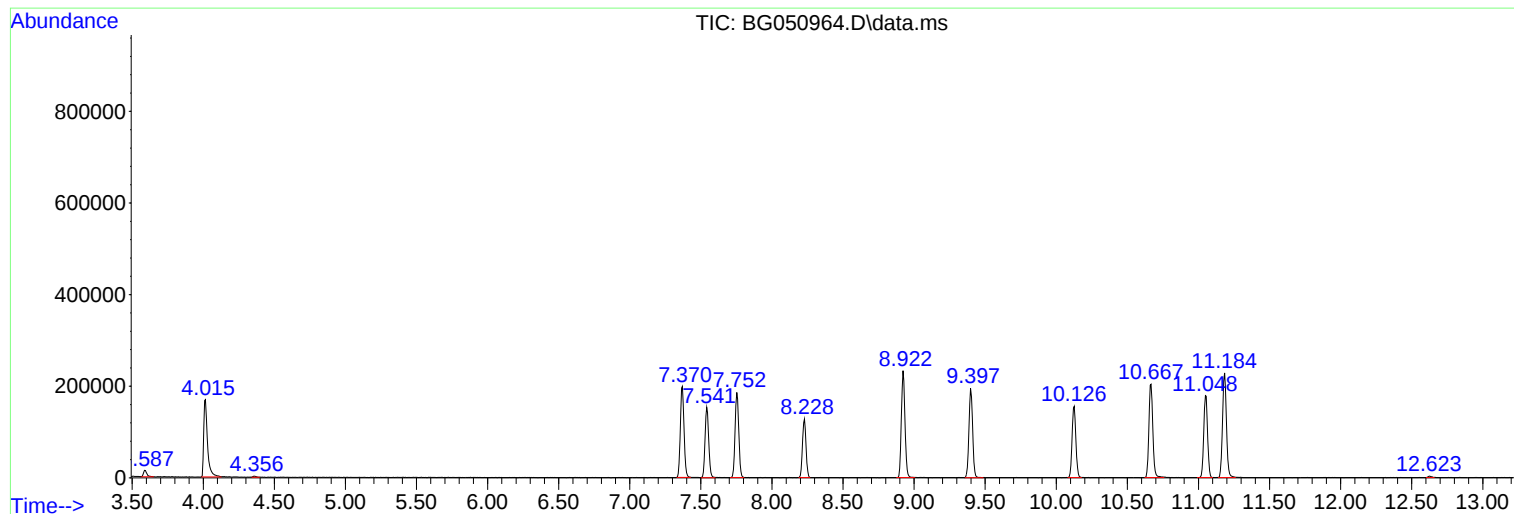

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111121\
Data File : BG050964.D
Acq On : 11 Nov 2021 11:58
Operator : CG/JU
Sample : PB140630BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK630

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110321.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111121\
Data File : BG050964.D
Acq On : 11 Nov 2021 11:58
Operator : CG/JU
Sample : PB140630BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK630

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110321.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
