

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111121\
 Data File : BG050984.D
 Acq On : 12 Nov 2021 2:38
 Operator : CG/JU
 Sample : M4522-14
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BG327

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110321.M
 Title : SVOA CALIBRATION

Signal : TIC: BG050984.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.589	13	17	24	rVB	9519	14956	1.26%	0.142%
2	4.024	86	91	105	rBV2	31750	62895	5.30%	0.596%
3	4.253	125	130	137	rVB2	5278	9535	0.80%	0.090%
4	4.358	145	148	152	rVV2	2203	3012	0.25%	0.029%
5	4.488	165	170	172	rBV2	892	1529	0.13%	0.014%
6	4.893	235	239	240	rBV2	1539	1558	0.13%	0.015%
7	5.704	374	377	380	rVB2	1045	1433	0.12%	0.014%
8	7.373	655	661	668	rBV2	39022	70000	5.89%	0.663%
9	7.543	683	690	698	rBV	126676	210950	17.76%	1.998%
10	7.754	719	726	734	rBV	117707	208531	17.56%	1.975%
11	7.825	734	738	741	rVB2	1251	1343	0.11%	0.013%
12	8.230	799	807	819	rVB	116528	205864	17.34%	1.950%
13	8.924	919	925	934	rBV	101350	184792	15.56%	1.750%
14	9.400	997	1006	1017	rBV	152504	284126	23.93%	2.691%
15	10.128	1122	1130	1139	rBV	125784	229982	19.37%	2.178%
16	10.669	1215	1222	1232	rBV	161134	302837	25.50%	2.868%
17	10.810	1241	1246	1255	rBV3	4166	9794	0.82%	0.093%
18	11.051	1279	1287	1295	rBV	168043	315716	26.59%	2.990%
19	11.186	1302	1310	1327	rBV	147764	283953	23.91%	2.689%
20	11.562	1370	1374	1379	rBV2	1915	2651	0.22%	0.025%
21	11.615	1379	1383	1385	rBV2	2129	2737	0.23%	0.026%
22	12.625	1550	1555	1562	rVB3	3412	5509	0.46%	0.052%
23	13.448	1690	1695	1699	rBV3	1875	2756	0.23%	0.026%
24	14.241	1824	1830	1842	rVB	387800	580529	48.88%	5.498%
25	14.546	1875	1882	1889	rBV	413784	669152	56.35%	6.337%
26	14.852	1927	1934	1941	rBV	290672	454757	38.29%	4.307%
27	15.046	1961	1967	1982	rBV2	28895	69060	5.82%	0.654%
28	15.616	2060	2064	2067	rBV2	1263	1966	0.17%	0.019%
29	15.651	2067	2070	2075	rVB2	854	1227	0.10%	0.012%
30	15.839	2095	2102	2112	rVB	564942	863495	72.71%	8.177%
31	15.951	2115	2121	2133	rBV	190976	305609	25.73%	2.894%
32	16.074	2140	2142	2148	rVB3	1712	2243	0.19%	0.021%
33	17.384	2361	2365	2367	rBV2	1224	1596	0.13%	0.015%
34	17.596	2394	2401	2408	rBV	359251	553331	46.59%	5.240%
35	17.696	2411	2418	2426	rVV	663229	1031231	86.84%	9.766%
36	17.848	2441	2444	2449	rVV3	1011	1428	0.12%	0.014%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111121\
 Data File : BG050984.D
 Acq On : 12 Nov 2021 2:38
 Operator : CG/JU
 Sample : M4522-14
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BG327

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110321.M
 Title : SVOA CALIBRATION

37	17.966	2461	2464	2466	rBV3	971	1231	0.10%	0.012%
38	18.178	2496	2500	2505	rBV3	786	1429	0.12%	0.014%
39	18.230	2505	2509	2514	rBV4	3863	4837	0.41%	0.046%
40	18.536	2556	2561	2563	rBV2	1890	2553	0.21%	0.024%
41	19.182	2668	2671	2674	rBV3	1067	1413	0.12%	0.013%
42	19.417	2708	2711	2714	rVB3	1013	1272	0.11%	0.012%
43	19.535	2727	2731	2737	rVB4	8495	12112	1.02%	0.115%
44	19.605	2740	2743	2748	rVB2	7987	12085	1.02%	0.114%
45	19.858	2783	2786	2787	rBV2	1527	1453	0.12%	0.014%
46	19.970	2797	2805	2816	rBV	806998	1187552	100.00%	11.246%
47	20.128	2830	2832	2834	rVB3	1593	1377	0.12%	0.013%
48	20.187	2840	2842	2845	rBV4	1277	1549	0.13%	0.015%
49	20.398	2875	2878	2879	rBV3	1812	2479	0.21%	0.023%
50	20.445	2884	2886	2888	rBV3	2532	3020	0.25%	0.029%
51	20.551	2901	2904	2905	rBV3	2131	2354	0.20%	0.022%
52	20.675	2923	2925	2927	rBV3	1439	1220	0.10%	0.012%
53	20.757	2937	2939	2941	rBV3	1613	1418	0.12%	0.013%
54	20.839	2948	2953	2954	rBV4	4833	7052	0.59%	0.067%
55	20.962	2970	2974	2975	rBV4	3267	4300	0.36%	0.041%
56	21.039	2985	2987	2988	rVB2	2439	1427	0.12%	0.014%
57	21.245	3020	3022	3023	rBV2	2031	1690	0.14%	0.016%
58	21.356	3039	3041	3043	rVB2	3376	1807	0.15%	0.017%
59	21.380	3043	3045	3047	rBV3	1962	1590	0.13%	0.015%
60	21.491	3060	3064	3074	rBV8	17019	46446	3.91%	0.440%
61	21.738	3104	3106	3113	rVB7	5107	7272	0.61%	0.069%
62	21.891	3125	3132	3141	rVB	311987	545730	45.95%	5.168%
63	22.343	3207	3209	3211	rVB3	3224	1674	0.14%	0.016%
64	22.678	3262	3266	3273	rBV8	5356	11657	0.98%	0.110%
65	22.884	3299	3301	3302	rBV2	2788	1801	0.15%	0.017%
66	23.407	3388	3390	3397	rVB8	8313	14102	1.19%	0.134%
67	24.253	3531	3534	3540	rVB4	8845	15789	1.33%	0.150%
68	24.341	3547	3549	3551	rVB3	2744	1517	0.13%	0.014%
69	25.052	3659	3670	3684	rVB2	359535	1059090	89.18%	10.030%
70	25.287	3699	3710	3722	rVB2	178317	567410	47.78%	5.373%
71	25.539	3752	3753	3754	rBV	3035	1673	0.14%	0.016%
72	26.215	3866	3868	3870	rBV3	2553	2047	0.17%	0.019%
73	26.303	3881	3883	3887	rBV4	2688	3428	0.29%	0.032%
74	26.450	3903	3908	3909	rBV5	9736	13007	1.10%	0.123%
75	26.797	3965	3967	3970	rVB4	2873	2240	0.19%	0.021%
76	27.602	4102	4104	4106	rBV2	2624	2527	0.21%	0.024%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111121\
Data File : BG050984.D
Acq On : 12 Nov 2021 2:38
Operator : CG/JU
Sample : M4522-14
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BG327

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110321.M
Title : SVOA CALIBRATION

77	27.837	4142	4144	4146	rBV3	3026	2165	0.18%	0.021%
78	27.890	4146	4153	4161	rVV8	12153	38438	3.24%	0.364%
79	28.460	4248	4250	4252	rVB3	3570	2269	0.19%	0.021%
80	29.476	4421	4423	4425	rBV3	2544	1826	0.15%	0.017%
81	29.582	4439	4441	4442	rBV2	3424	2679	0.23%	0.025%
82	31.609	4784	4786	4787	rBV2	2622	1293	0.11%	0.012%
83	32.008	4852	4854	4856	rBV3	2902	2512	0.21%	0.024%
84	32.543	4944	4945	4946	rBV	3121	1548	0.13%	0.015%




Sum of corrected areas: 10559443

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111121\
Data File : BG050984.D
Acq On : 12 Nov 2021 2:38
Operator : CG/JU
Sample : M4522-14
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BG327

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110321.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

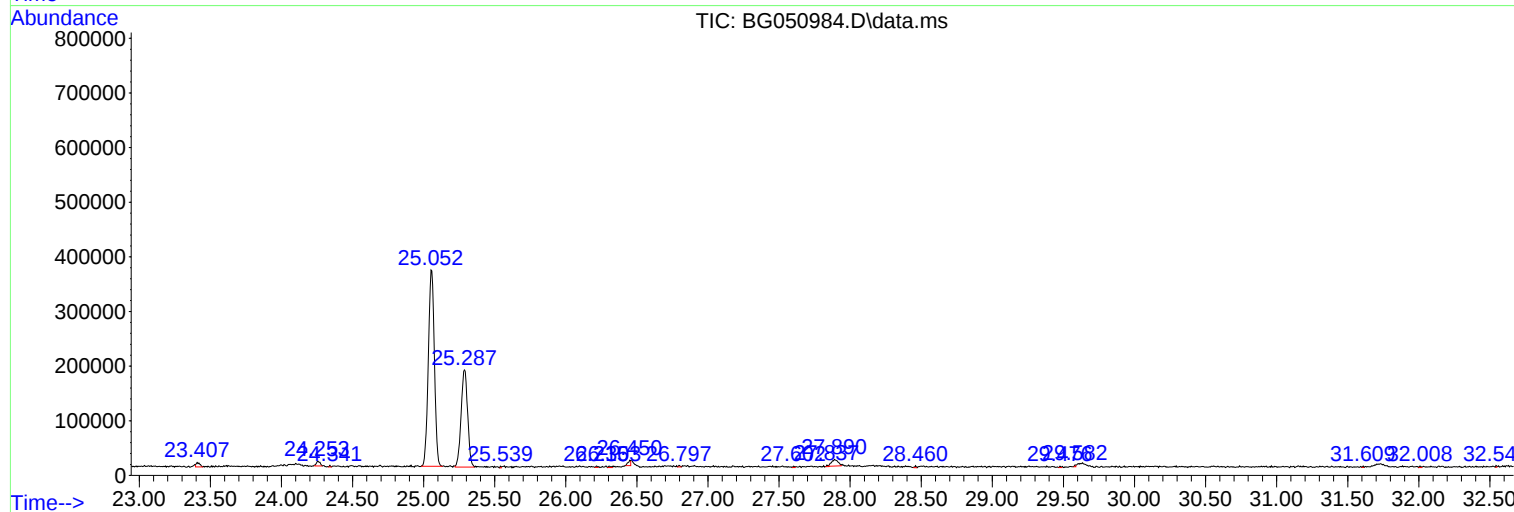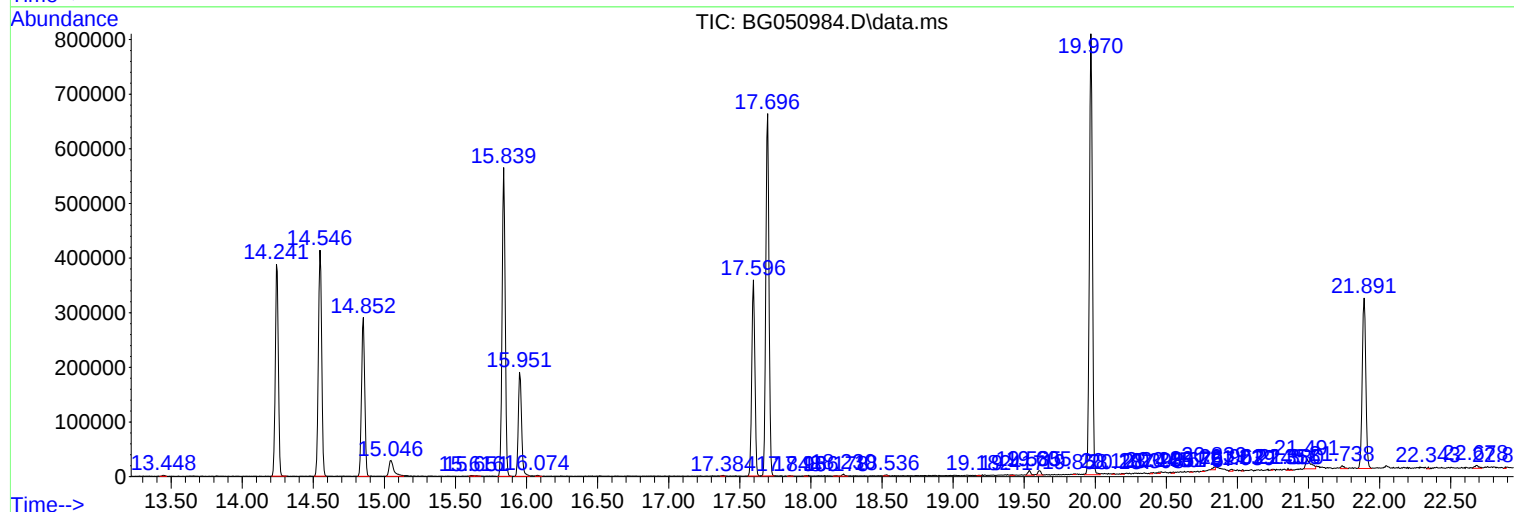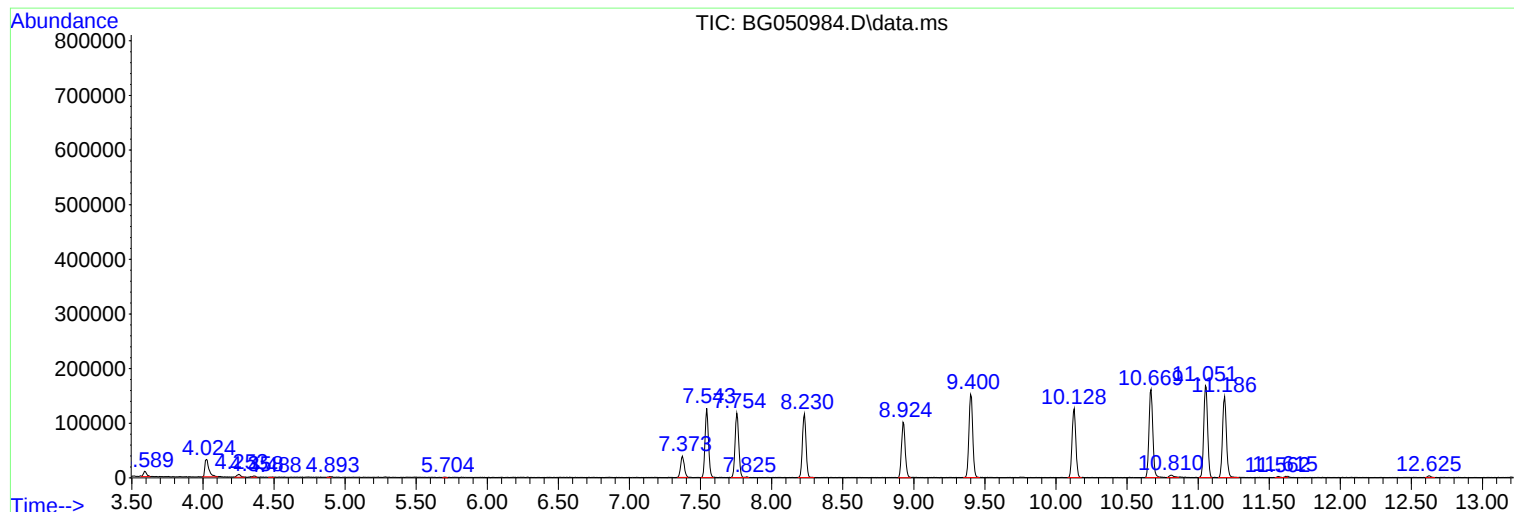

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111121\
Data File : BG050984.D
Acq On : 12 Nov 2021 2:38
Operator : CG/JU
Sample : M4522-14
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BG327

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110321.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111121\
Data File : BG050984.D
Acq On : 12 Nov 2021 2:38
Operator : CG/JU
Sample : M4522-14
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BG327

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110321.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
