

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111121\
 Data File : BG050992.D
 Acq On : 12 Nov 2021 8:50
 Operator : CG/JU
 Sample : PB140665BL
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK665

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110321.M
 Title : SVOA CALIBRATION

Signal : TIC: BG050992.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.587	12	17	26	rVB	15681	24199	1.57%	0.151%
2	4.010	85	89	109	rBV	181502	332092	21.51%	2.070%
3	4.175	115	117	122	rBV5	1057	1958	0.13%	0.012%
4	4.357	144	148	152	rBV	3440	4880	0.32%	0.030%
5	7.371	654	661	673	rBV	226541	395465	25.62%	2.465%
6	7.541	682	690	699	rBV	173113	298812	19.36%	1.862%
7	7.753	718	726	738	rBV	210614	369452	23.93%	2.303%
8	8.229	799	807	814	rBV	172302	300060	19.44%	1.870%
9	8.922	918	925	936	rBV	262678	474257	30.72%	2.956%
10	9.404	997	1007	1017	rBV	210971	396368	25.68%	2.470%
11	10.127	1122	1130	1140	rBV	188475	336151	21.78%	2.095%
12	10.667	1214	1222	1240	rBV	249976	464554	30.09%	2.895%
13	11.055	1280	1288	1296	rBV	253421	465711	30.17%	2.903%
14	11.184	1303	1310	1326	rBV	264462	498654	32.30%	3.108%
15	12.630	1551	1556	1563	rVB3	4268	6804	0.44%	0.042%
16	14.245	1824	1831	1838	rBV	525834	792725	51.35%	4.941%
17	14.545	1874	1882	1890	rBV	557217	920966	59.66%	5.740%
18	14.851	1927	1934	1943	rVB	430081	683742	44.29%	4.261%
19	15.039	1959	1966	1982	rBV	219526	414495	26.85%	2.583%
20	15.838	2095	2102	2111	rBV	749834	1150478	74.53%	7.170%
21	15.955	2116	2122	2132	rVV	248395	377677	24.47%	2.354%
22	16.020	2132	2133	2137	rVV2	2731	2891	0.19%	0.018%
23	16.073	2139	2142	2143	rVV2	2111	2365	0.15%	0.015%
24	16.084	2143	2144	2147	rVB2	3056	1793	0.12%	0.011%
25	17.389	2360	2366	2370	rVB	1643	2446	0.16%	0.015%
26	17.594	2394	2401	2411	rBV	587836	881244	57.09%	5.492%
27	17.694	2411	2418	2427	rVV2	835903	1312744	85.04%	8.182%
28	19.533	2723	2731	2736	rBV3	10982	17247	1.12%	0.107%
29	19.610	2738	2744	2749	rBV	9782	15743	1.02%	0.098%
30	19.968	2799	2805	2813	rBV	1031499	1543728	100.00%	9.621%
31	20.068	2819	2822	2825	rVB4	1370	1918	0.12%	0.012%
32	20.855	2944	2956	2970	rBV8	13710	57503	3.72%	0.358%
33	20.985	2977	2978	2981	rBV3	1654	2011	0.13%	0.013%
34	21.742	3105	3107	3109	rVB3	3041	1716	0.11%	0.011%
35	21.889	3125	3132	3140	rBV	498179	889978	57.65%	5.547%
36	22.295	3199	3201	3204	rVB4	2759	2173	0.14%	0.014%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111121\
 Data File : BG050992.D
 Acq On : 12 Nov 2021 8:50
 Operator : CG/JU
 Sample : PB140665BL
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK665

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110321.M
 Title : SVOA CALIBRATION

37	22.871	3297	3299	3302	rBV4	2269	2092	0.14%	0.013%
38	23.417	3386	3392	3397	rBV2	14085	27156	1.76%	0.169%
39	24.257	3529	3535	3544	rVB5	17766	41618	2.70%	0.259%
40	24.809	3628	3629	3631	rBV	2260	1792	0.12%	0.011%
41	25.056	3659	3671	3685	rVB2	462499	1378780	89.31%	8.593%
42	25.291	3698	3711	3723	rVB2	301990	931703	60.35%	5.807%
43	26.449	3900	3908	3920	rVB5	21431	64523	4.18%	0.402%
44	26.836	3972	3974	3977	rBV4	2194	2928	0.19%	0.018%
45	27.107	4018	4020	4022	rBV3	2479	1600	0.10%	0.010%
46	27.177	4030	4032	4034	rBV3	1782	1766	0.11%	0.011%
47	27.894	4146	4154	4167	rVB4	21782	77448	5.02%	0.483%
48	28.717	4292	4294	4296	rVB3	2263	1698	0.11%	0.011%
49	28.893	4323	4324	4326	rBV2	2164	1869	0.12%	0.012%
50	29.627	4441	4449	4463	rVB6	13280	53936	3.49%	0.336%
51	30.391	4577	4579	4582	rVB3	2005	1735	0.11%	0.011%
52	30.703	4630	4632	4635	rVB4	2482	1793	0.12%	0.011%
53	31.155	4707	4709	4711	rBV3	2103	2229	0.14%	0.014%
54	32.013	4851	4855	4857	rBV5	2130	3195	0.21%	0.020%
55	32.459	4930	4931	4934	rBV3	2770	1904	0.12%	0.012%




Sum of corrected areas: 16044765

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111121\
Data File : BG050992.D
Acq On : 12 Nov 2021 8:50
Operator : CG/JU
Sample : PB140665BL
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK665

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110321.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

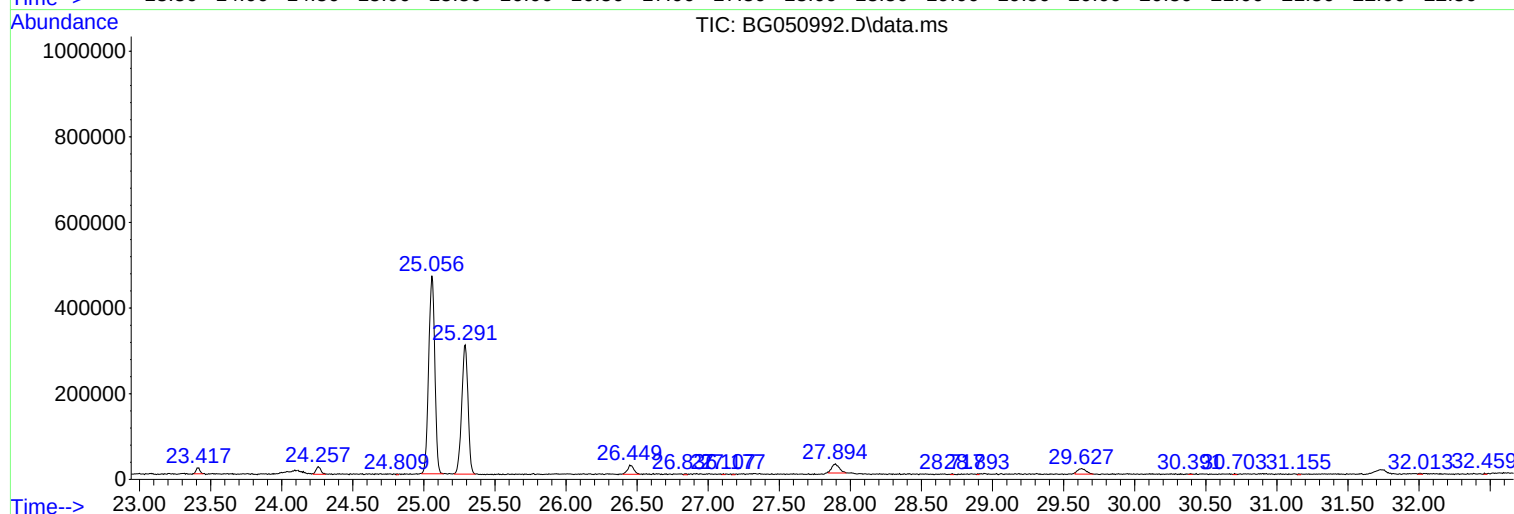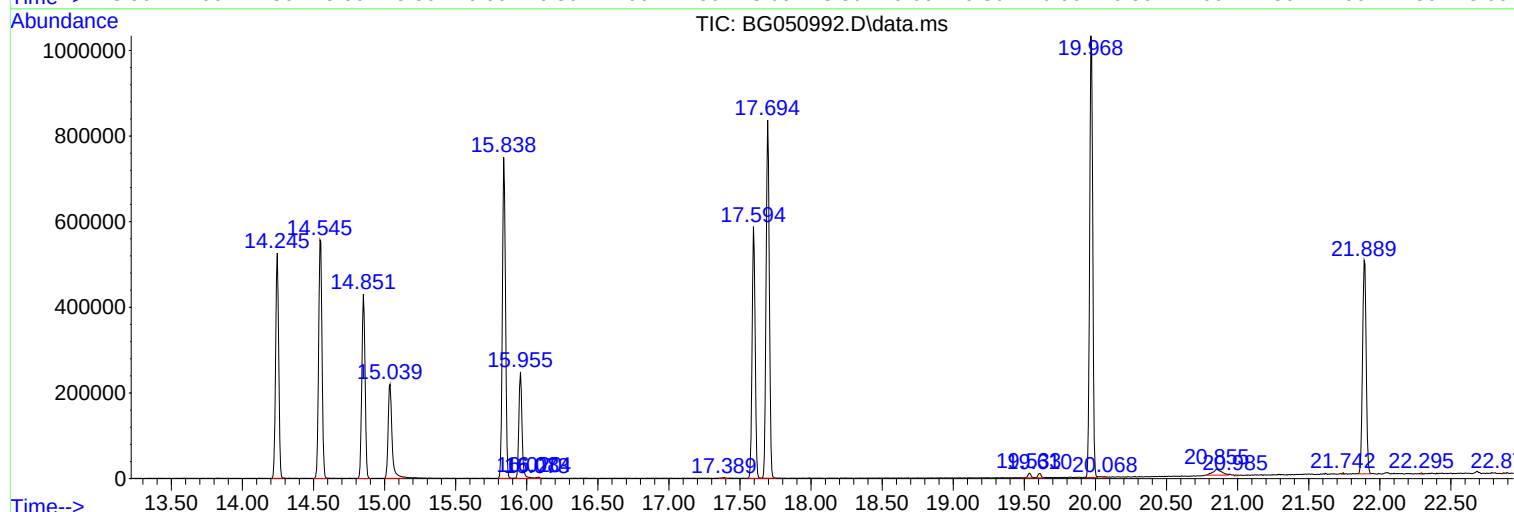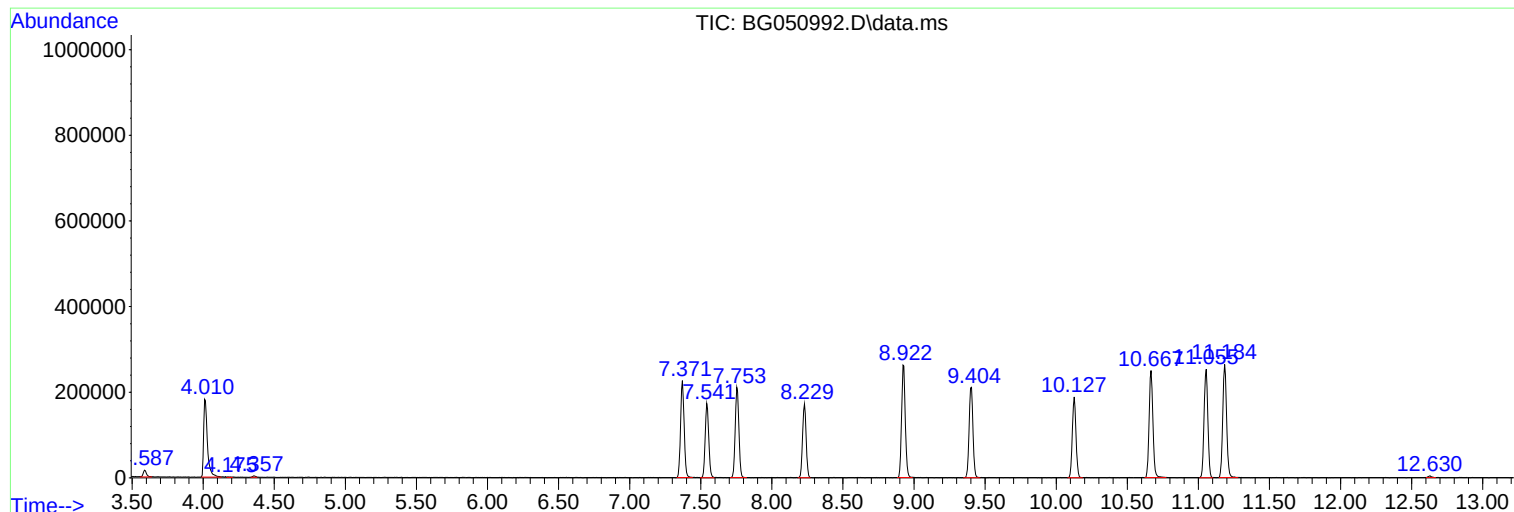

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111121\
Data File : BG050992.D
Acq On : 12 Nov 2021 8:50
Operator : CG/JU
Sample : PB140665BL
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK665

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110321.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111121\
Data File : BG050992.D
Acq On : 12 Nov 2021 8:50
Operator : CG/JU
Sample : PB140665BL
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK665

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110321.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc