
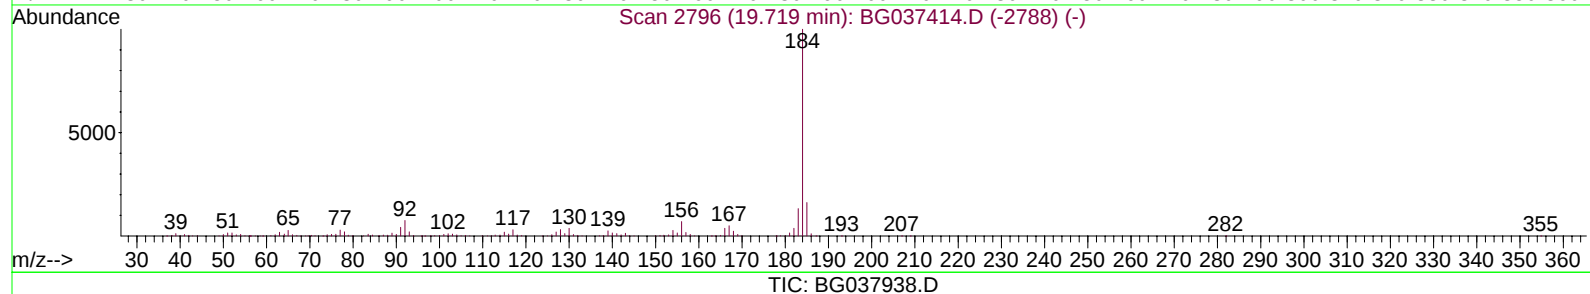
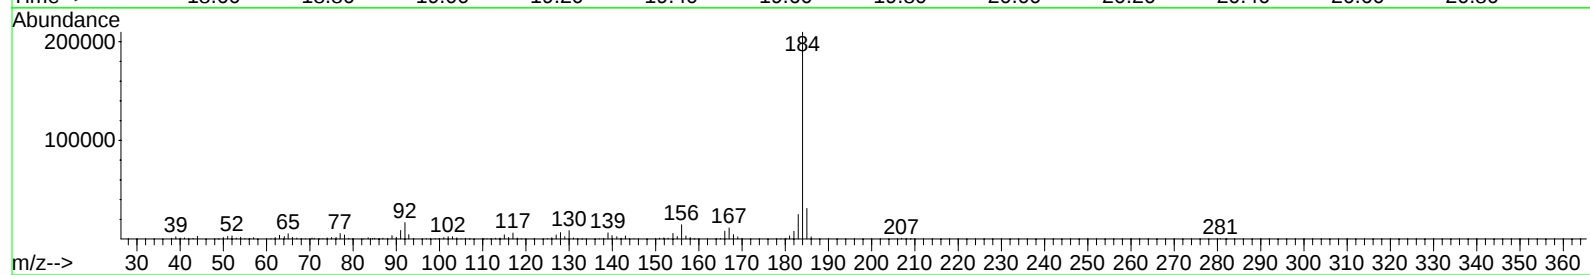


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG111218\
Data File : BG037938.D
Acq On : 12 Nov 2018 10:40
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 12 18:08:26 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG101818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 18 14:06:42 2018
Response via : Initial Calibration

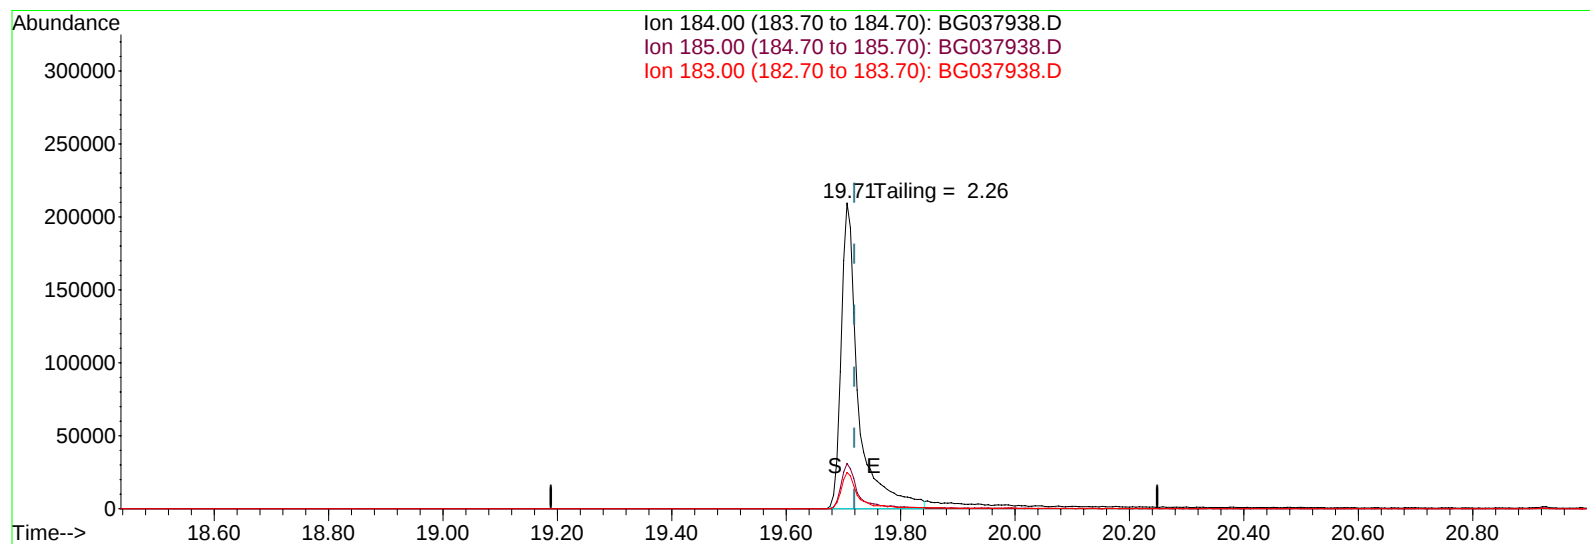

(77) Benzidine




19.706min (-0.013) 236494.53ng

response 450320

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.83
183.00	12.70	11.89
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG111218\
Data File : BG037938.D
Acq On : 12 Nov 2018 10:40
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 12 18:08:26 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG101818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 18 14:06:42 2018
Response via : Initial Calibration

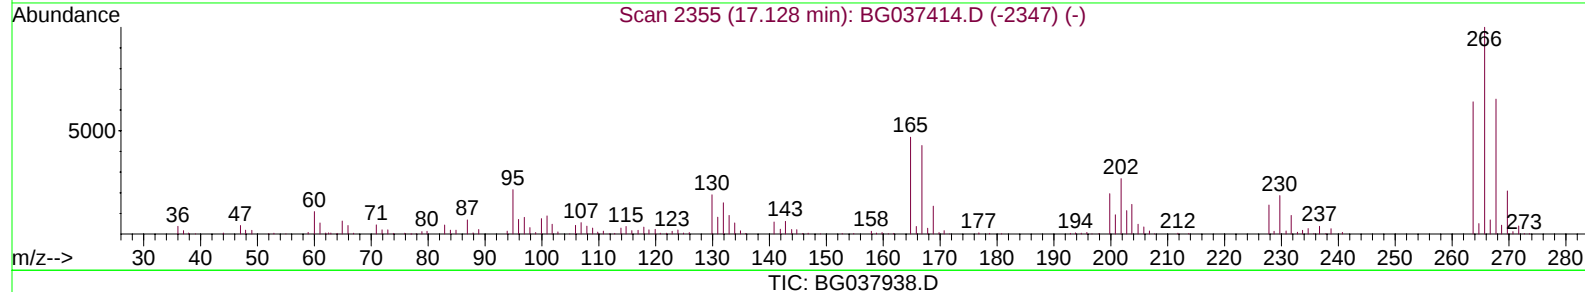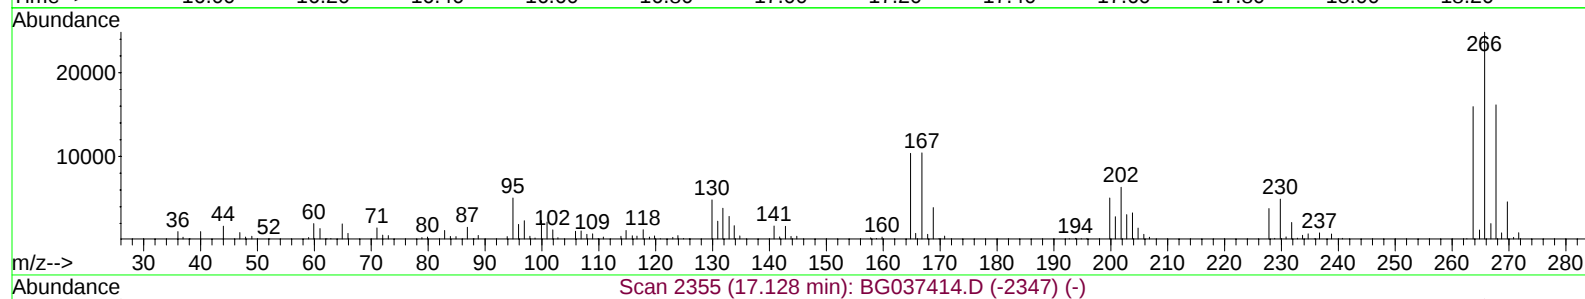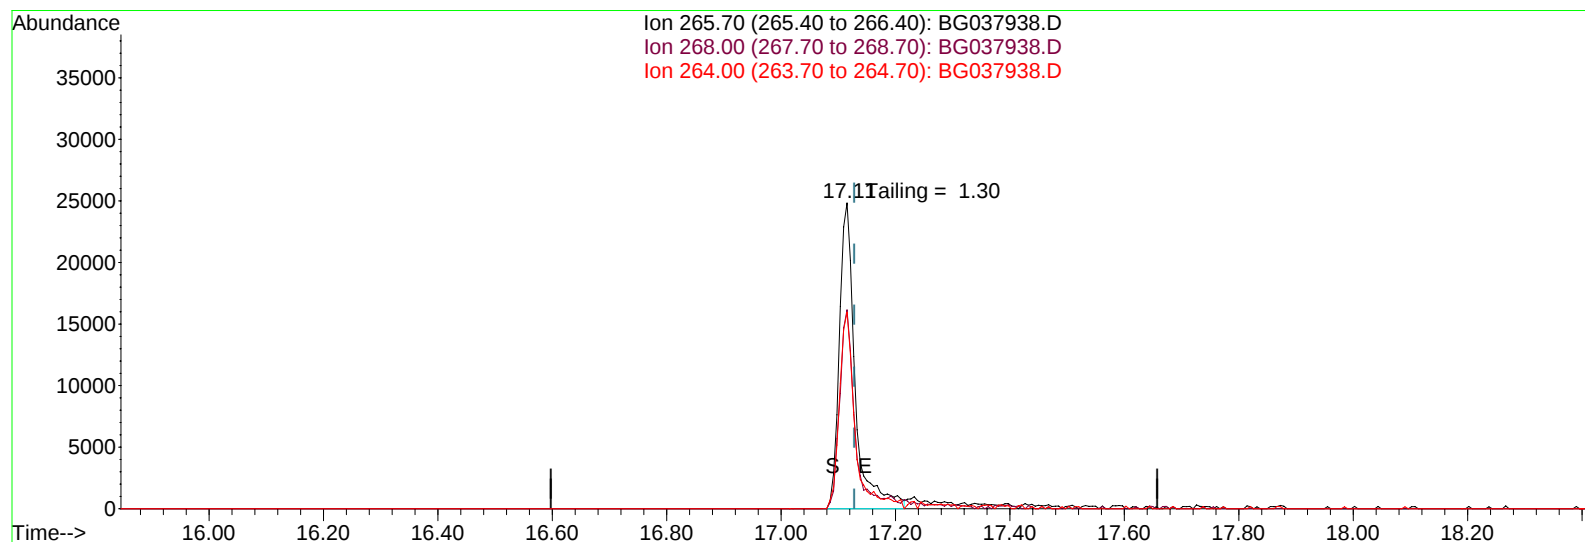

(70) Pentachlorophenol (C)

17.115min (-0.013) 15506.37ng

response 48232

Ion	Exp%	Act%
265.70	100	100
268.00	68.80	68.56
264.00	73.60	64.25
0.00	0.00	0.00