


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111218\
 Data File : BG037938.D
 Acq On : 12 Nov 2018 10:40
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG101818.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Oct 18 14:06:42 2018

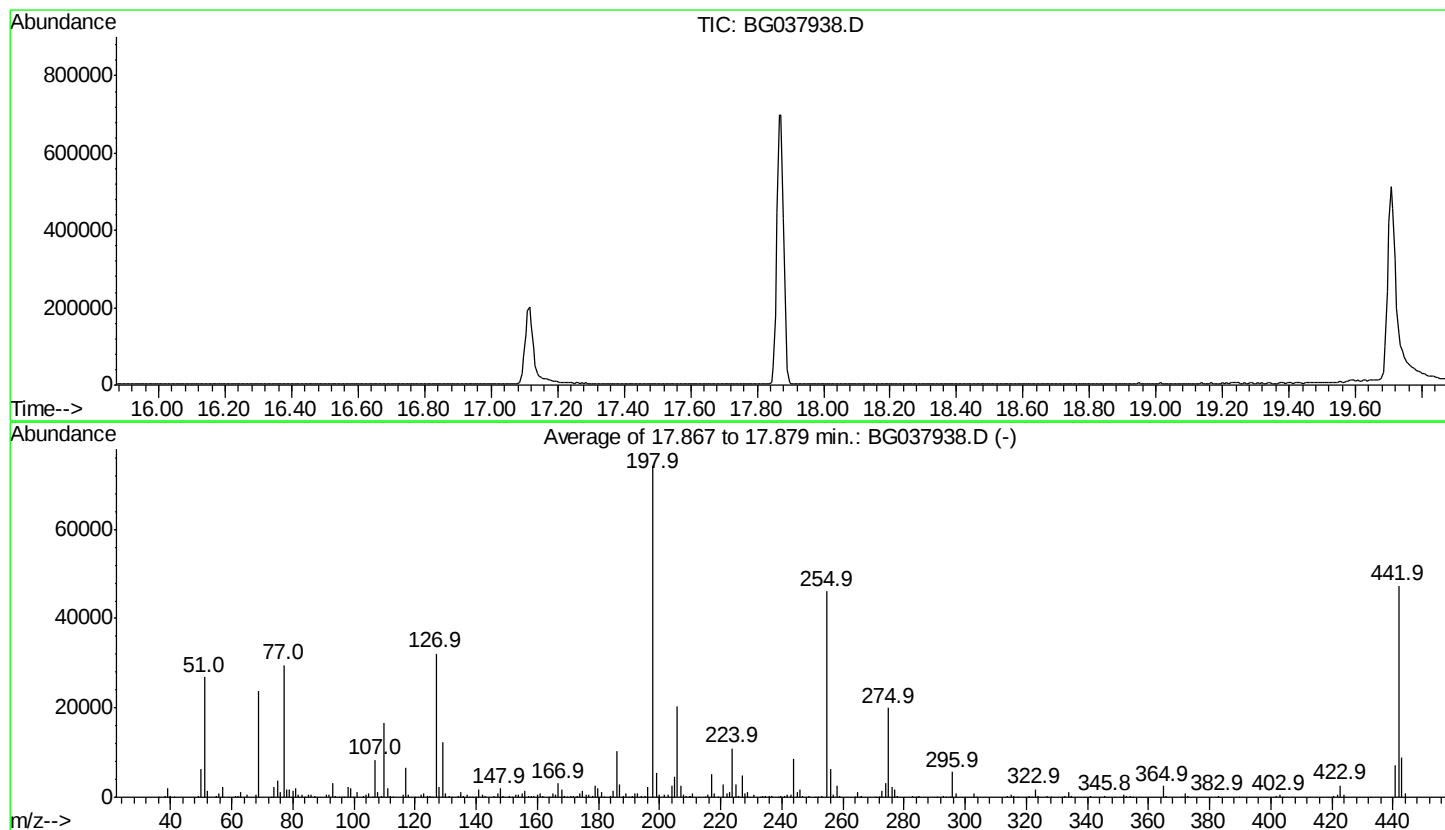

AutoFind: Scans 2481, 2482, 2483; Background Corrected with Scan 2474

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.3	26917	PASS
68	69	0.00	2	1.9	442	PASS
69	198	0.00	100	32.2	23882	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	43.3	32170	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	74242	PASS
199	198	5	9	7.2	5379	PASS
275	198	10	60	26.9	19952	PASS
365	198	1	100	3.5	2567	PASS
441	198	0.01	100	9.7	7166	PASS
442	198	50	100	63.7	47301	PASS
443	442	15	24	18.5	8759	PASS