

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG111220\
 Data File : BG047312.D
 Acq On : 12 Nov 2020 18:38
 Operator : CG/JU
 Sample : PB132980BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK80

Quant Time: Nov 13 03:19:06 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG102220MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Nov 10 10:50:02 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.01	152	49534	20.00	ng/ul	0.00
18) Naphthalene-d8	10.82	136	195098	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.65	164	138709	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.39	188	315281	20.00	ng/ul	0.00
78) Chrysene-d12	21.65	240	293944	20.00	ng/ul	0.00
86) Perylene-d12	24.86	264	197085	20.00	ng/ul	0.02

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.40	96	6646	5.41	ng/uL	0.00
5) Phenol-d5	7.17	99	141139	32.83	ng/ul	0.01
7) Bis-(2-Chloroethyl)ether-d	7.33	67	82954	33.55	ng/ul	0.00
9) 2-Chlorophenol-d4	7.54	132	110677	33.11	ng/ul	0.00
13) 4-Methylphenol-d8	8.71	113	115607	33.70	ng/ul	0.00
19) Nitrobenzene-d5	9.17	128	55707	34.07	ng/ul	0.00
22) 2-Nitrophenol-d4	9.90	143	66865	35.00	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.44	165	123768	33.21	ng/ul	0.01
29) 4-Chloroaniline-d4	10.95	131	168288	52.95	ng/ul	0.01
44) Dimethylphthalate-d6	14.05	166	413920	36.29	ng/ul	0.01
47) Acenaphthylene-d8	14.34	160	469363	34.78	ng/ul	0.01
52) 4-Nitrophenol-d4	14.85	143	58372	32.51	ng/ul	0.02
58) Fluorene-d10	15.64	176	352315	33.27	ng/ul	0.01
63) 4,6-Dinitro-2-methylphenol	15.76	200	73425	33.77	ng/ul	0.01
71) Anthracene-d10	17.49	188	561474	36.74	ng/ul	0.00
79) Pyrene-d10	19.78	212	614180	36.63	ng/ul	0.01
90) Benzo(a)pyrene-d12	24.64	264	403526	37.24	ng/ul	0.02


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
15) N-Nitroso-di-n-propylamine	8.71	70	3237	1.142	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG111220\
Data File : BG047312.D
Acq On : 12 Nov 2020 18:38
Operator : CG/JU
Sample : PB132980BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK80

Quant Time: Nov 13 03:19:06 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG102220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Nov 10 10:50:02 2020
Response via : Initial Calibration

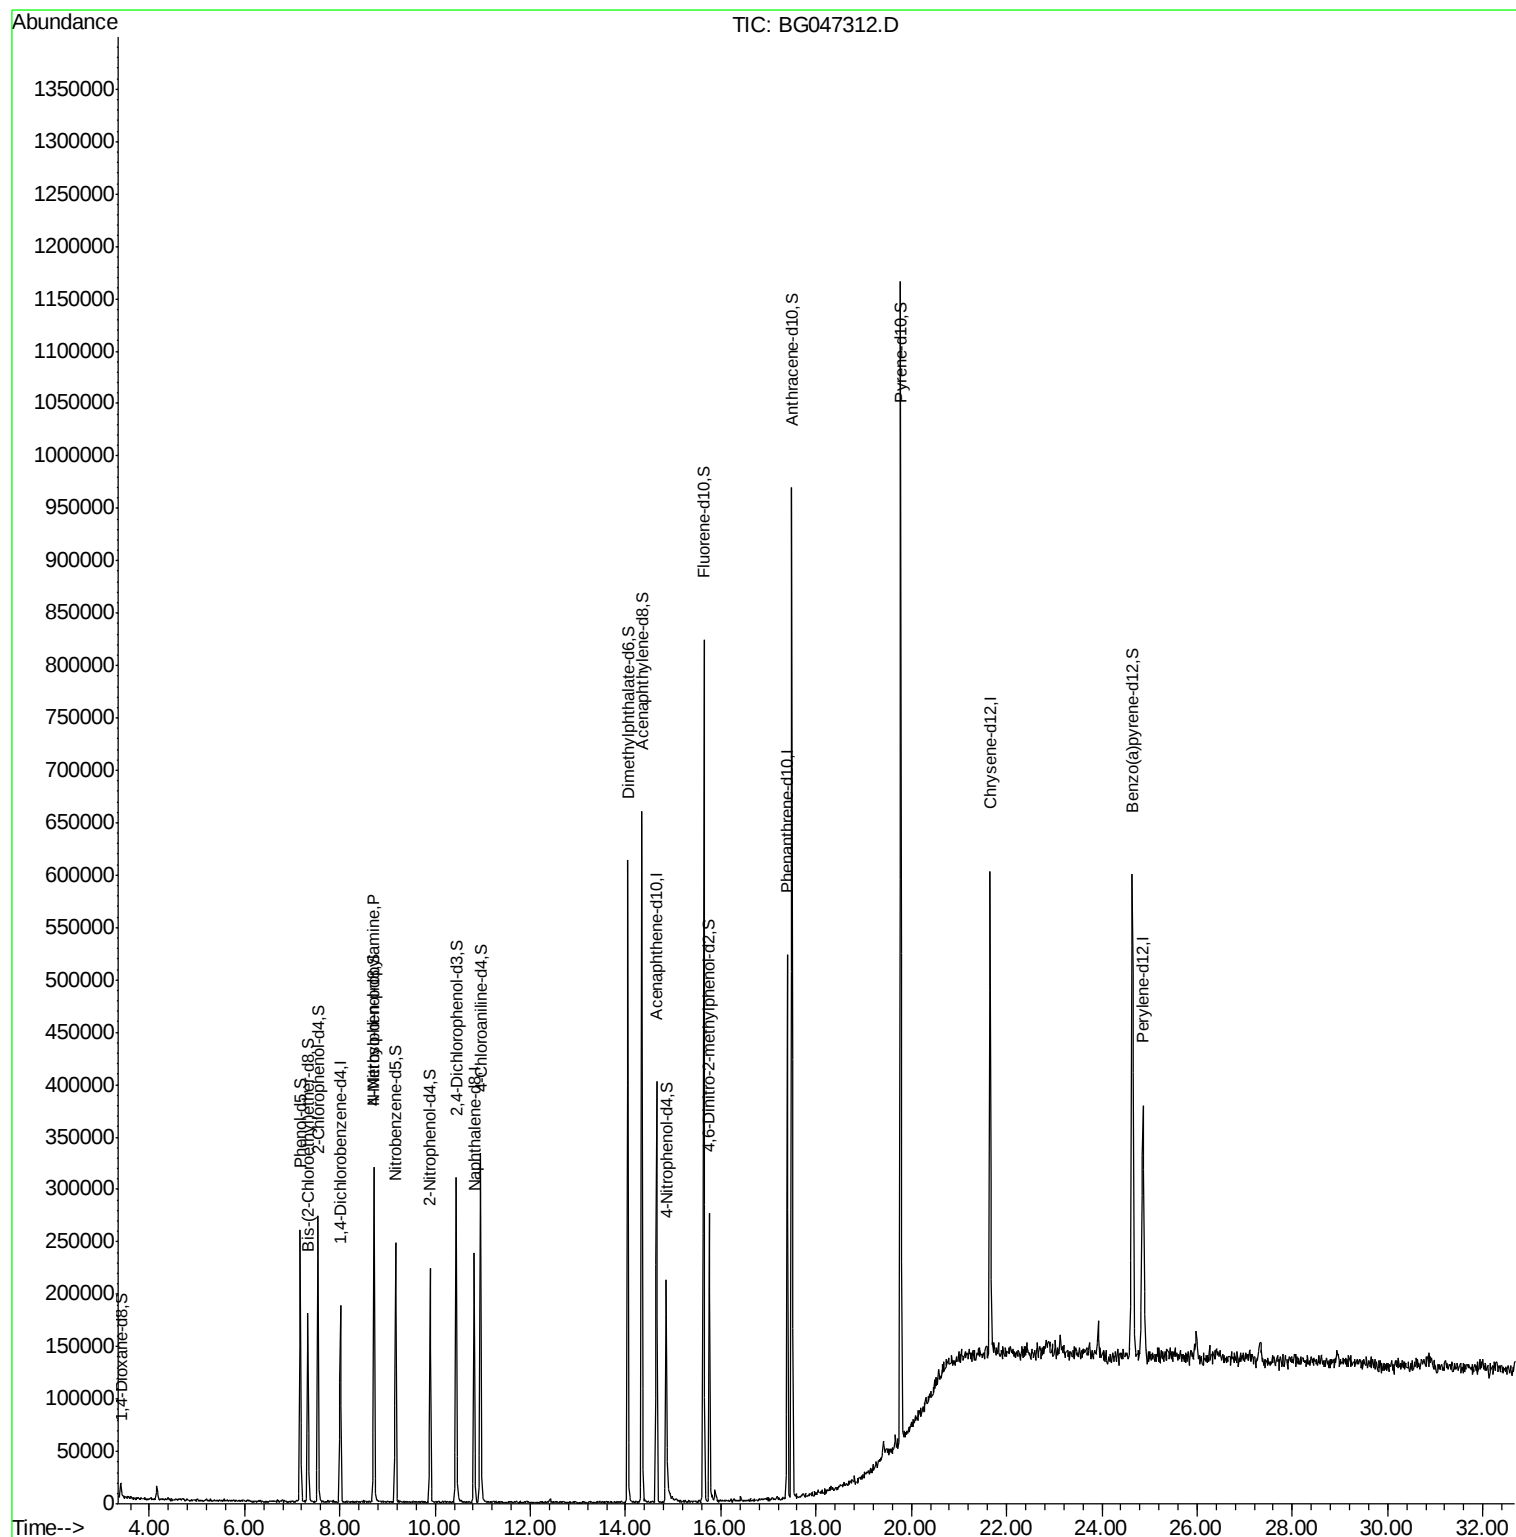

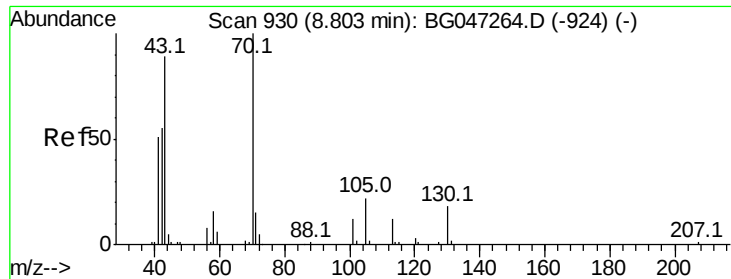

#15
 N-Nitroso-di-n-propylamine
 Concen: 1.142 ng/ul
 RT: 8.71 min Scan# 914
 Delta R.T. -0.09 min
 Lab File: BG047312.D
 Acq: 12 Nov 2020 18:38

Instrument :
 BNA_G
 ClientSampleId :
 SBLK80

Tot Ion: 70 Resp: 3237
 Ion Ratio Lower Upper
 70 100
 42 316.5 45.3 67.9#
 101 0.0 9.5 14.3#
 130 0.0 14.6 22.0#

