

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG111220\
 Data File : BG047315.D
 Acq On : 12 Nov 2020 20:39
 Operator : CG/JU
 Sample : L4726-07
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DBGf1

Quant Time: Nov 13 03:19:21 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG102220MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Nov 10 10:50:02 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.01	152	42138	20.00	ng/ul	0.00
18) Naphthalene-d8	10.82	136	162723	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.64	164	115555	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.39	188	273984	20.00	ng/ul	0.00
78) Chrysene-d12	21.65	240	280678	20.00	ng/ul	0.00
86) Perylene-d12	24.85	264	287008	20.00	ng/ul	0.01

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.40	96	4006	3.83	ng/uL	0.00
5) Phenol-d5	7.17	99	21924	5.99	ng/ul	0.01
7) Bis-(2-Chloroethyl)ether-d	7.33	67	64573	30.70	ng/ul	0.00
9) 2-Chlorophenol-d4	7.54	132	70936	24.94	ng/ul	0.00
13) 4-Methylphenol-d8	8.72	113	44353	15.20	ng/ul	0.00
19) Nitrobenzene-d5	9.17	128	45275	33.19	ng/ul	0.00
22) 2-Nitrophenol-d4	9.90	143	54287	34.07	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.44	165	87252	28.07	ng/ul	0.00
29) 4-Chloroaniline-d4	10.96	131	7686	2.90	ng/ul	0.02
44) Dimethylphthalate-d6	14.05	166	341880	35.98	ng/ul	0.00
47) Acenaphthylene-d8	14.34	160	403424	35.89	ng/ul	0.00
52) 4-Nitrophenol-d4	14.86	143	7790	5.21	ng/ul	0.03
58) Fluorene-d10	15.64	176	314771	35.68	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.76	200	72583	38.41	ng/ul	0.00
71) Anthracene-d10	17.49	188	578465	43.56	ng/ul	0.00
79) Pyrene-d10	19.77	212	709047	44.29	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.63	264	676536	42.88	ng/ul	0.01


Target Compounds				Ovalue	
45) Dimethylphthalate	14.09	163	30062	3.153	ng/ul# 91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG111220\
Data File : BG047315.D
Acq On : 12 Nov 2020 20:39
Operator : CG/JU
Sample : L4726-07
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DBGF1

Quant Time: Nov 13 03:19:21 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG102220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Nov 10 10:50:02 2020
Response via : Initial Calibration

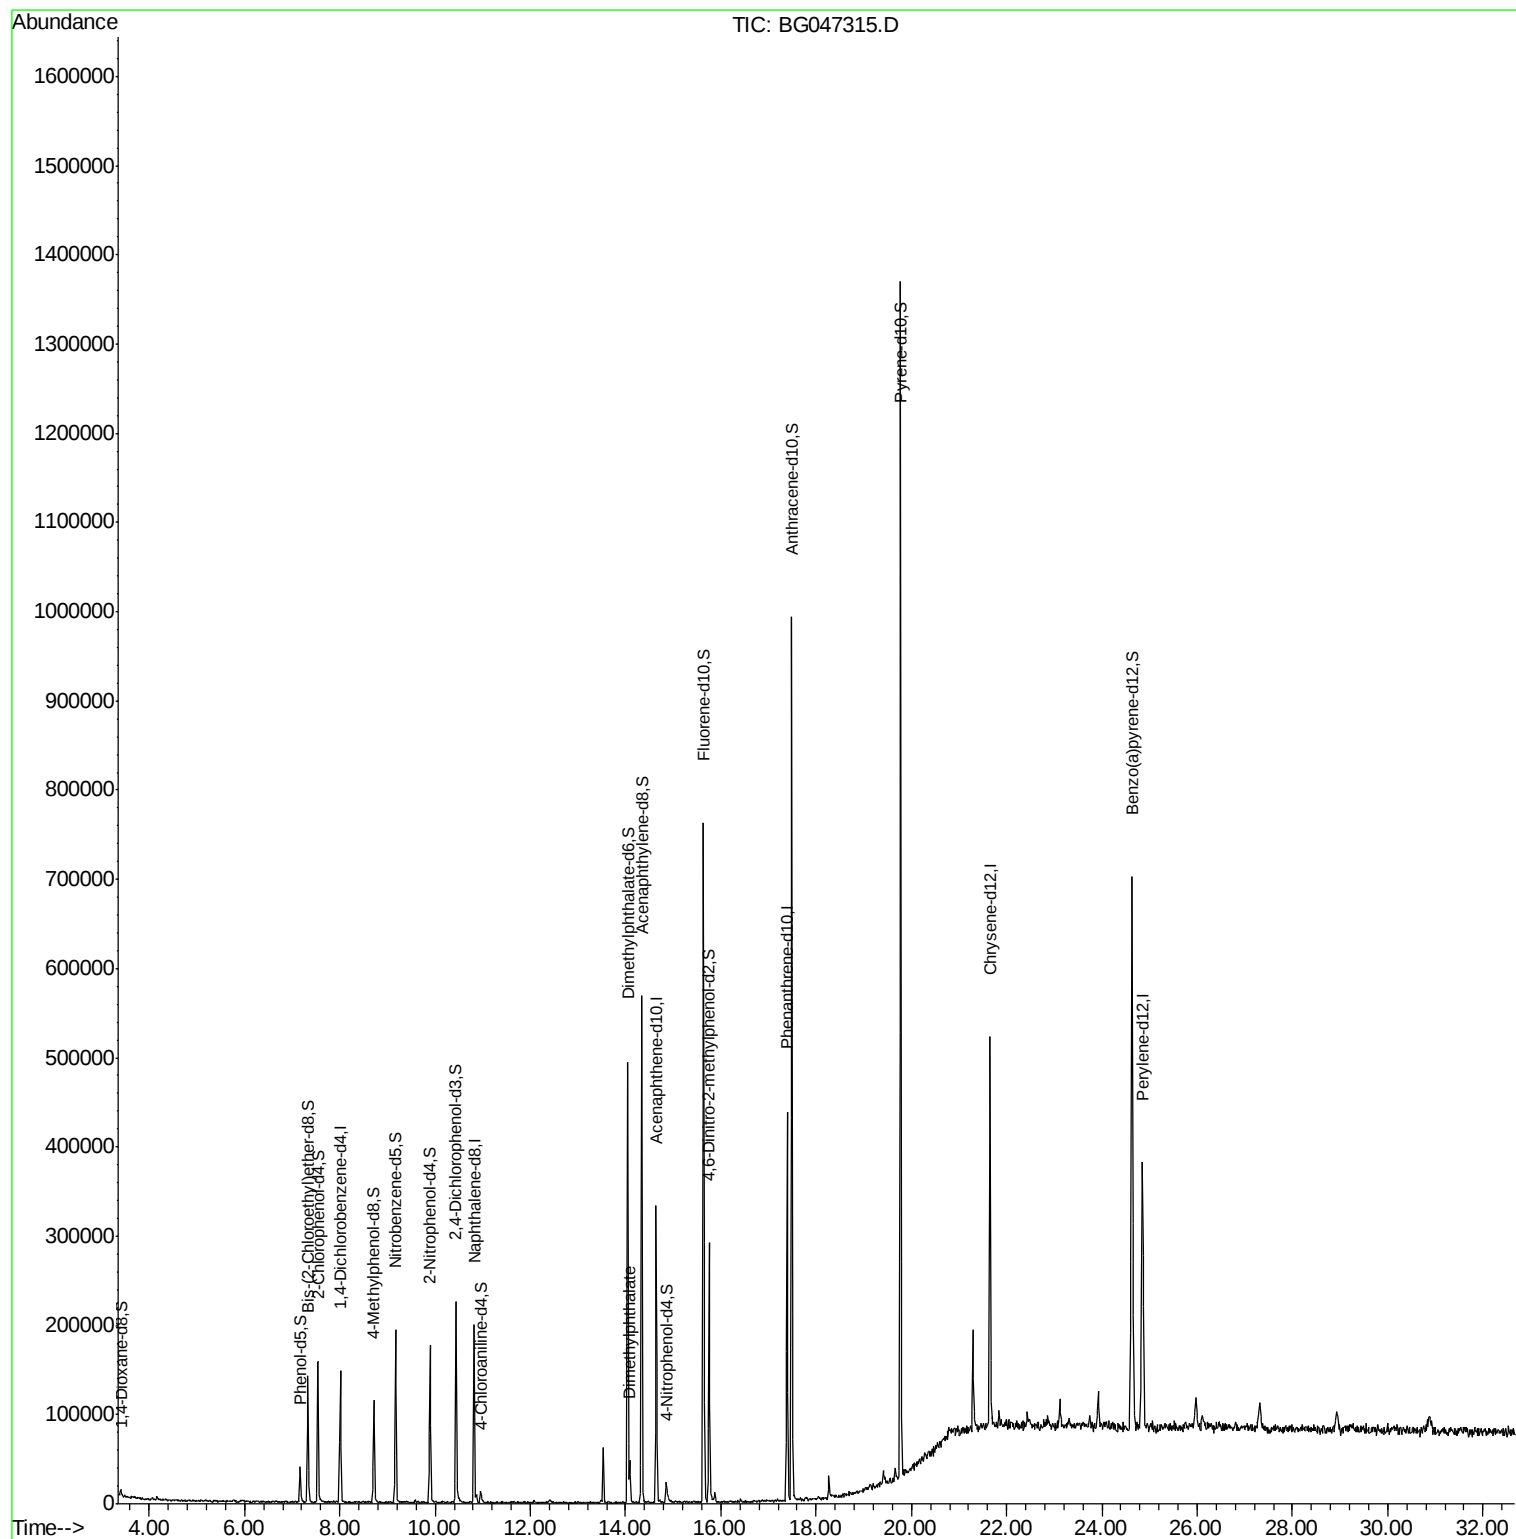

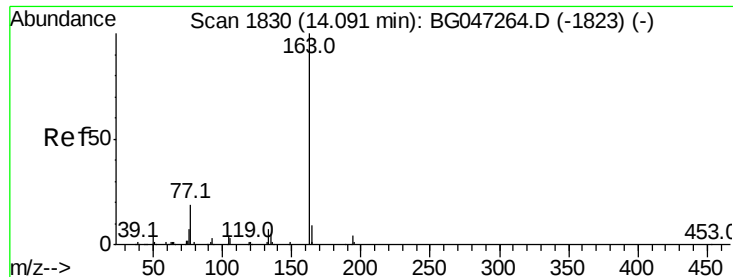

#45

Dimethylphthalate

Concen: 3.153 ng/ul

RT: 14.09 min Scan# 1830

Delta R.T. 0.00 min

Lab File: BG047315.D

Acq: 12 Nov 2020 20:39

Instrument :

BNA_G

ClientSampleId :

DBGF1

Tot Ion:163 Resp: 30062

Ion Ratio Lower Upper

163 100

194 5.5 3.4 5.0#

164 13.0 7.2 10.8#

