

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG111220\
 Data File : BG047318.D
 Acq On : 12 Nov 2020 22:40
 Operator : CG/JU
 Sample : L4726-03
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DBGE7

Quant Time: Nov 13 03:19:39 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG102220MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Nov 10 10:50:02 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.01	152	40433	20.00	ng/ul	0.00
18) Naphthalene-d8	10.82	136	160914	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.64	164	118346	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.39	188	303383	20.00	ng/ul	0.00
78) Chrysene-d12	21.65	240	300538	20.00	ng/ul	0.00
86) Perylene-d12	24.84	264	296502	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.40	96	4405	4.39	ng/uL	0.00
5) Phenol-d5	7.17	99	24221	6.90	ng/ul	0.01
7) Bis-(2-Chloroethyl)ether-d	7.33	67	67433	33.41	ng/ul	0.00
9) 2-Chlorophenol-d4	7.53	132	74400	27.26	ng/ul	0.00
13) 4-Methylphenol-d8	8.71	113	45127	16.12	ng/ul	0.00
19) Nitrobenzene-d5	9.17	128	44076	32.68	ng/ul	0.00
22) 2-Nitrophenol-d4	9.89	143	54358	34.50	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.44	165	91147	29.65	ng/ul	0.00
29) 4-Chloroaniline-d4	10.95	131	9920	3.78	ng/ul	0.00
44) Dimethylphthalate-d6	14.04	166	362170	37.22	ng/ul	0.00
47) Acenaphthylene-d8	14.34	160	414326	35.99	ng/ul	0.00
52) 4-Nitrophenol-d4	14.85	143	12545	8.19	ng/ul	0.02
58) Fluorene-d10	15.64	176	336997	37.30	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.75	200	81019	38.72	ng/ul	0.00
71) Anthracene-d10	17.49	188	622737	42.35	ng/ul	0.00
79) Pyrene-d10	19.77	212	752684	43.91	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.63	264	697718	42.80	ng/ul	0.01


Target Compounds				Ovalue	
45) Dimethylphthalate	14.09	163	58536	5.994	ng/ul# 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG111220\
Data File : BG047318.D
Acq On : 12 Nov 2020 22:40
Operator : CG/JU
Sample : L4726-03
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DBGE7

Quant Time: Nov 13 03:19:39 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG102220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Nov 10 10:50:02 2020
Response via : Initial Calibration

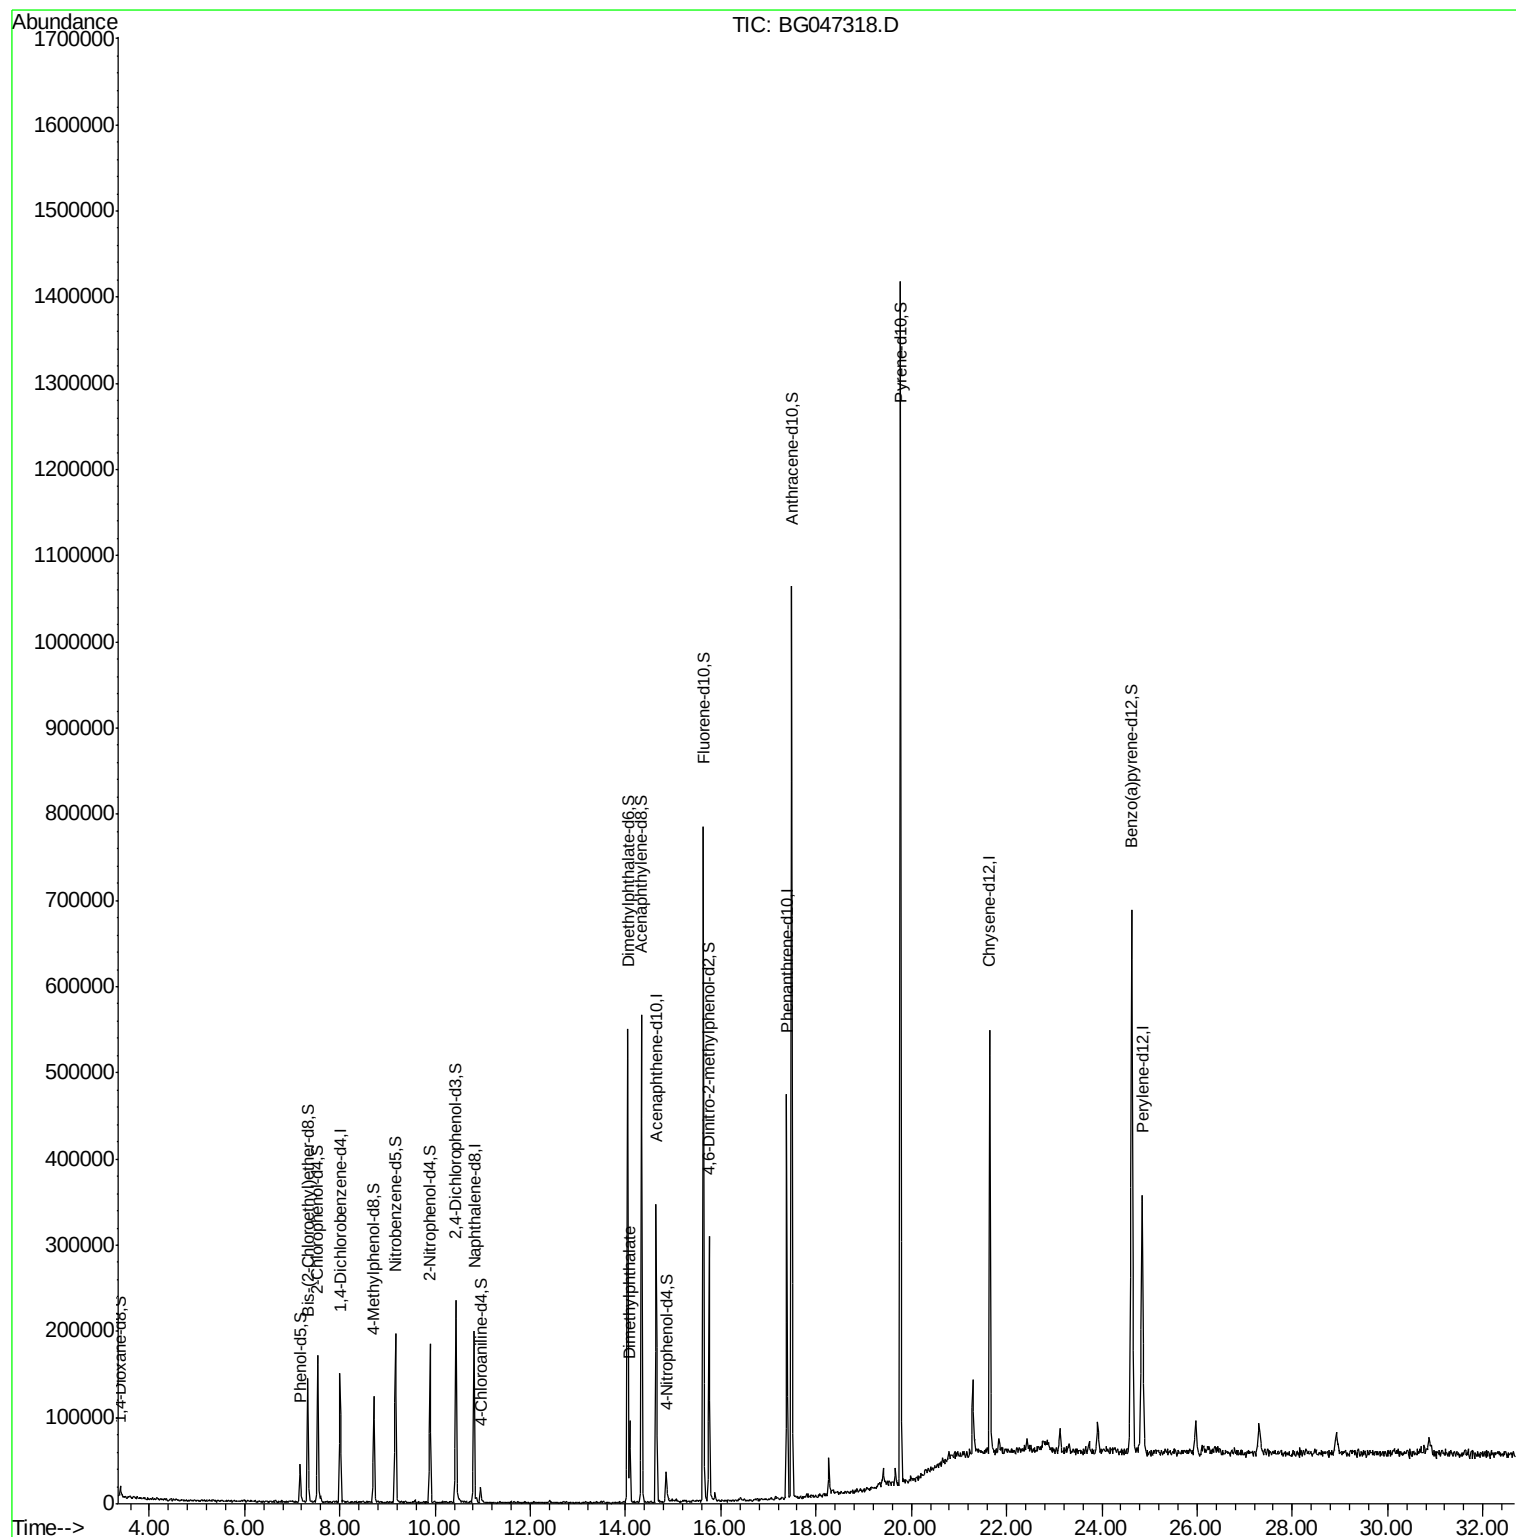

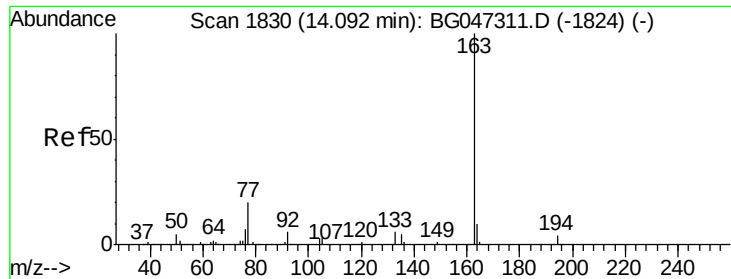

#45

Dimethylphthalate

Concen: 5.994 ng/ul

RT: 14.09 min Scan# 1830

Delta R.T. -0.00 min

Lab File: BG047318.D

Acq: 12 Nov 2020 22:40

Instrument :

BNA_G

ClientSampleId :

DBGE7


Tot Ion:163 Resp: 58536

Ion Ratio Lower Upper

163 100

194 5.2 3.4 5.0#

164 10.5 7.2 10.8

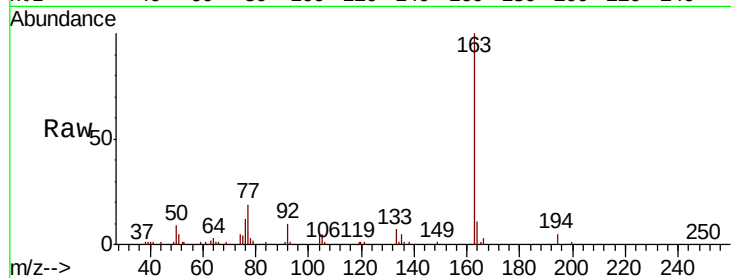

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

