
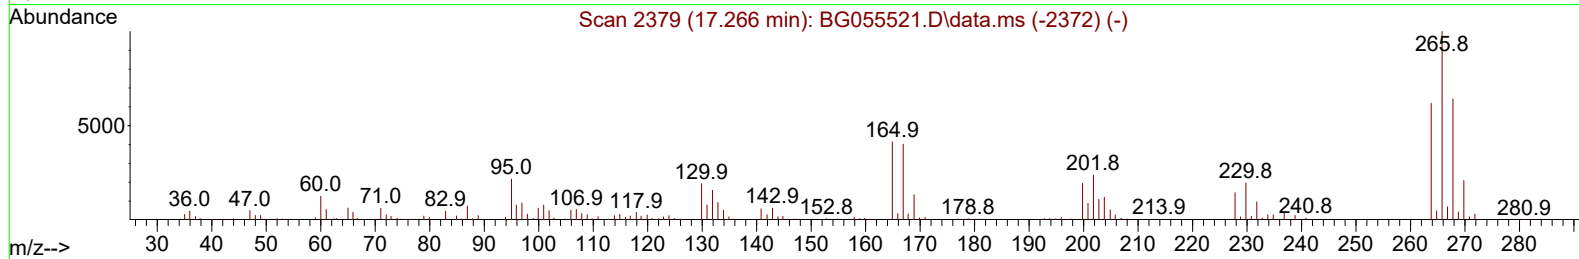
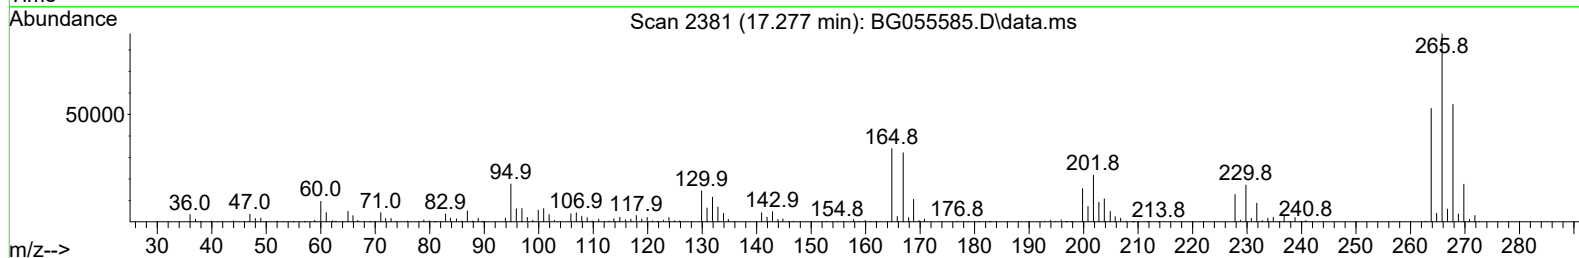


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111222\
Data File : BG055585.D
Acq On : 12 Nov 2022 10:48
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 14 08:23:15 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG110922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 10 03:39:46 2022
Response via : Initial Calibration

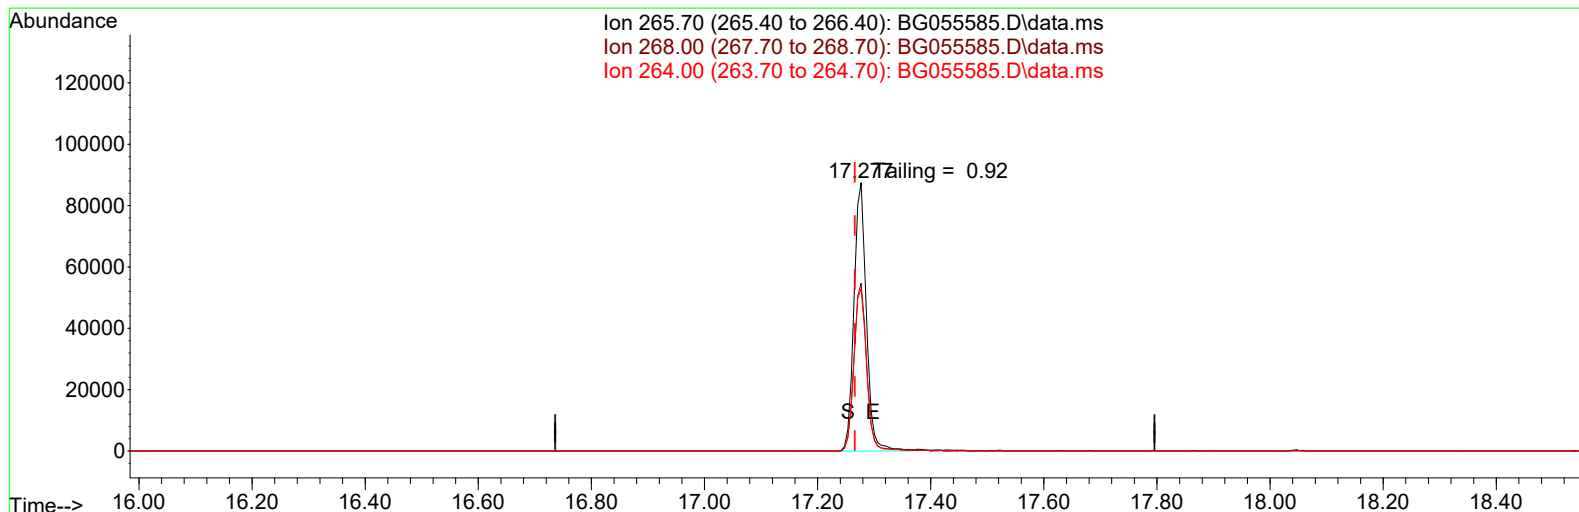

TIC: BG055585.D\data.ms

(70) Pentachlorophenol (C)




17.277min (+ 0.011) 24769.90 ng

response 133479

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.20	62.46
264.00	61.90	60.36
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111222\
Data File : BG055585.D
Acq On : 12 Nov 2022 10:48
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 14 08:23:15 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG110922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 10 03:39:46 2022
Response via : Initial Calibration

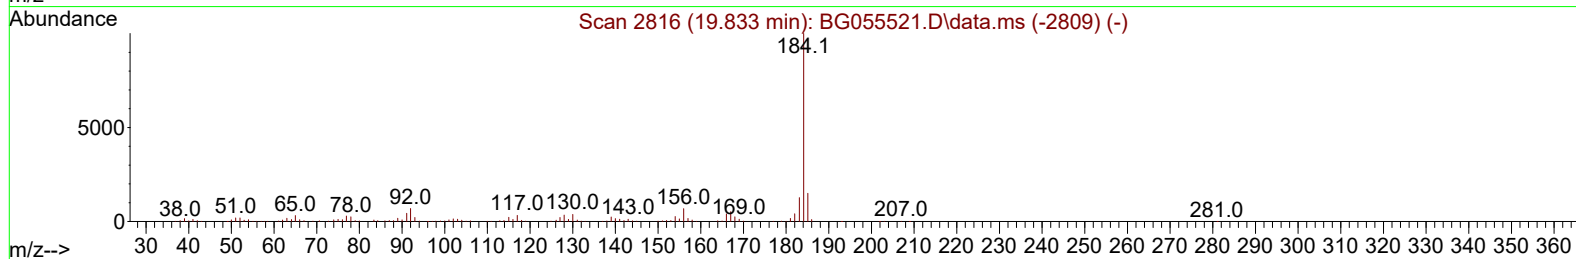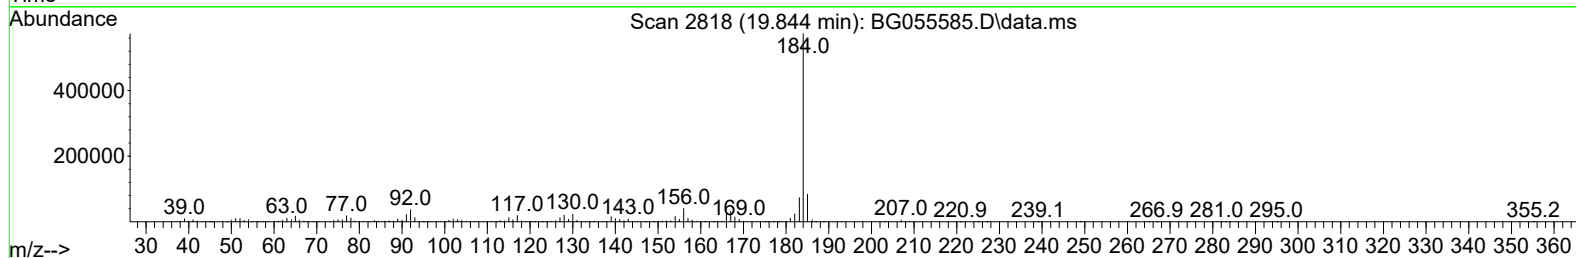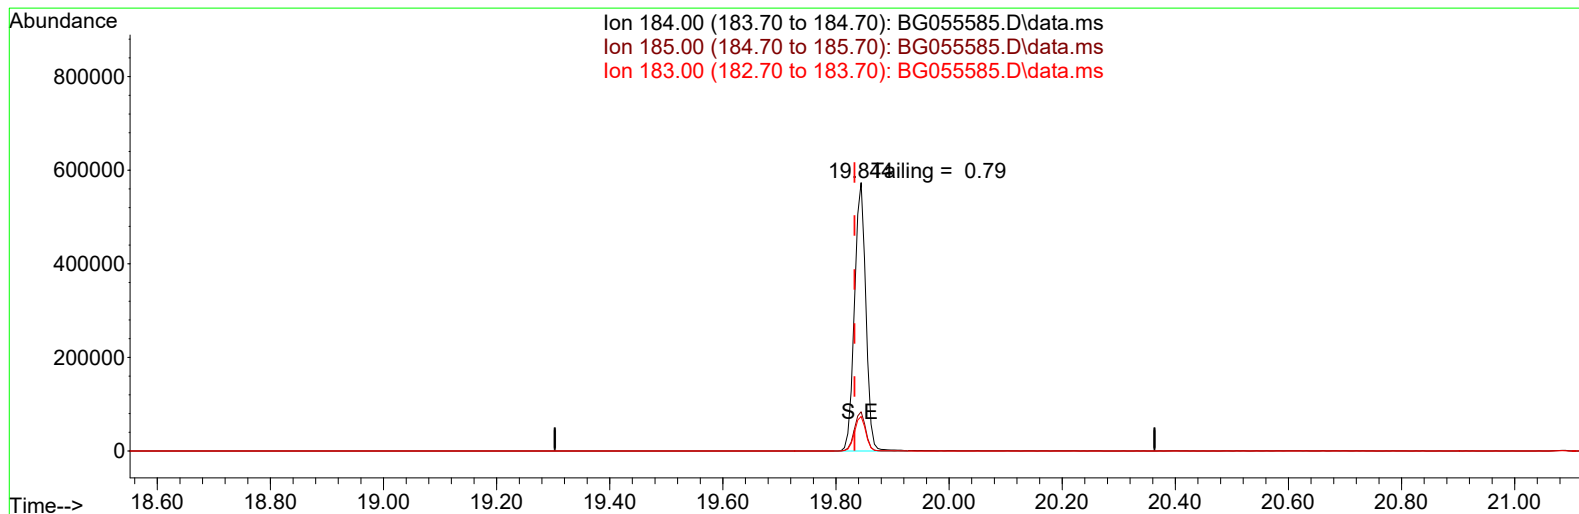

TIC: BG055585.D\data.ms

(77) Benzidine**19.844min (+ 0.011) 432024.50 ng****response 806473**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	14.64
183.00	12.70	12.89
0.00	0.00	0.00