


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111222\
 Data File : BG055585.D
 Acq On : 12 Nov 2022 10:48
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG110922.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Nov 10 03:39:46 2022

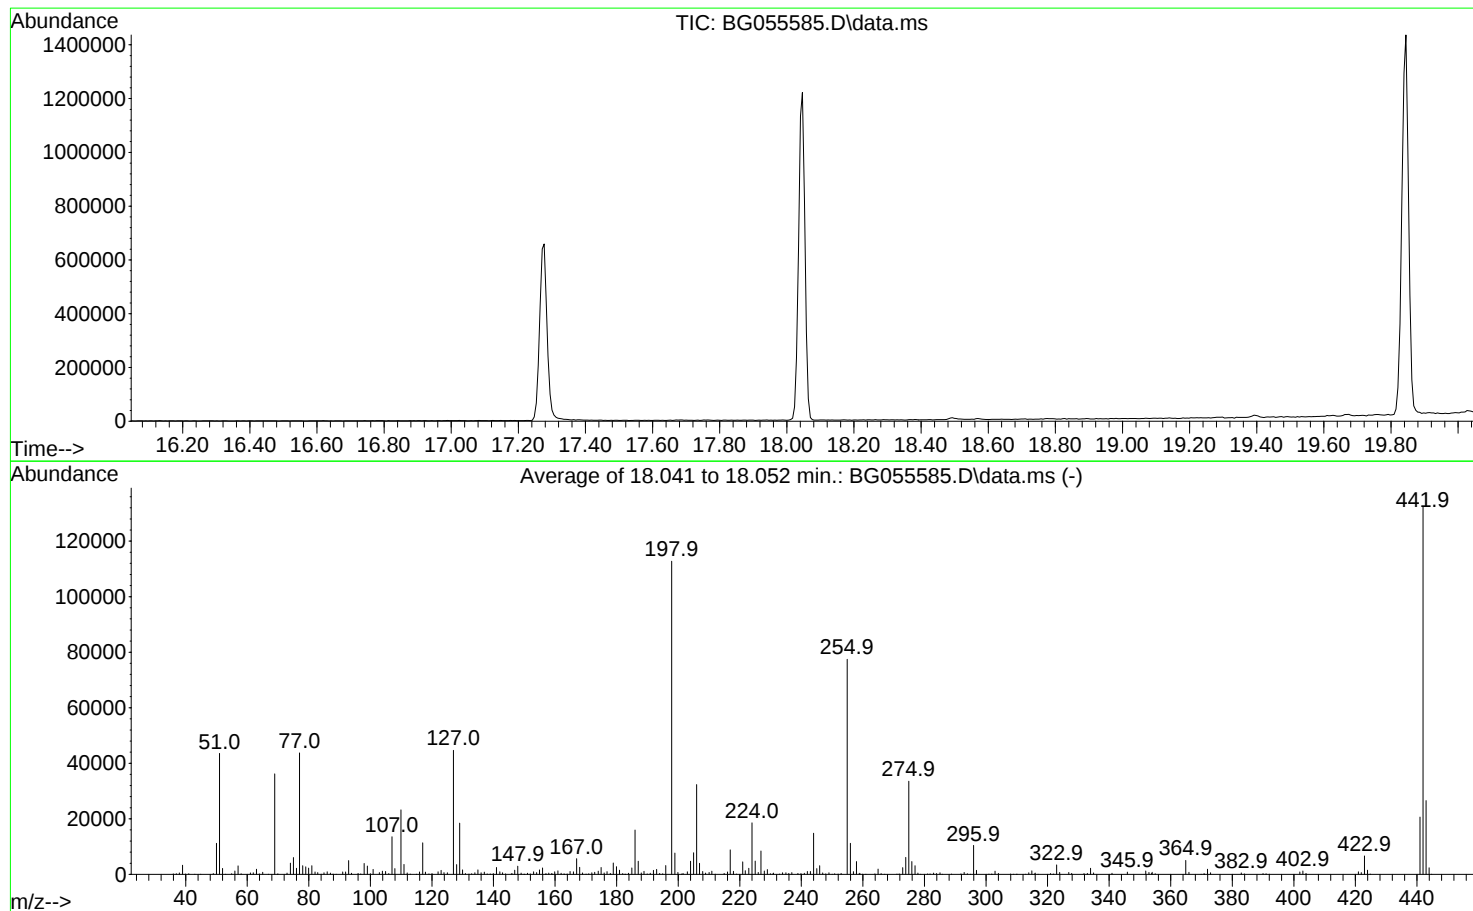




AutoFind: Scans 2511, 2512, 2513; Background Corrected with Scan 2504

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.6	43541	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	32.1	36213	PASS
70	69	0.00	2	0.5	186	PASS
127	198	10	80	39.6	44661	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	112781	PASS
199	198	5	9	6.8	7662	PASS
275	198	10	60	29.8	33555	PASS
365	198	1	100	4.5	5045	PASS
441	198	0.01	100	18.3	20624	PASS
442	442	50	100	100.0	132472	PASS
443	442	15	24	20.1	26568	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111222\
Data File : BG055585.D
Acq On : 12 Nov 2022 10:48
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Nov 14 08:23:15 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG110922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 10 03:39:46 2022
Response via : Initial Calibration

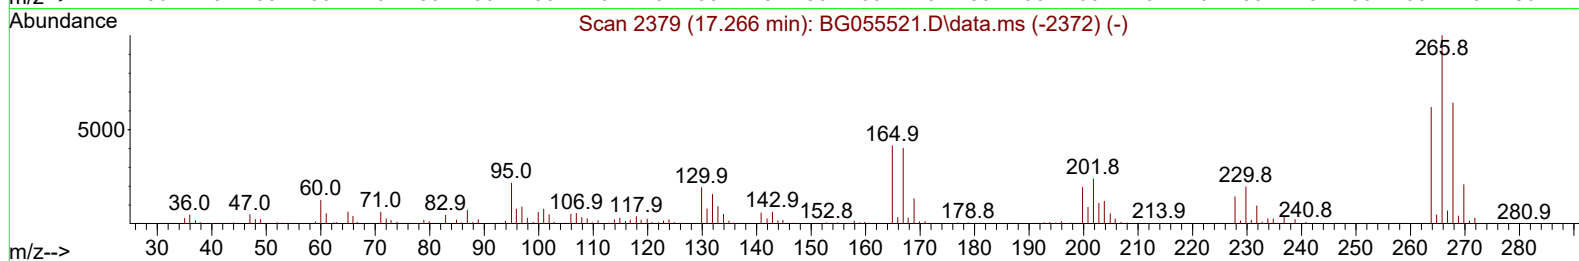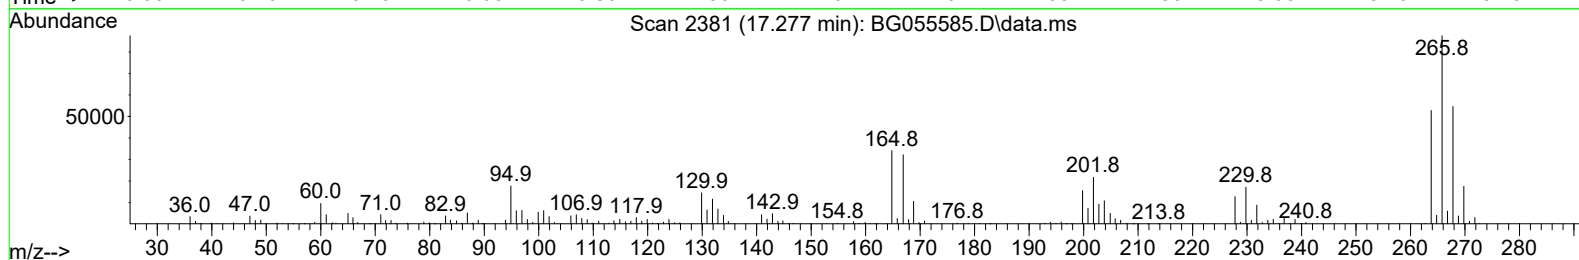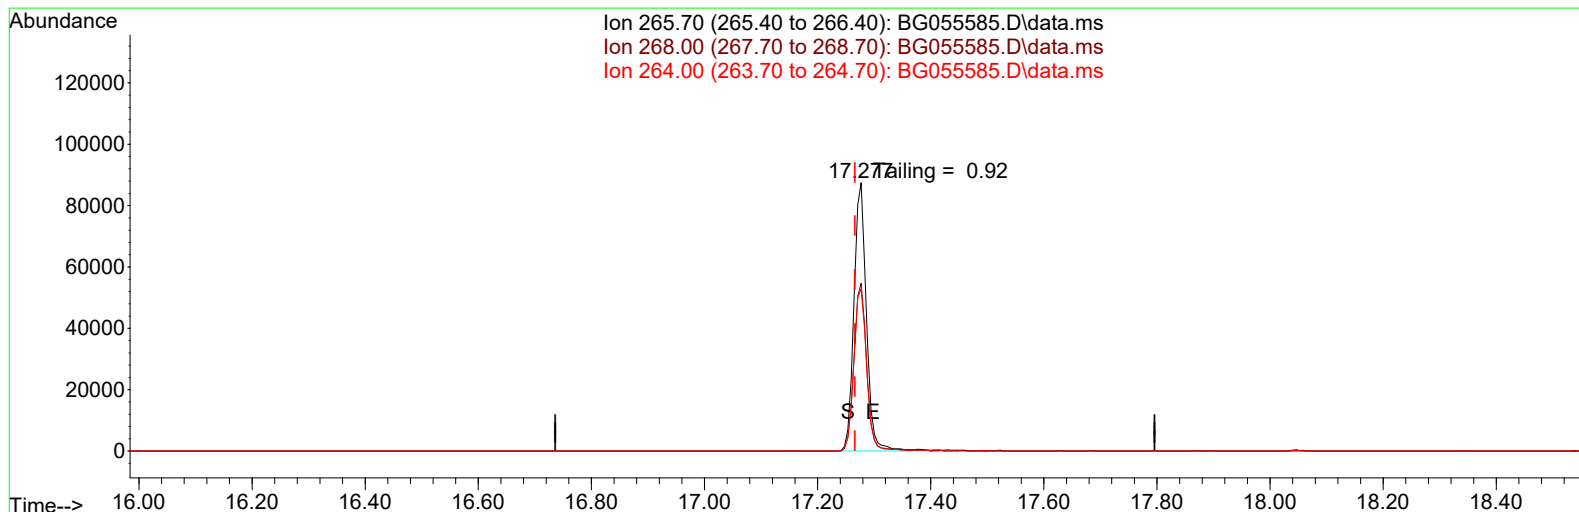

TIC: BG055585.D\data.ms

(70) Pentachlorophenol (C)

17.277min (+ 0.011) 24769.90 ng




response 133479

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.20	62.46
264.00	61.90	60.36
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111222\
Data File : BG055585.D
Acq On : 12 Nov 2022 10:48
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Nov 14 08:23:15 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG110922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 10 03:39:46 2022
Response via : Initial Calibration

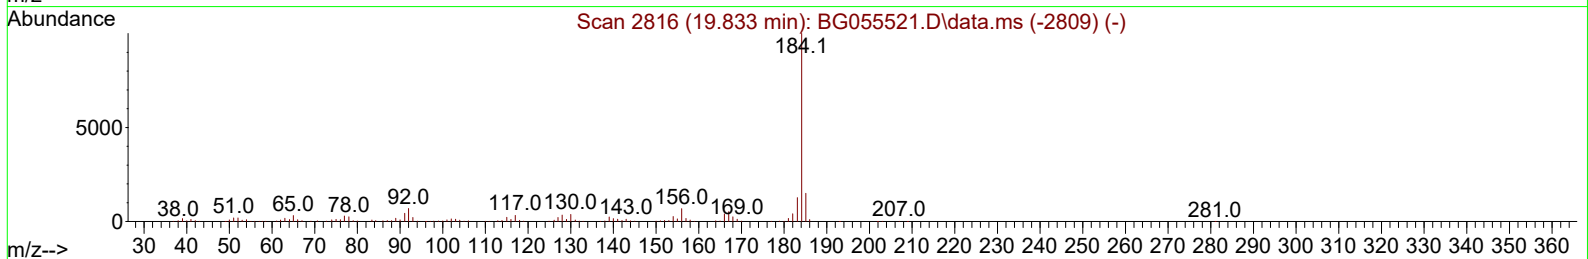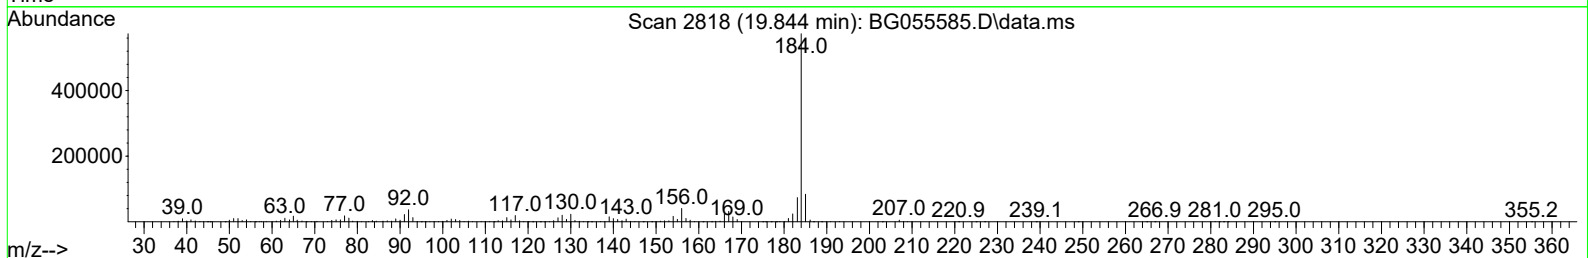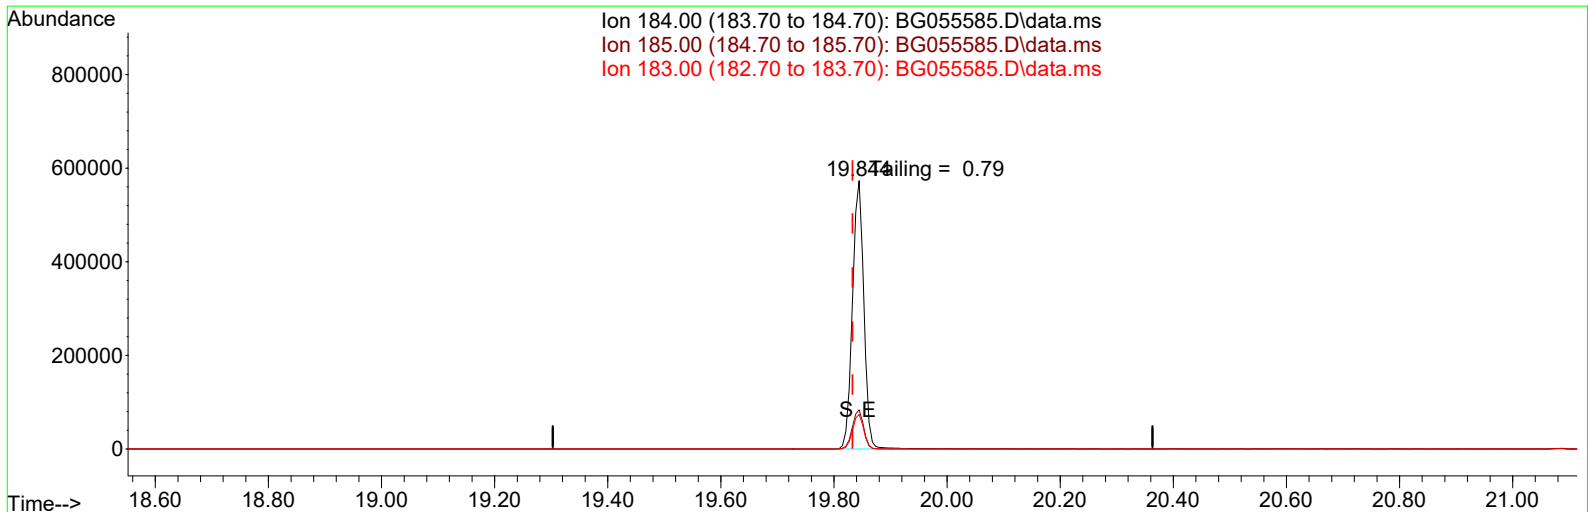

TIC: BG055585.D\data.ms

(77) Benzidine

19.844min (+ 0.011) 432024.50 ng

response 806473

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	14.64
183.00	12.70	12.89
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/12/2022	BNA_G	BG055585.D
Compound Name	Response	Retention Time
DDT	339716	21.084
DDD	12350	20.626
DDE	668	20.121
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
13018	352734	3.69

Instrument :
BNA_G
ClientSampleId :
DFTPP