
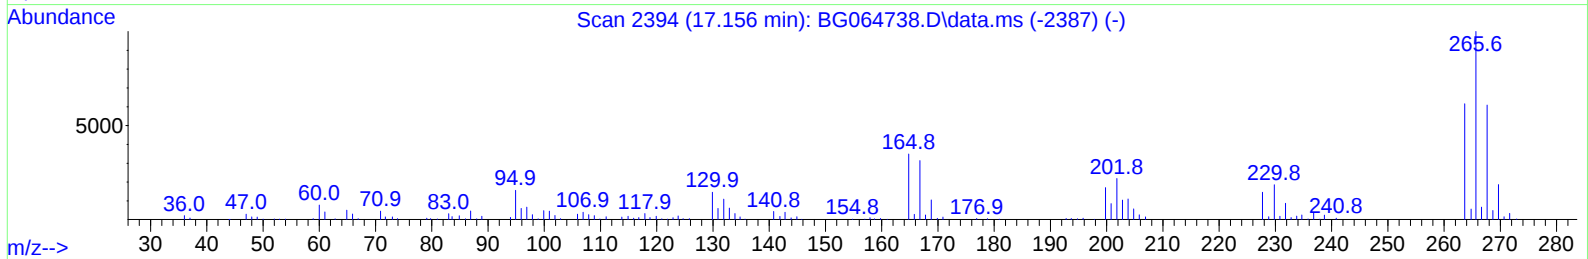
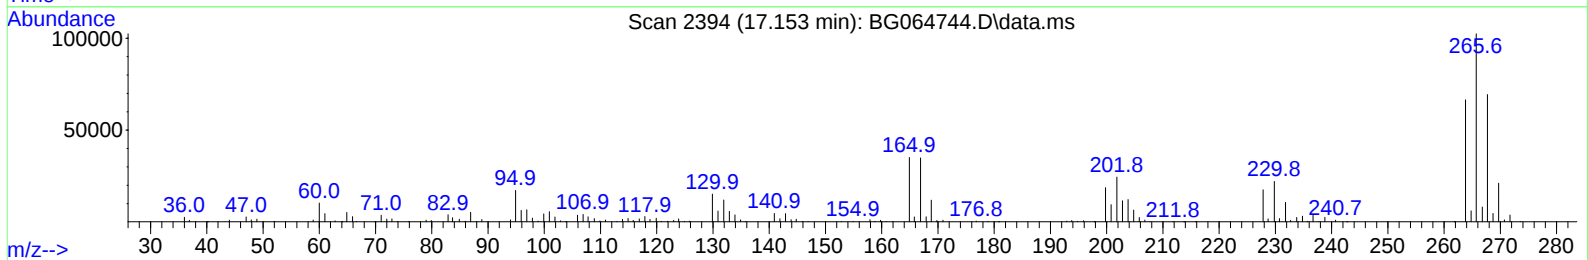


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111225\
Data File : BG064744.D
Acq On : 12 Nov 2025 10:37
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 12 11:53:33 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 12 01:10:41 2025
Response via : Initial Calibration

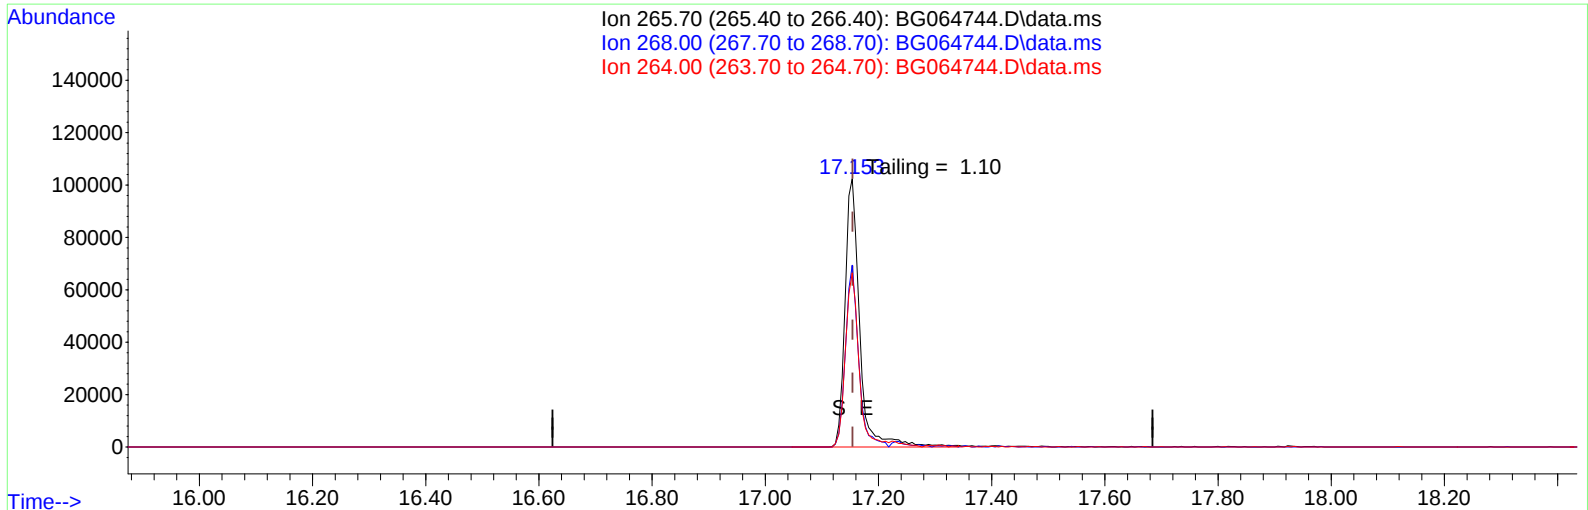

TIC: BG064744.D\data.ms

(70) Pentachlorophenol (C)




17.153min (-0.001) 31332.04 ng

response 182303

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.80	72.31
264.00	61.60	64.88
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111225\
Data File : BG064744.D
Acq On : 12 Nov 2025 10:37
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 12 11:53:33 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 12 01:10:41 2025
Response via : Initial Calibration

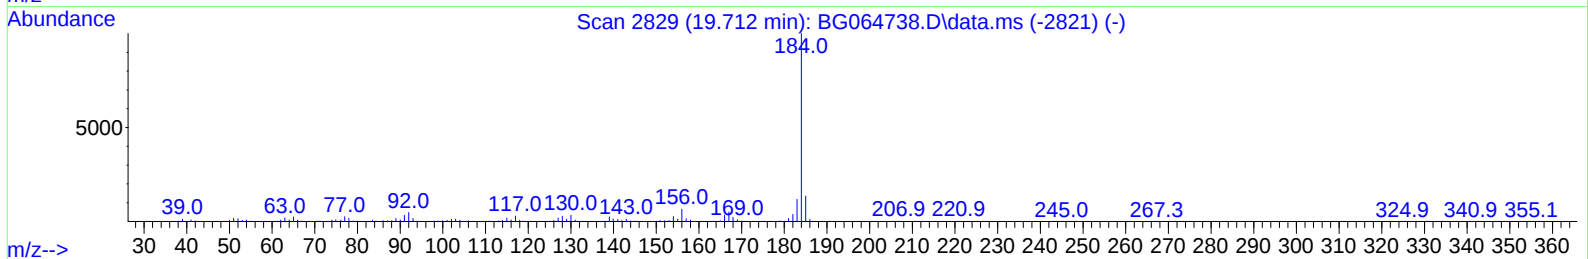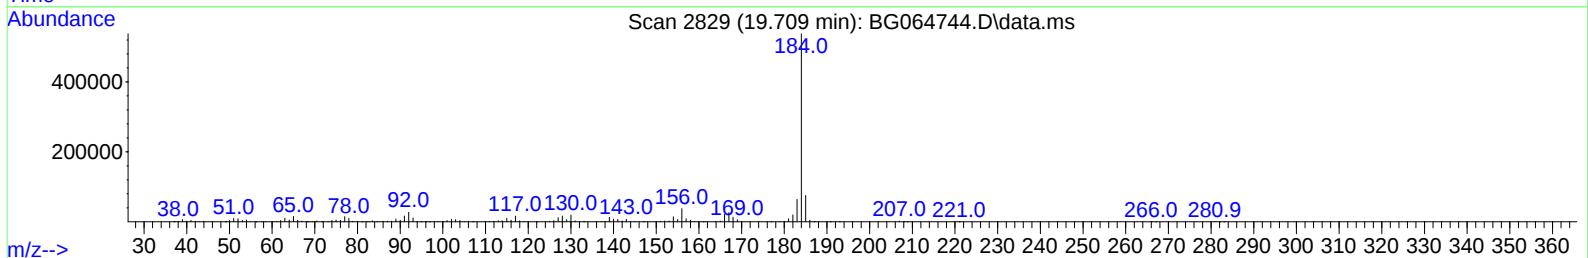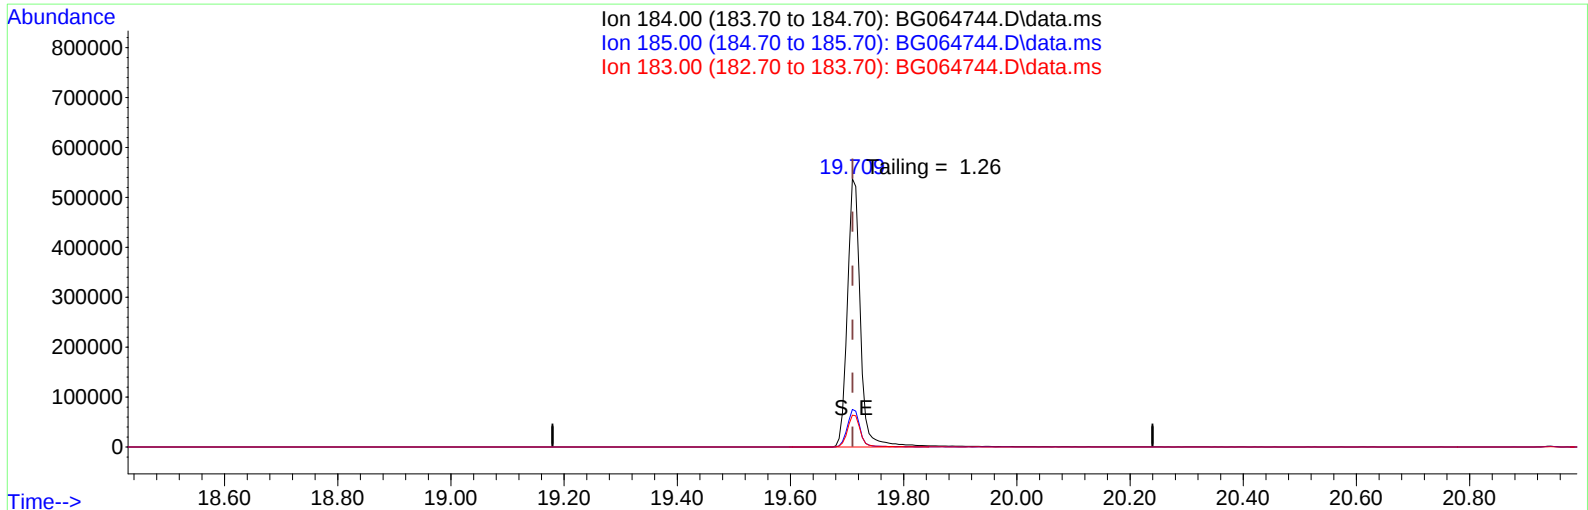

TIC: BG064744.D\data.ms

(77) Benzidine

19.709min (-0.000) 0.00 ng

response 866225

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.60	14.01
183.00	11.80	11.91
0.00	0.00	0.00