
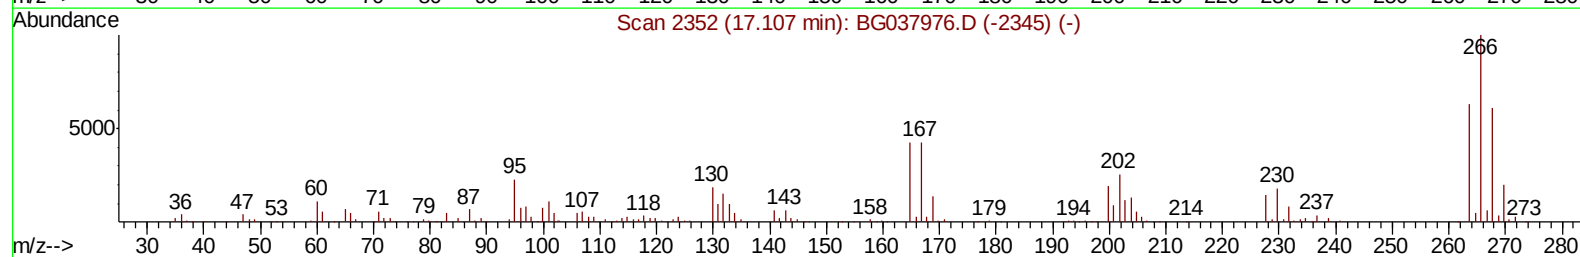
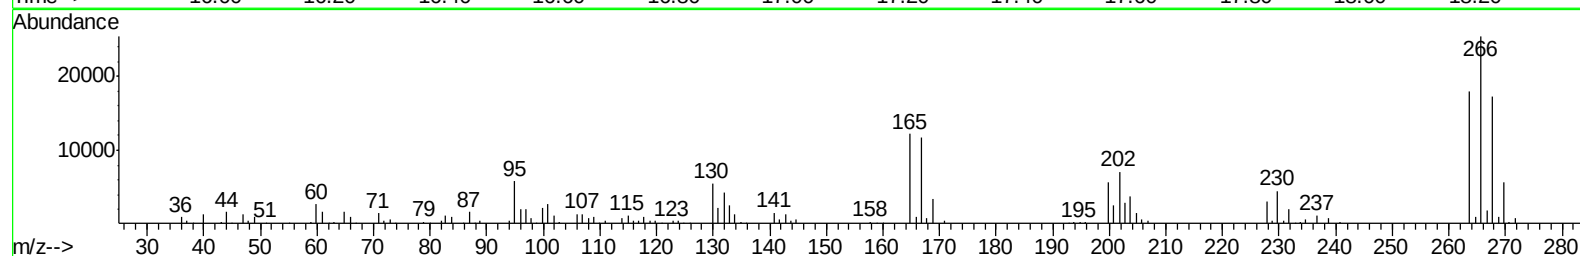


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG111318\
Data File : BG037972.D
Acq On : 13 Nov 2018 10:56
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 14 00:49:30 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG111318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 13 16:39:28 2018
Response via : Initial Calibration

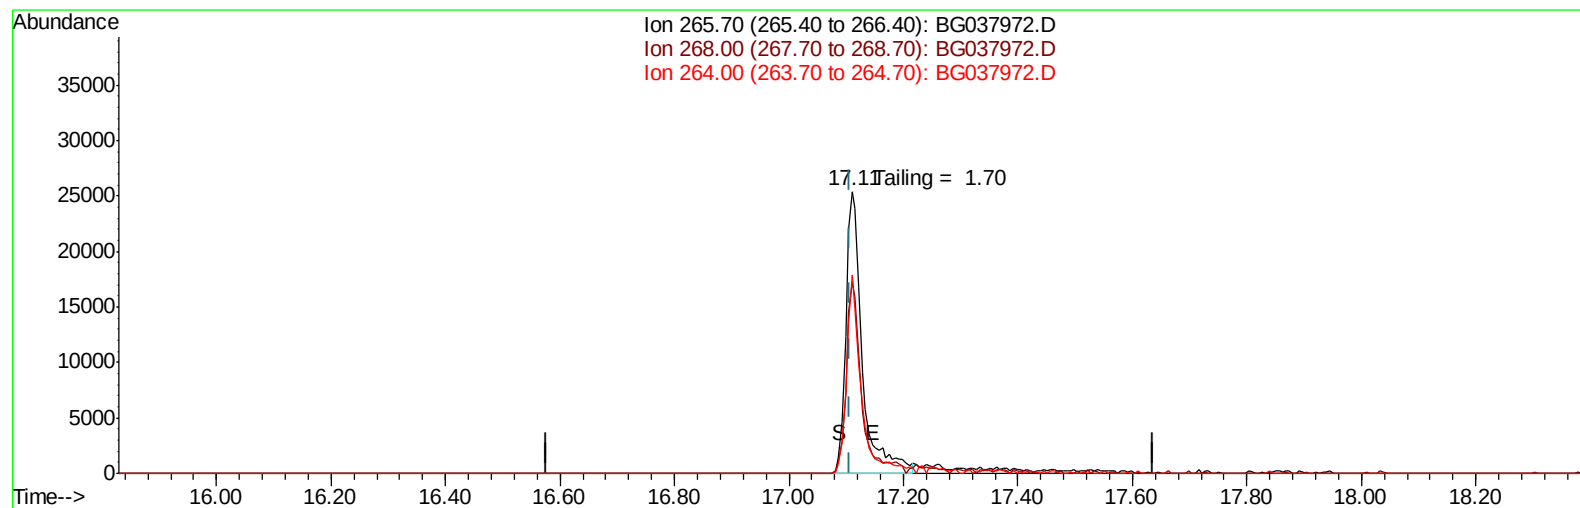

TIC: BG037972.D

(70) Pentachlorophenol (C)




17.110min (+0.003) 17579.68ng

response 50860

Ion	Exp%	Act%
265.70	100	100
268.00	68.80	71.69
264.00	73.60	74.81
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG111318\
Data File : BG037972.D
Acq On : 13 Nov 2018 10:56
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 14 00:49:30 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG111318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 13 16:39:28 2018
Response via : Initial Calibration

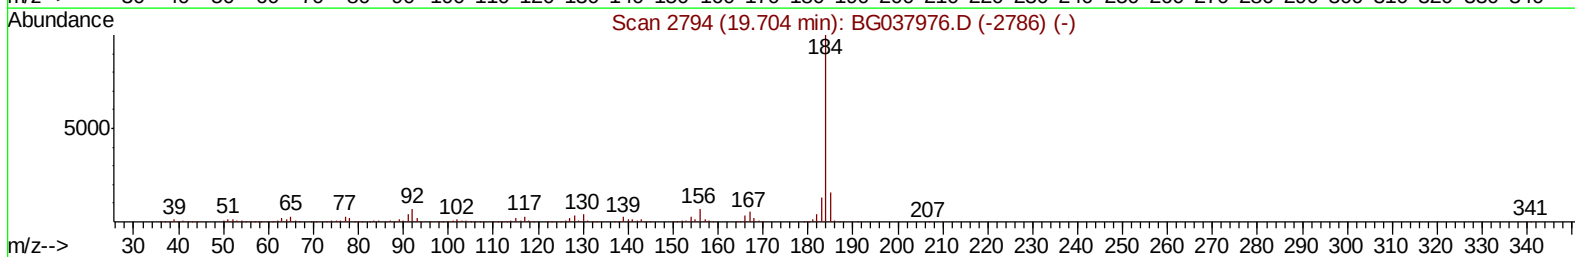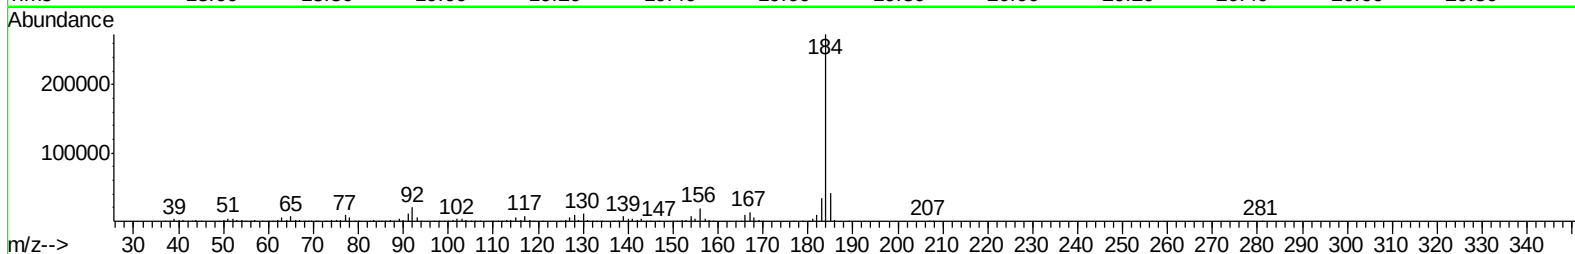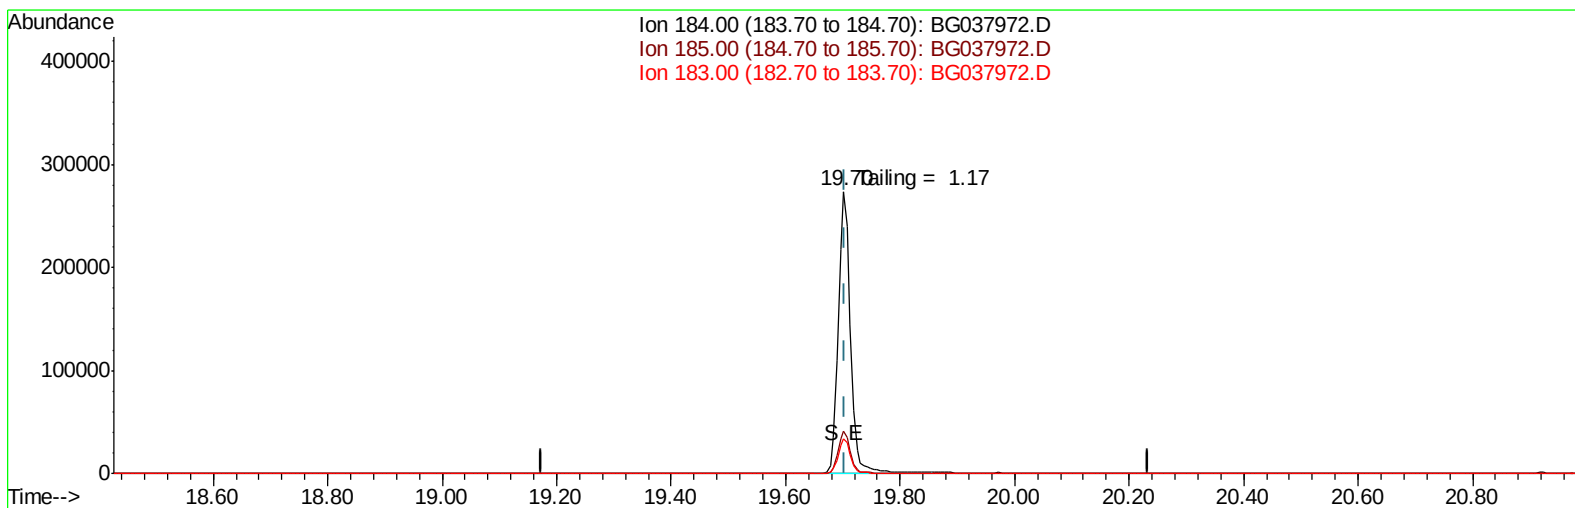

TIC: BG037972.D

(77) Benzidine

19.701min (-0.003) 3398.24ng

response 411383

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	15.10
183.00	12.70	12.23
0.00	0.00	0.00