
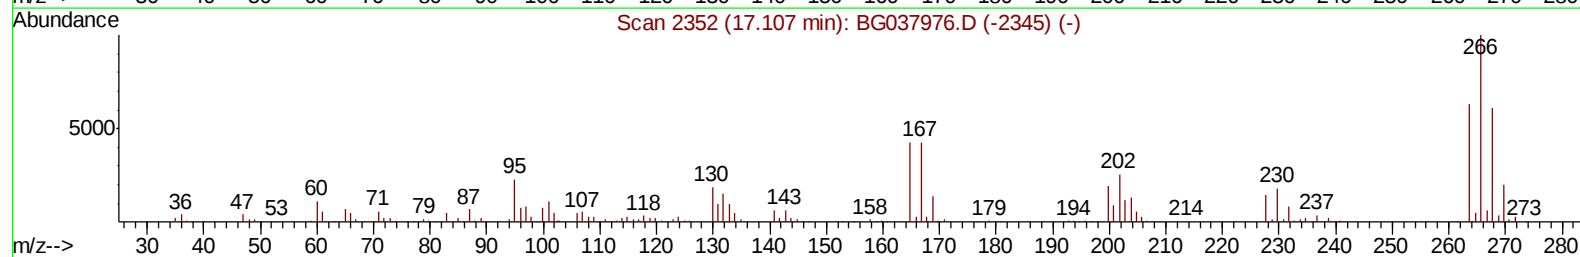
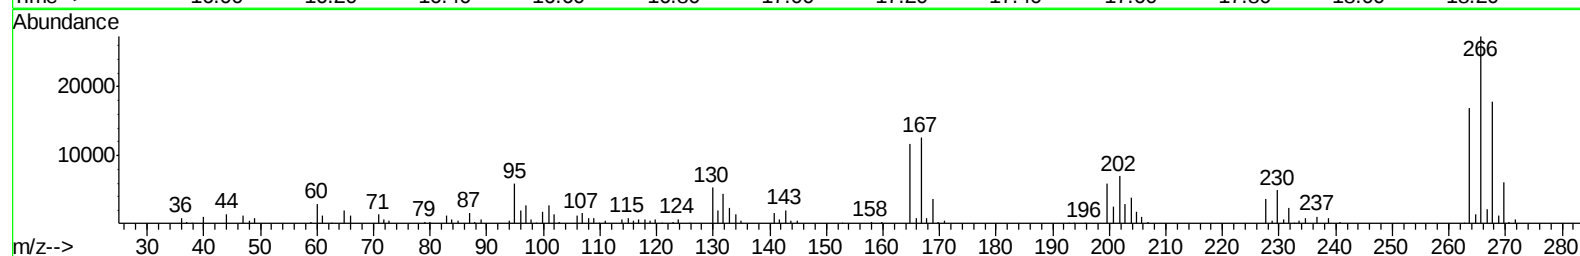


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG111318\
Data File : BG037981.D
Acq On : 13 Nov 2018 17:21
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 14 00:52:56 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG111318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 13 16:39:28 2018
Response via : Initial Calibration

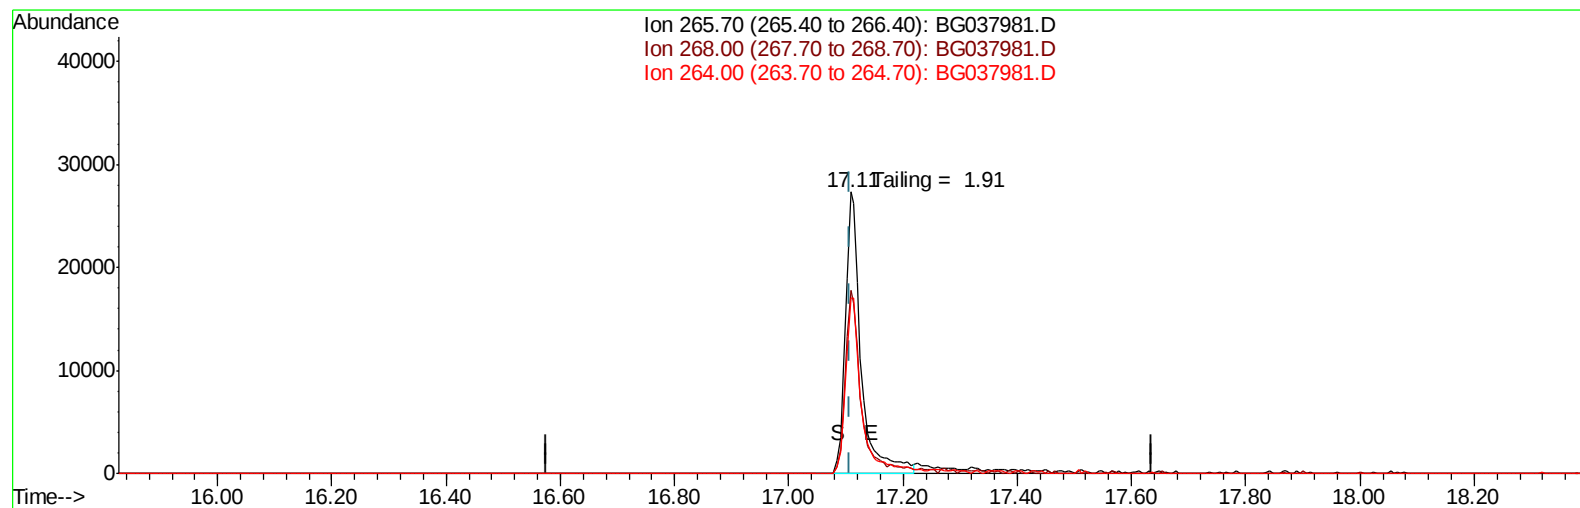

TIC: BG037981.D

(70) Pentachlorophenol (C)




17.108min (+0.000) 17818.38ng

response 52099

Ion	Exp%	Act%
265.70	100	100
268.00	68.80	69.63
264.00	73.60	67.22
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG111318\
 Data File : BG037981.D
 Acq On : 13 Nov 2018 17:21
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 14 00:52:56 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG111318.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 13 16:39:28 2018
 Response via : Initial Calibration

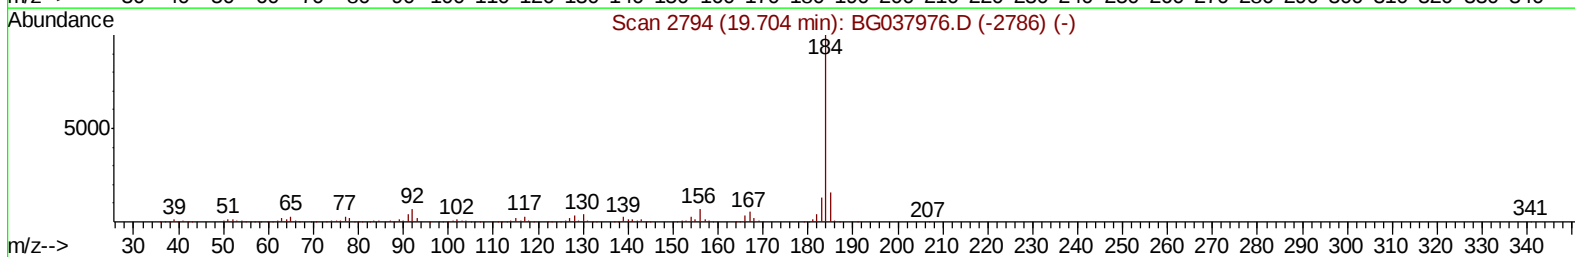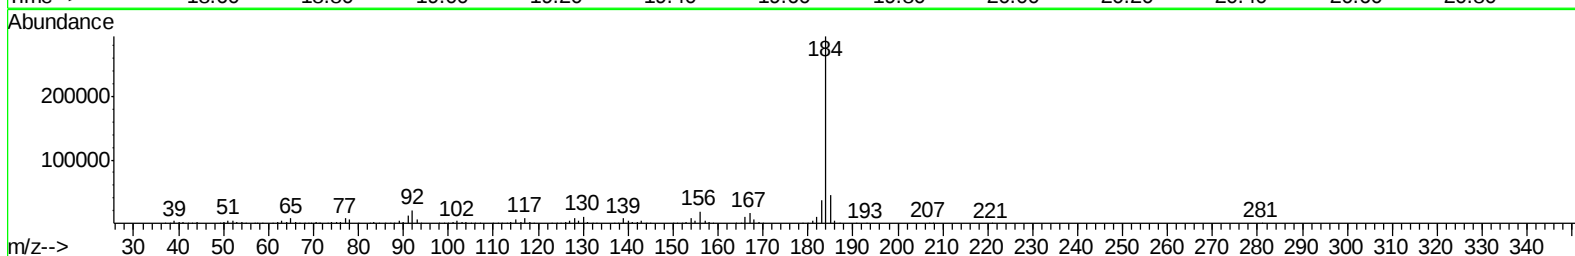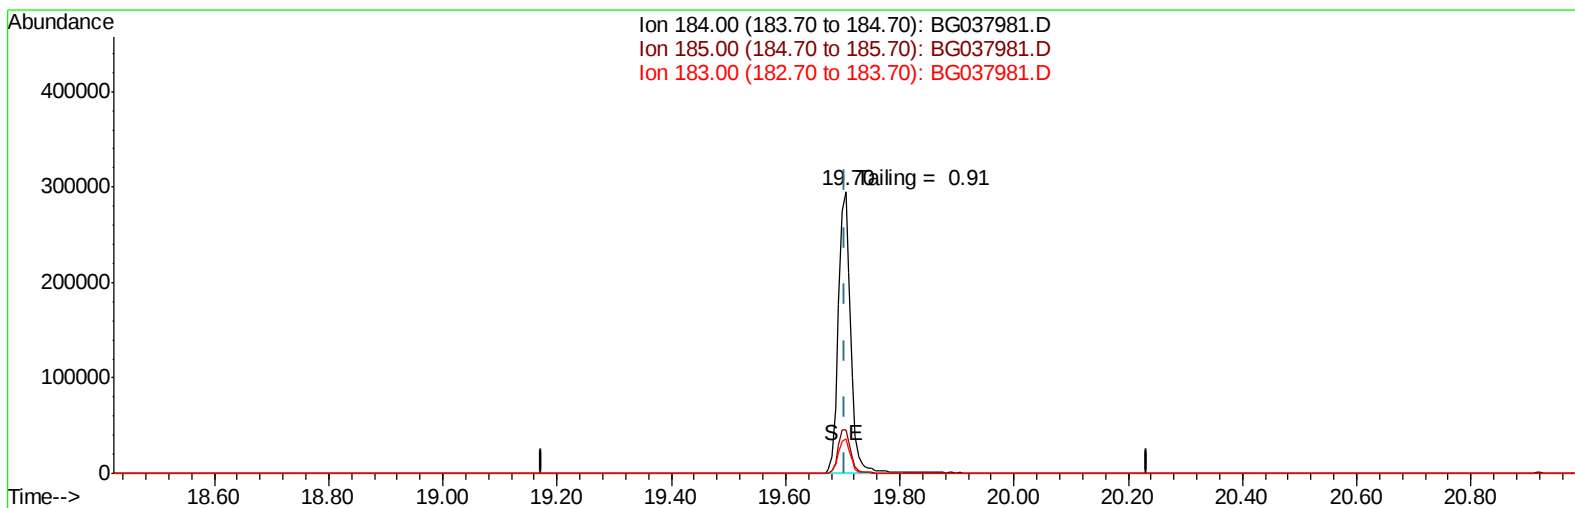

TIC: BG037981.D

(77) Benzidine

19.705min (+0.000) 13925.73ng

response 441733

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	15.47
183.00	12.70	12.25
0.00	0.00	0.00