


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG111318\
 Data File : BG037972.D
 Acq On : 13 Nov 2018 10:56
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG111318.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Nov 13 16:39:28 2018

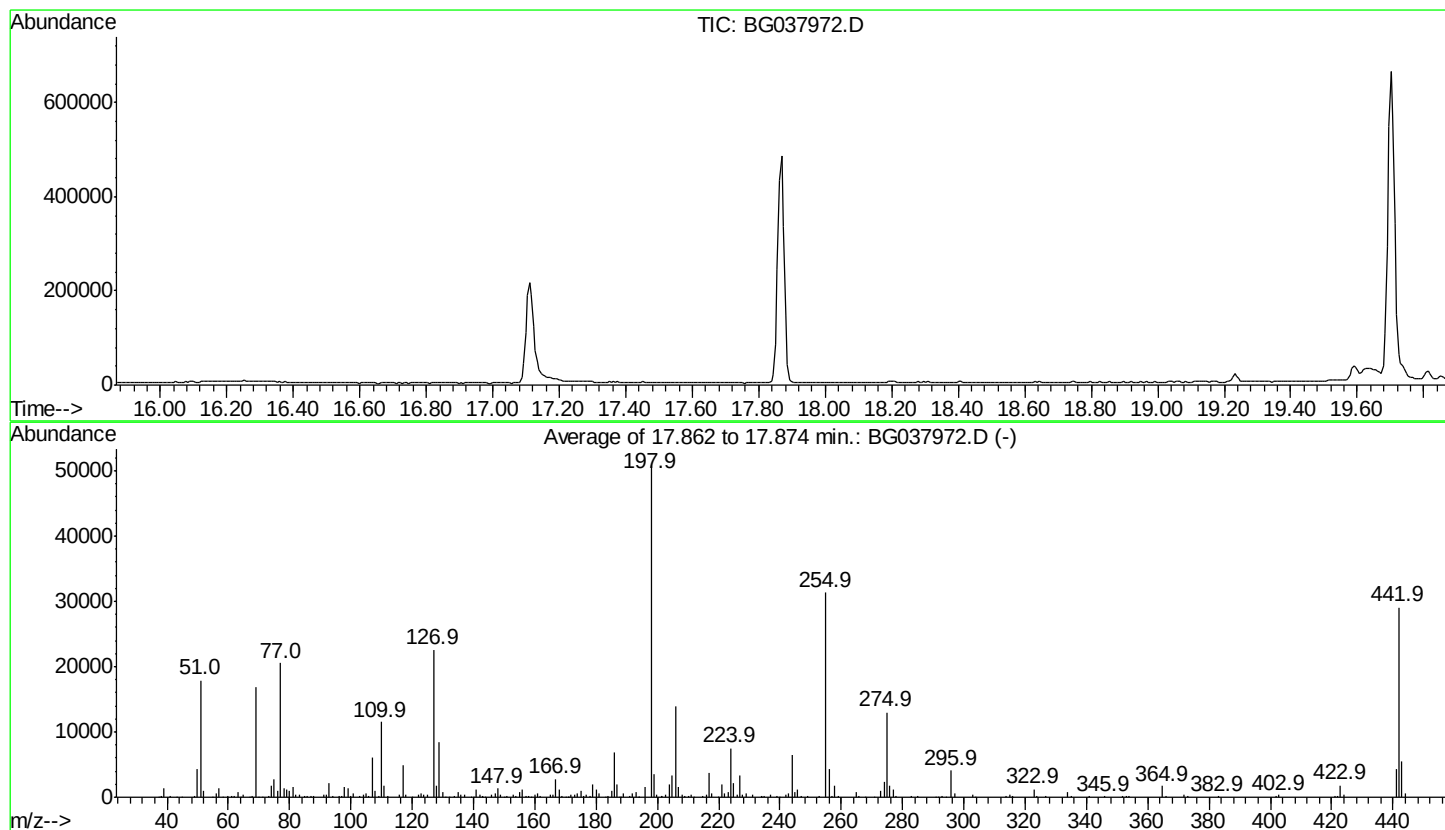

AutoFind: Scans 2480, 2481, 2482; Background Corrected with Scan 2473

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.2	17890	PASS
68	69	0.00	2	1.2	210	PASS
69	198	0.00	100	33.3	16927	PASS
70	69	0.00	2	0.5	82	PASS
127	198	10	80	44.5	22622	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	50784	PASS
199	198	5	9	6.8	3473	PASS
275	198	10	60	25.6	13013	PASS
365	198	1	100	3.3	1697	PASS
441	198	0.01	100	8.4	4282	PASS
442	198	50	100	57.3	29101	PASS
443	442	15	24	18.7	5451	PASS