




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111324\
Data File : BG063359.D
Acq On : 13 Nov 2024 18:05
Operator : RC/JU
Sample : PB164928BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK928

Manual IntegrationsAPPROVED

Quant Time: Nov 13 17:58:35 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 06 15:45:52 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/14/2024
Supervised By :mohammad ahmed 11/18/2024

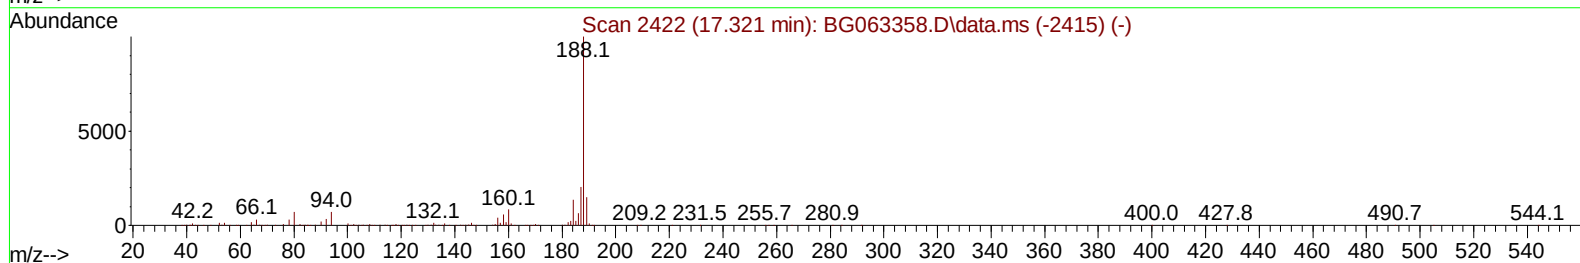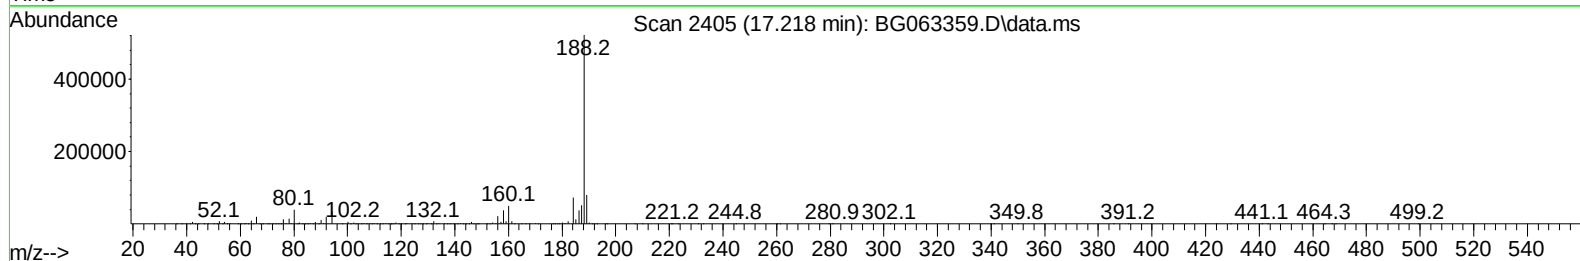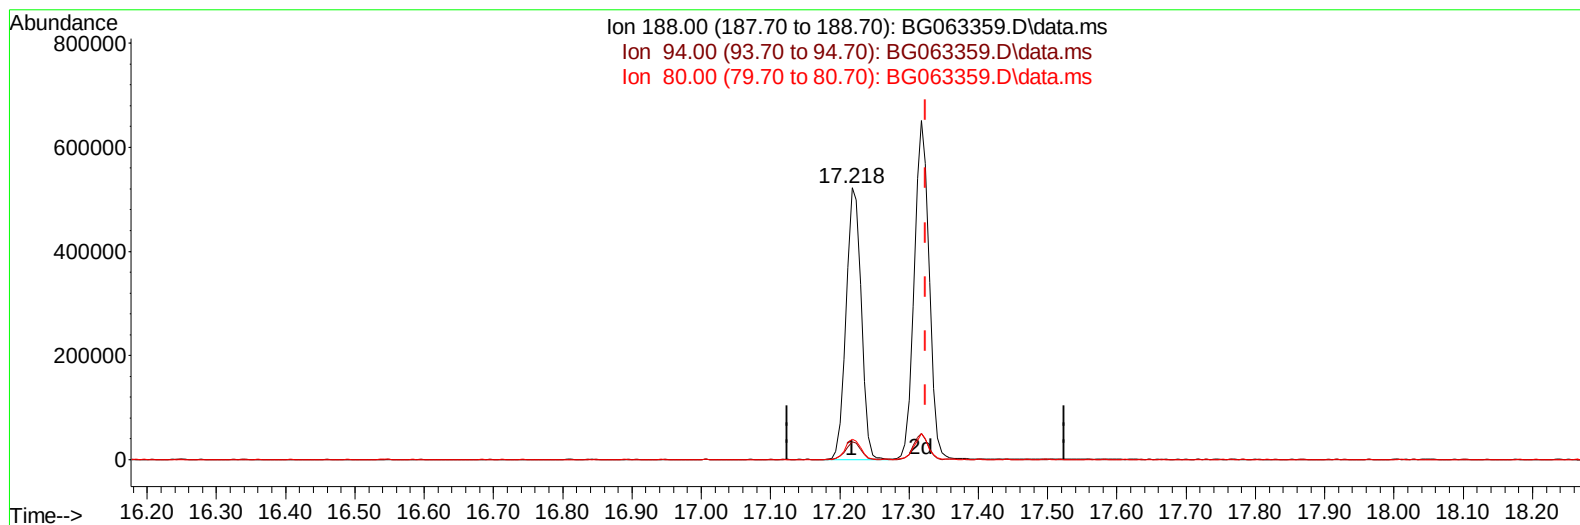

TIC: BG063359.D\data.ms

(73) Anthracene-d10 (S)

17.218min (-0.106) 23.27 ng/u1

response 782237

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	6.70	6.47
80.00	6.30	7.51
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111324\
Data File : BG063359.D
Acq On : 13 Nov 2024 18:05
Operator : RC/JU
Sample : PB164928BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK928

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/14/2024
Supervised By :mohammad ahmed 11/18/2024

Quant Time: Nov 13 17:58:35 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 06 15:45:52 2024
Response via : Initial Calibration

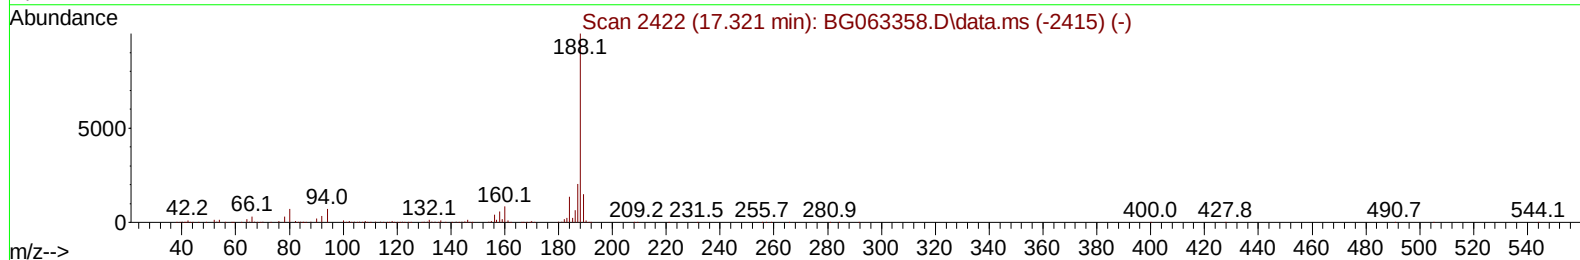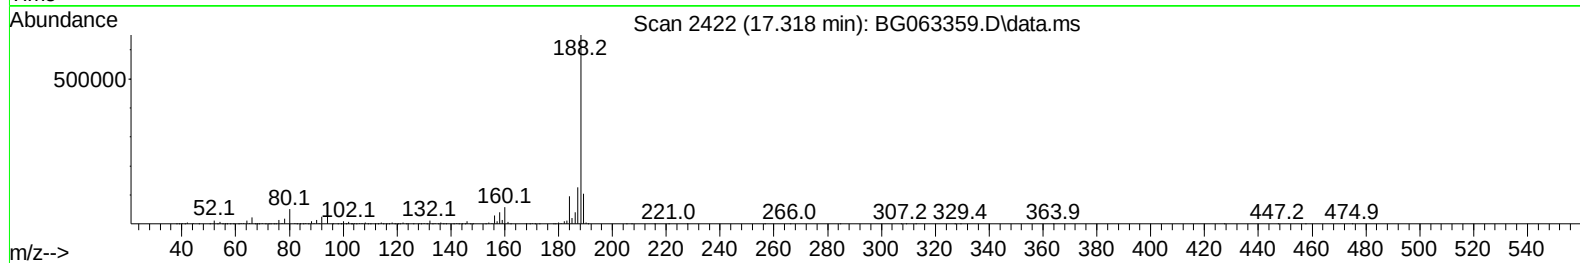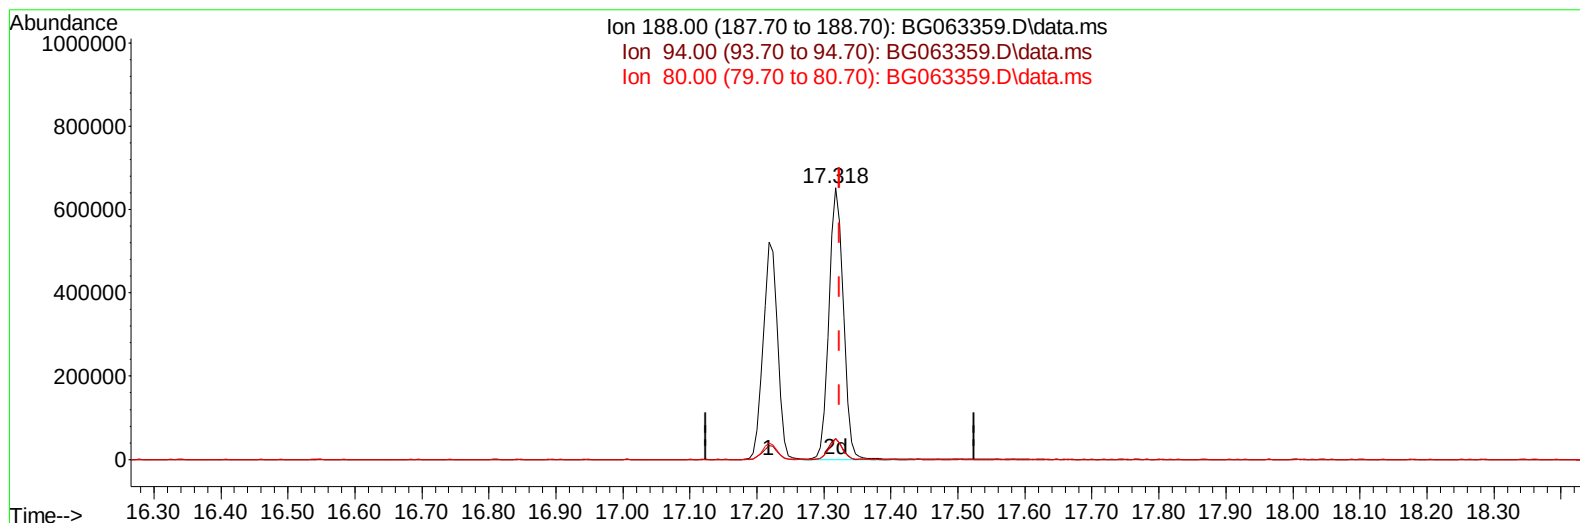

TIC: BG063359.D\data.ms

(73) Anthracene-d10 (S)

17.318min (-0.006) 28.98 ng/ul m

response 974380

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	6.70	7.59
80.00	6.30	7.74#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111324\
 Data File : BG063359.D
 Acq On : 13 Nov 2024 18:05
 Operator : RC/JU
 Sample : PB164928BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK928

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/14/2024
 Supervised By :mohammad ahmed 11/18/2024

Quant Time: Nov 13 17:59:13 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 06 15:45:52 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.835	152	78140	20.000	ng/ul	0.00
20) Naphthalene-d8	10.620	136	322870	20.000	ng/ul	# 0.00
38) Acenaphthene-d10	14.468	164	293482	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.218	188	782237	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.472	240	870485	20.000	ng/ul	# 0.00
88) Perylene-d12	24.503	264	913558	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.299	96	9980	5.775	ng/uL	0.00
4) Pyridine-d5	3.704	84	146358	25.624	ng/ul	0.00
7) Phenol-d5	7.006	99	164699	23.358	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.159	67	104781	25.335	ng/ul	-0.01
11) 2-Chlorophenol-d4	7.365	132	116812	25.524	ng/ul	-0.01
15) 4-Methylphenol-d8	8.540	113	137932	23.080	ng/ul	0.00
21) Nitrobenzene-d5	8.986	128	63421	27.940	ng/ul	0.00
24) 2-Nitrophenol-d4	9.709	143	77593	26.449	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.250	165	146222	25.398	ng/ul	0.00
31) 4-Chloroaniline-d4	10.755	131	189857	25.318	ng/ul	0.00
46) Dimethylphthalate-d6	13.875	166	567059	24.667	ng/ul	0.00
49) Acenaphthylene-d8	14.163	160	602700	26.786	ng/ul	0.00
54) 4-Nitrophenol-d4	14.680	143	76431	24.283	ng/ul	0.00
60) Fluorene-d10	15.467	176	512650	26.423	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.590	200	108420	22.054	ng/ul	0.00
73) Anthracene-d10	17.318	188	974380m	28.983	ng/ul	0.00
81) Pyrene-d10	19.615	212	1275394	29.223	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.298	264	1238531	28.080	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111324\
Data File : BG063359.D
Acq On : 13 Nov 2024 18:05
Operator : RC/JU
Sample : PB164928BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK928

Manual IntegrationsAPPROVED

Quant Time: Nov 13 17:59:13 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 06 15:45:52 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/14/2024
Supervised By :mohammad ahmed 11/18/2024

