




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111324\
Data File : BG063380.D
Acq On : 14 Nov 2024 7:57
Operator : RC/JU
Sample : P4802-06
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
GCPC8

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/15/2024
Supervised By :mohammad ahmed 11/18/2024

Quant Time: Nov 14 07:30:33 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 06 15:45:52 2024
Response via : Initial Calibration

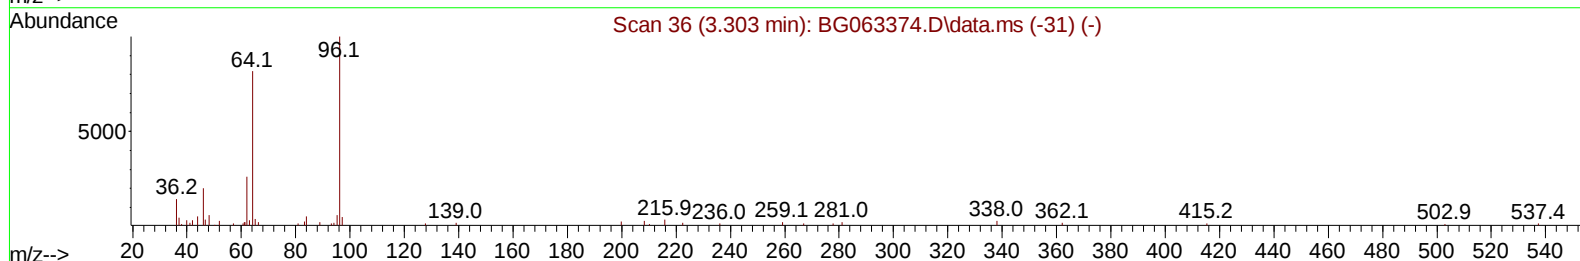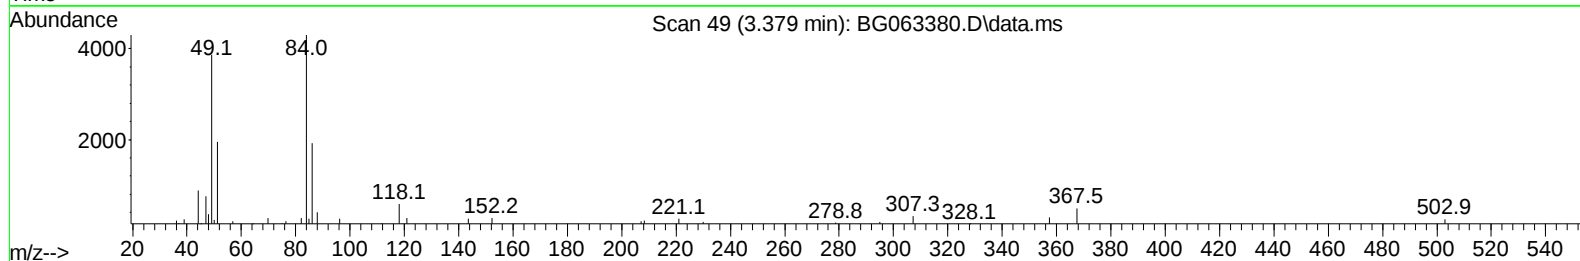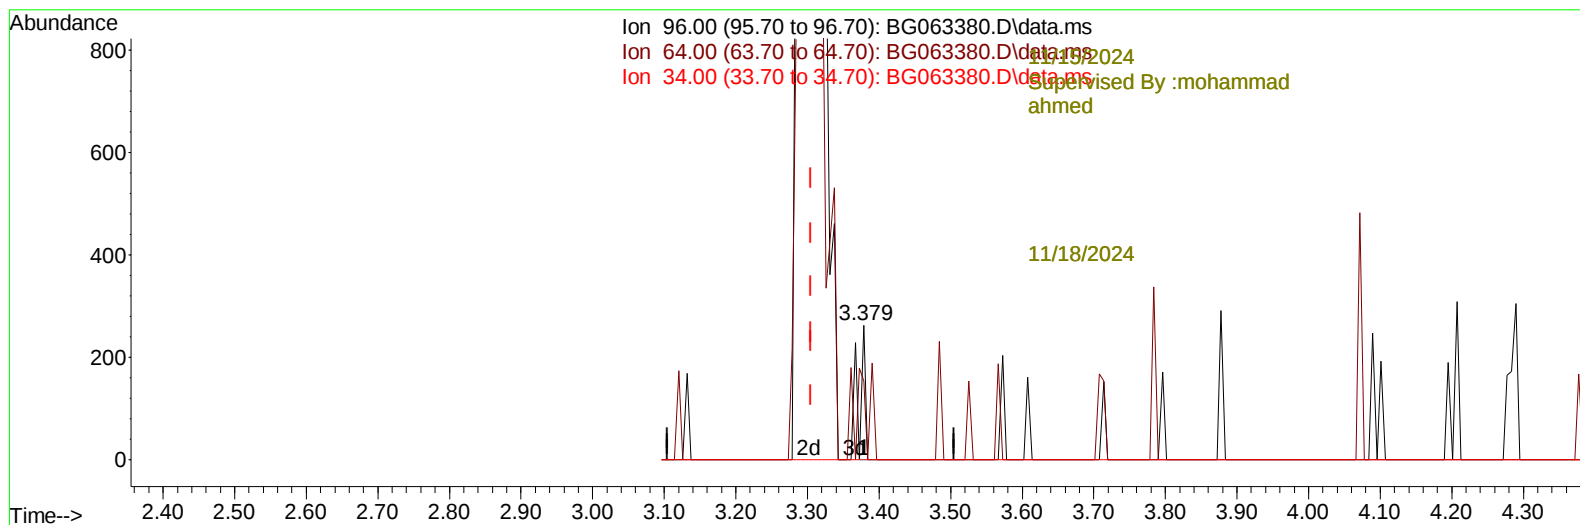

TIC: BG063380.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.379min (+ 0.073) 0.04 ng/uL

response	93	
Ion	Exp%	Act%
96.00	100.00	100.00
64.00	52.20	58.17
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111324\
Data File : BG063380.D
Acq On : 14 Nov 2024 7:57
Operator : RC/JU
Sample : P4802-06
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
GCPC8

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/15/2024
Supervised By :mohammad ahmed 11/18/2024

Quant Time: Nov 14 07:30:33 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 06 15:45:52 2024
Response via : Initial Calibration

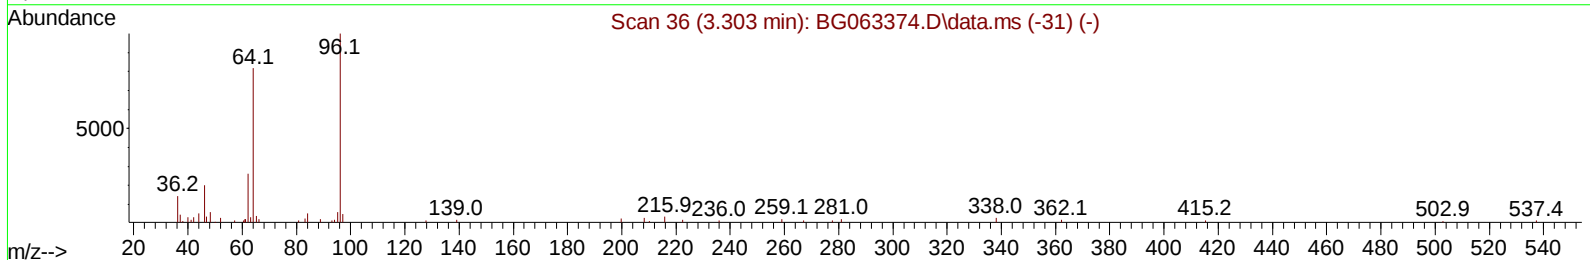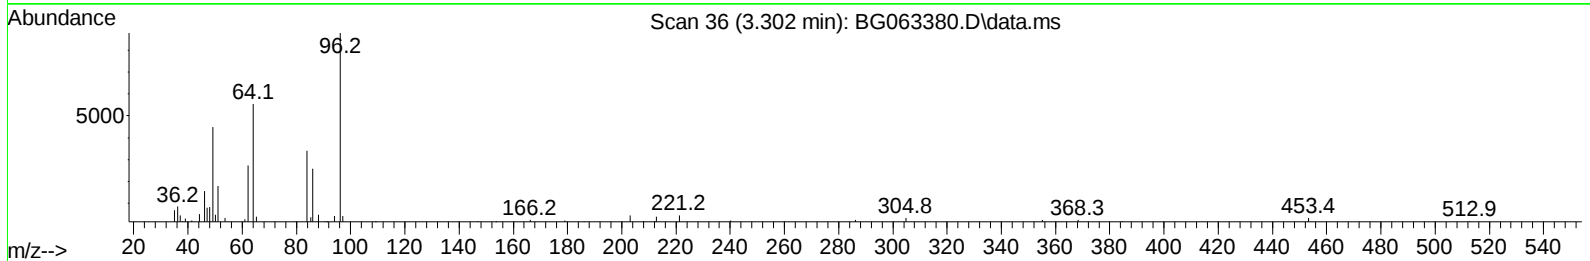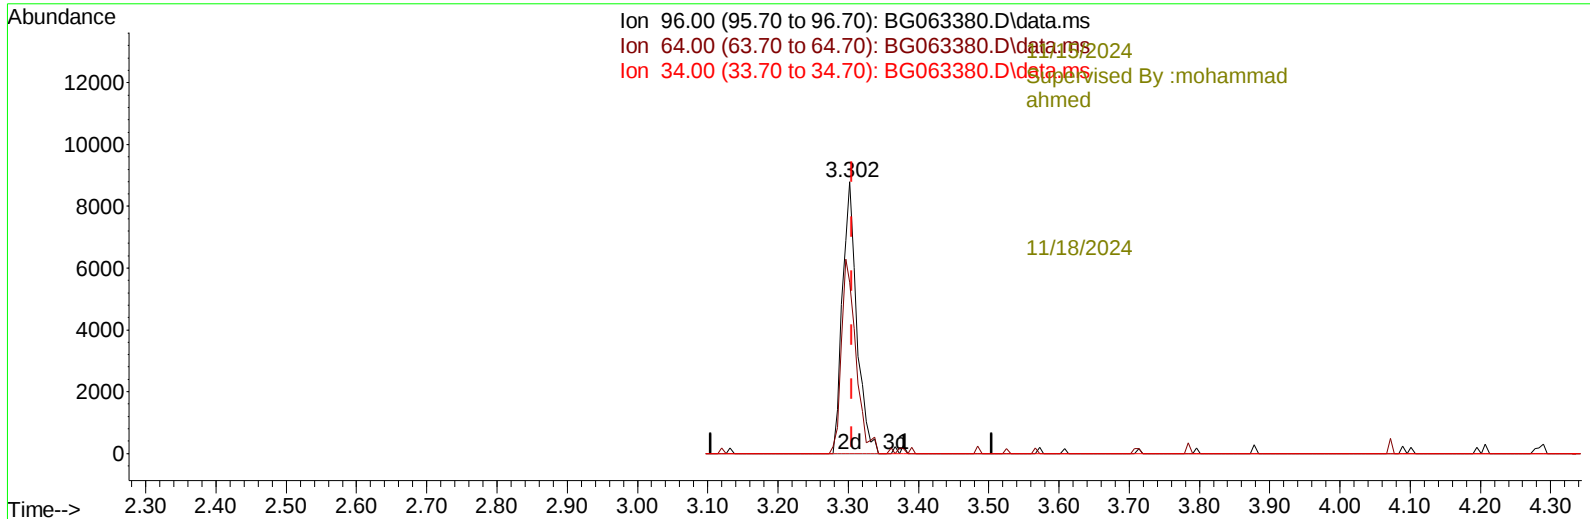

TIC: BG063380.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.302min (-0.003) 5.49 ng/uL m

response 12386

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	52.20	63.04#
34.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111324\
 Data File : BG063380.D
 Acq On : 14 Nov 2024 7:57
 Operator : RC/JU
 Sample : P4802-06
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 GCPC8

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/15/2024
 Supervised By :mohammad ahmed 11/18/2024

Quant Time: Nov 14 07:30:49 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 06 15:45:52 2024
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)
-----11/15/2024							
Supervised By :mohammad							
ahmed							
Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.832	152		101947	20.000	ng/ul	0.00
20) Naphthalene-d8	10.617	136		426219	20.000	ng/ul	# 0.00
38) Acenaphthene-d10	14.472	164		355158	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.221	188		935616	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.475	240		997059	20.000	ng/ul	# 0.00
88) Perylene-d12	24.507	264		1062548	20.000	ng/ul	0.0011/18/2024
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.302	96		12386m	5.494	ng/uL	0.00
4) Pyridine-d5	3.708	84		78704	10.562	ng/ul	0.00
7) Phenol-d5	7.004	99		118877	12.923	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.162	67		194309	36.011	ng/ul	0.00
11) 2-Chlorophenol-d4	7.368	132		210724	35.292	ng/ul	0.00
15) 4-Methylphenol-d8	8.537	113		195391	25.059	ng/ul	0.00
21) Nitrobenzene-d5	8.984	128		116464	38.867	ng/ul	0.00
24) 2-Nitrophenol-d4	9.707	143		152955	39.495	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.247	165		265855	34.980	ng/ul	0.00
31) 4-Chloroaniline-d4	10.758	131		268552	27.129	ng/ul	0.00
46) Dimethylphthalate-d6	13.878	166		964073	34.654	ng/ul	0.00
49) Acenaphthylene-d8	14.160	160		1061709	38.991	ng/ul	0.00
54) 4-Nitrophenol-d4	14.683	143		42060	11.042	ng/ul	0.00
60) Fluorene-d10	15.464	176		890879	37.944	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.588	200		201842	34.326	ng/ul	0.00
73) Anthracene-d10	17.321	188		1577983	39.242	ng/ul	0.00
81) Pyrene-d10	19.618	212		2072549	41.459	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.301	264		2027276	39.517	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111324\
Data File : BG063380.D
Acq On : 14 Nov 2024 7:57
Operator : RC/JU
Sample : P4802-06
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
GCPC8

Manual IntegrationsAPPROVED

Quant Time: Nov 14 07:30:49 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 06 15:45:52 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/15/2024
Supervised By :mohammad ahmed 11/18/2024

