




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111324\
 Data File : BG063382.D
 Acq On : 14 Nov 2024 9:12
 Operator : RC/JU
 Sample : P4802-08
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 GCPD0

Manual IntegrationsAPPROVED

Quant Time: Nov 14 10:19:53 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 06 15:45:52 2024
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/15/2024
 Supervised By :mohammad ahmed 11/18/2024

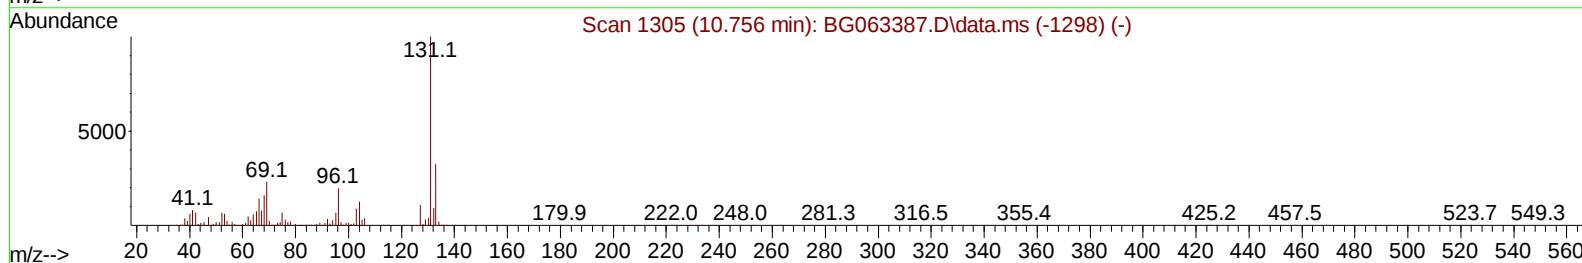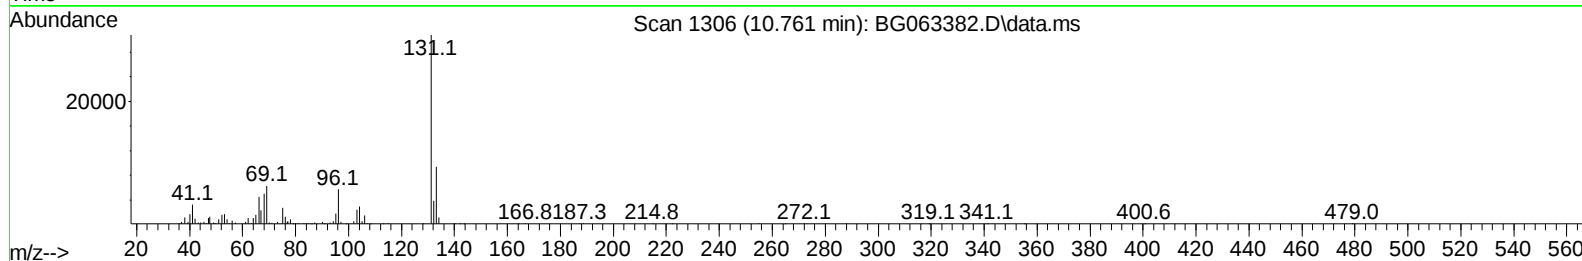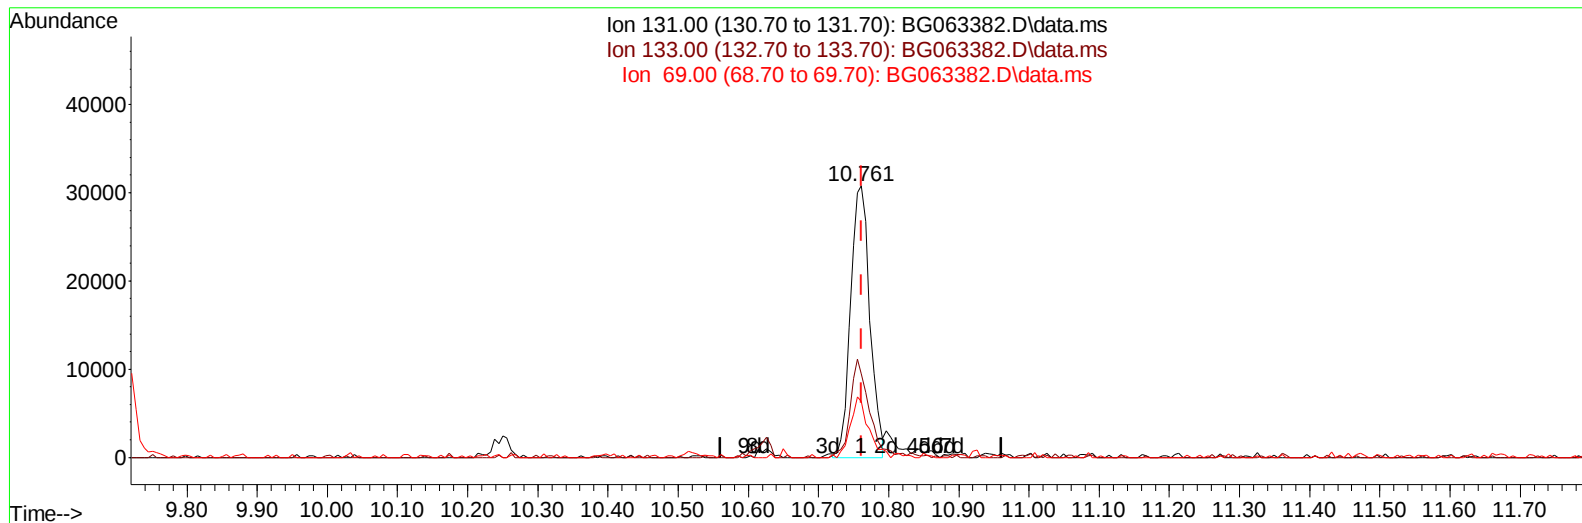

TIC: BG063382.D\data.ms

(31) 4-Chloroaniline-d4 (S)

10.761min (+ 0.000) 6.10 ng/u1

response 58821

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	29.80	30.70
69.00	24.60	20.56
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111324\
 Data File : BG063382.D
 Acq On : 14 Nov 2024 9:12
 Operator : RC/JU
 Sample : P4802-08
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 GCPD0

Manual IntegrationsAPPROVED

Quant Time: Nov 14 10:19:53 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 06 15:45:52 2024
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/15/2024
 Supervised By :mohammad ahmed 11/18/2024

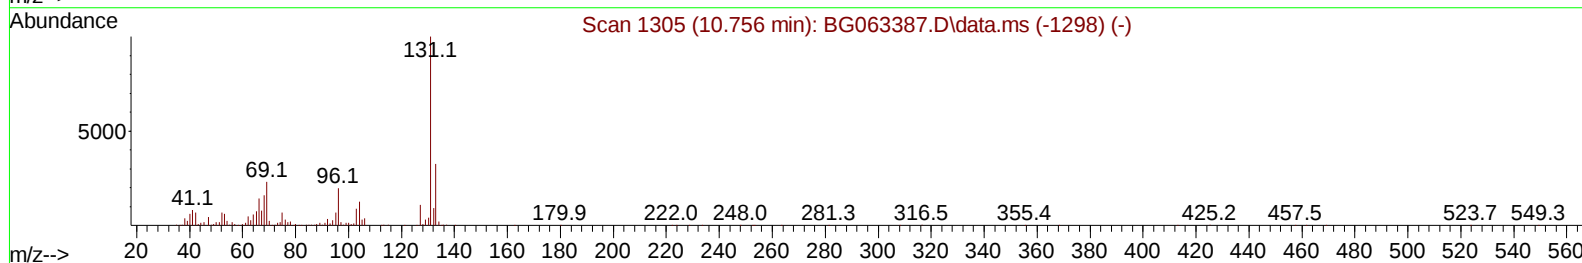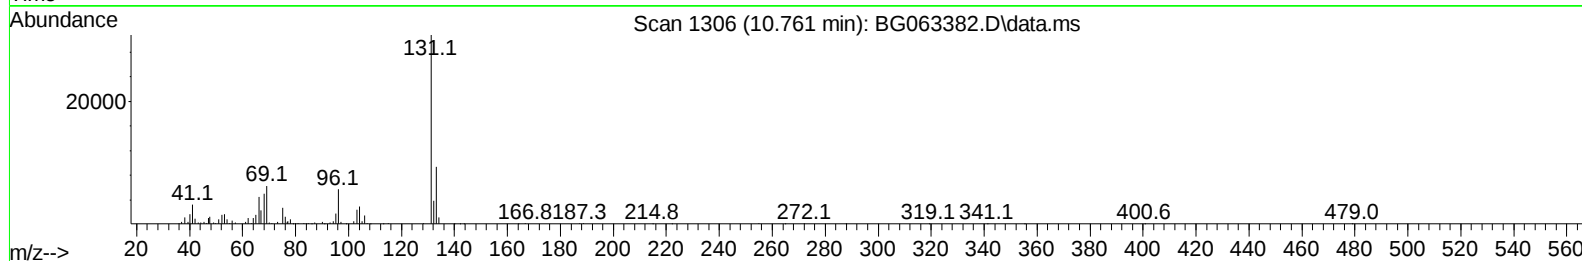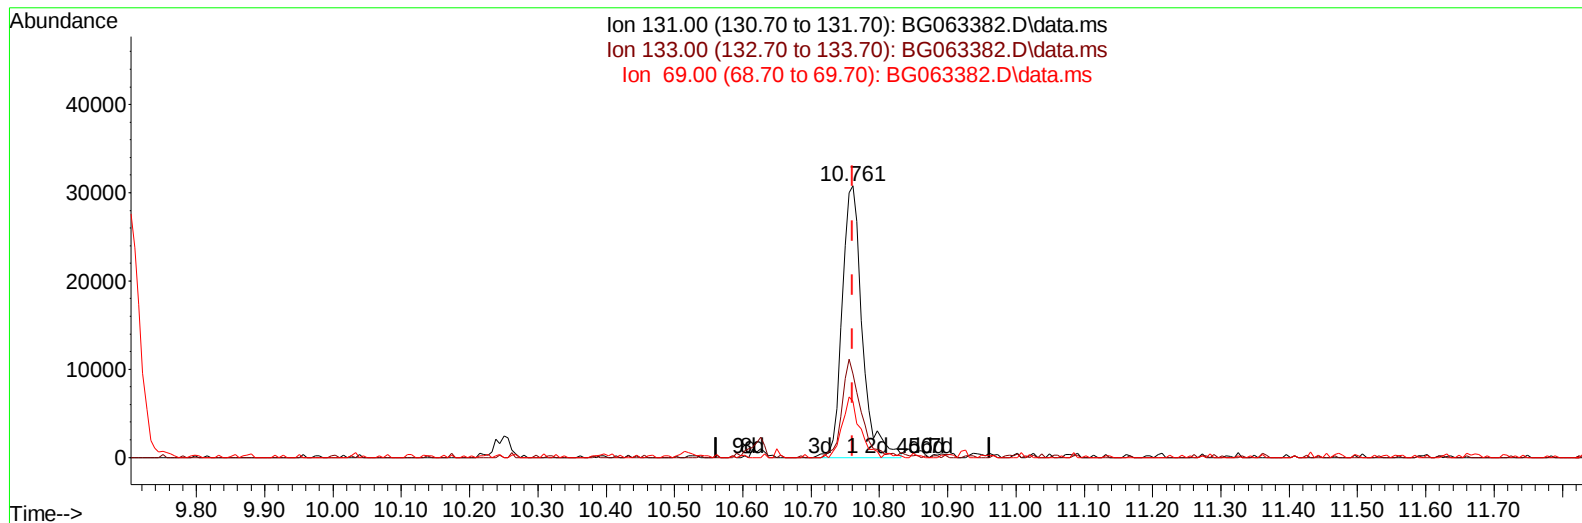

TIC: BG063382.D\data.ms

(31) 4-Chloroaniline-d4 (S)

10.761min (+ 0.000) 6.51 ng/ul m

response 62723

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	29.80	30.70
69.00	24.60	20.56
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111324\
 Data File : BG063382.D
 Acq On : 14 Nov 2024 9:12
 Operator : RC/JU
 Sample : P4802-08
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 GCPD0

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/15/2024
 Supervised By :mohammad ahmed 11/18/2024

Quant Time: Nov 14 23:36:44 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 06 15:45:52 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.829	152	97848	20.000	ng/ul	-0.01
20) Naphthalene-d8	10.620	136	415134	20.000	ng/ul	# 0.00
38) Acenaphthene-d10	14.469	164	347827	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.218	188	875136	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.472	240	912918	20.000	ng/ul	# 0.00
88) Perylene-d12	24.510	264	996267	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.299	96	10222	4.724	ng/uL	0.00
4) Pyridine-d5	0.000	84	0d	0.000	ng/ul	
7) Phenol-d5	7.007	99	68067	7.709	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.166	67	107401	20.738	ng/ul	0.00
11) 2-Chlorophenol-d4	7.371	132	105592	18.425	ng/ul	0.00
15) 4-Methylphenol-d8	8.540	113	106781	14.269	ng/ul	0.00
21) Nitrobenzene-d5	8.987	128	62311	21.350	ng/ul	0.00
24) 2-Nitrophenol-d4	9.704	143	76631	20.316	ng/ul	-0.01
28) 2,4-Dichlorophenol-d3	10.244	165	143810	19.427	ng/ul	0.00
31) 4-Chloroaniline-d4	10.761	131	62723m	6.505	ng/ul	0.00
46) Dimethylphthalate-d6	13.875	166	604352	22.182	ng/ul	0.00
49) Acenaphthylene-d8	14.163	160	590804	22.155	ng/ul	0.00
54) 4-Nitrophenol-d4	14.686	143	30042	8.053	ng/ul	0.00
60) Fluorene-d10	15.468	176	544979	23.701	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.591	200	127646	23.208	ng/ul	0.00
73) Anthracene-d10	17.318	188	973221	25.875	ng/ul	0.00
81) Pyrene-d10	19.616	212	1308483	28.587	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.298	264	1231462	25.602	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111324\
Data File : BG063382.D
Acq On : 14 Nov 2024 9:12
Operator : RC/JU
Sample : P4802-08
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
GCPD0

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/15/2024
Supervised By :mohammad ahmed 11/18/2024

Quant Time: Nov 14 23:36:44 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 06 15:45:52 2024
Response via : Initial Calibration

