

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111324\
 Data File : BG063414.D
 Acq On : 15 Nov 2024 6:03
 Operator : RC/JU
 Sample : P4761-05
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 A0AL7

Quant Time: Nov 15 05:38:39 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 06 15:45:52 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.831	152	119380	20.000	ng/u1	0.00
20) Naphthalene-d8	10.622	136	484120	20.000	ng/u1	# 0.00
38) Acenaphthene-d10	14.471	164	386773	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.226	188	945107	20.000	ng/u1	0.00
79) Chrysene-d12	21.480	240	947355	20.000	ng/u1	# 0.00
88) Perylene-d12	24.518	264	1035167	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.307	96	10554	3.998	ng/uL	0.00
4) Pyridine-d5	3.707	84	169583	19.434	ng/u1	0.00
7) Phenol-d5	7.015	99	99501	9.237	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.161	67	156023	24.693	ng/u1	0.00
11) 2-Chlorophenol-d4	7.367	132	174885	25.012	ng/u1	0.00
15) 4-Methylphenol-d8	8.542	113	182350	19.972	ng/u1	0.00
21) Nitrobenzene-d5	8.989	128	94130	27.657	ng/u1	0.00
24) 2-Nitrophenol-d4	9.706	143	121114	27.533	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.252	165	249435	28.895	ng/u1	0.00
31) 4-Chloroaniline-d4	10.757	131	522395	46.460	ng/u1	0.00
46) Dimethylphthalate-d6	13.877	166	872123	28.787	ng/u1	0.00
49) Acenaphthylene-d8	14.165	160	870949	29.371	ng/u1	0.00
54) 4-Nitrophenol-d4	14.700	143	35903	8.655	ng/u1	0.02
60) Fluorene-d10	15.464	176	770444	30.132	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.593	200	174429	29.366	ng/u1	0.00
73) Anthracene-d10	17.320	188	1366445	33.640	ng/u1	0.00
81) Pyrene-d10	19.623	212	1759233	37.038	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.312	264	1755950	35.134	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.342	88	7361	2.265	ng/uL#	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111324\
Data File : BG063414.D
Acq On : 15 Nov 2024 6:03
Operator : RC/JU
Sample : P4761-05
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
A0AL7

Quant Time: Nov 15 05:38:39 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 06 15:45:52 2024
Response via : Initial Calibration

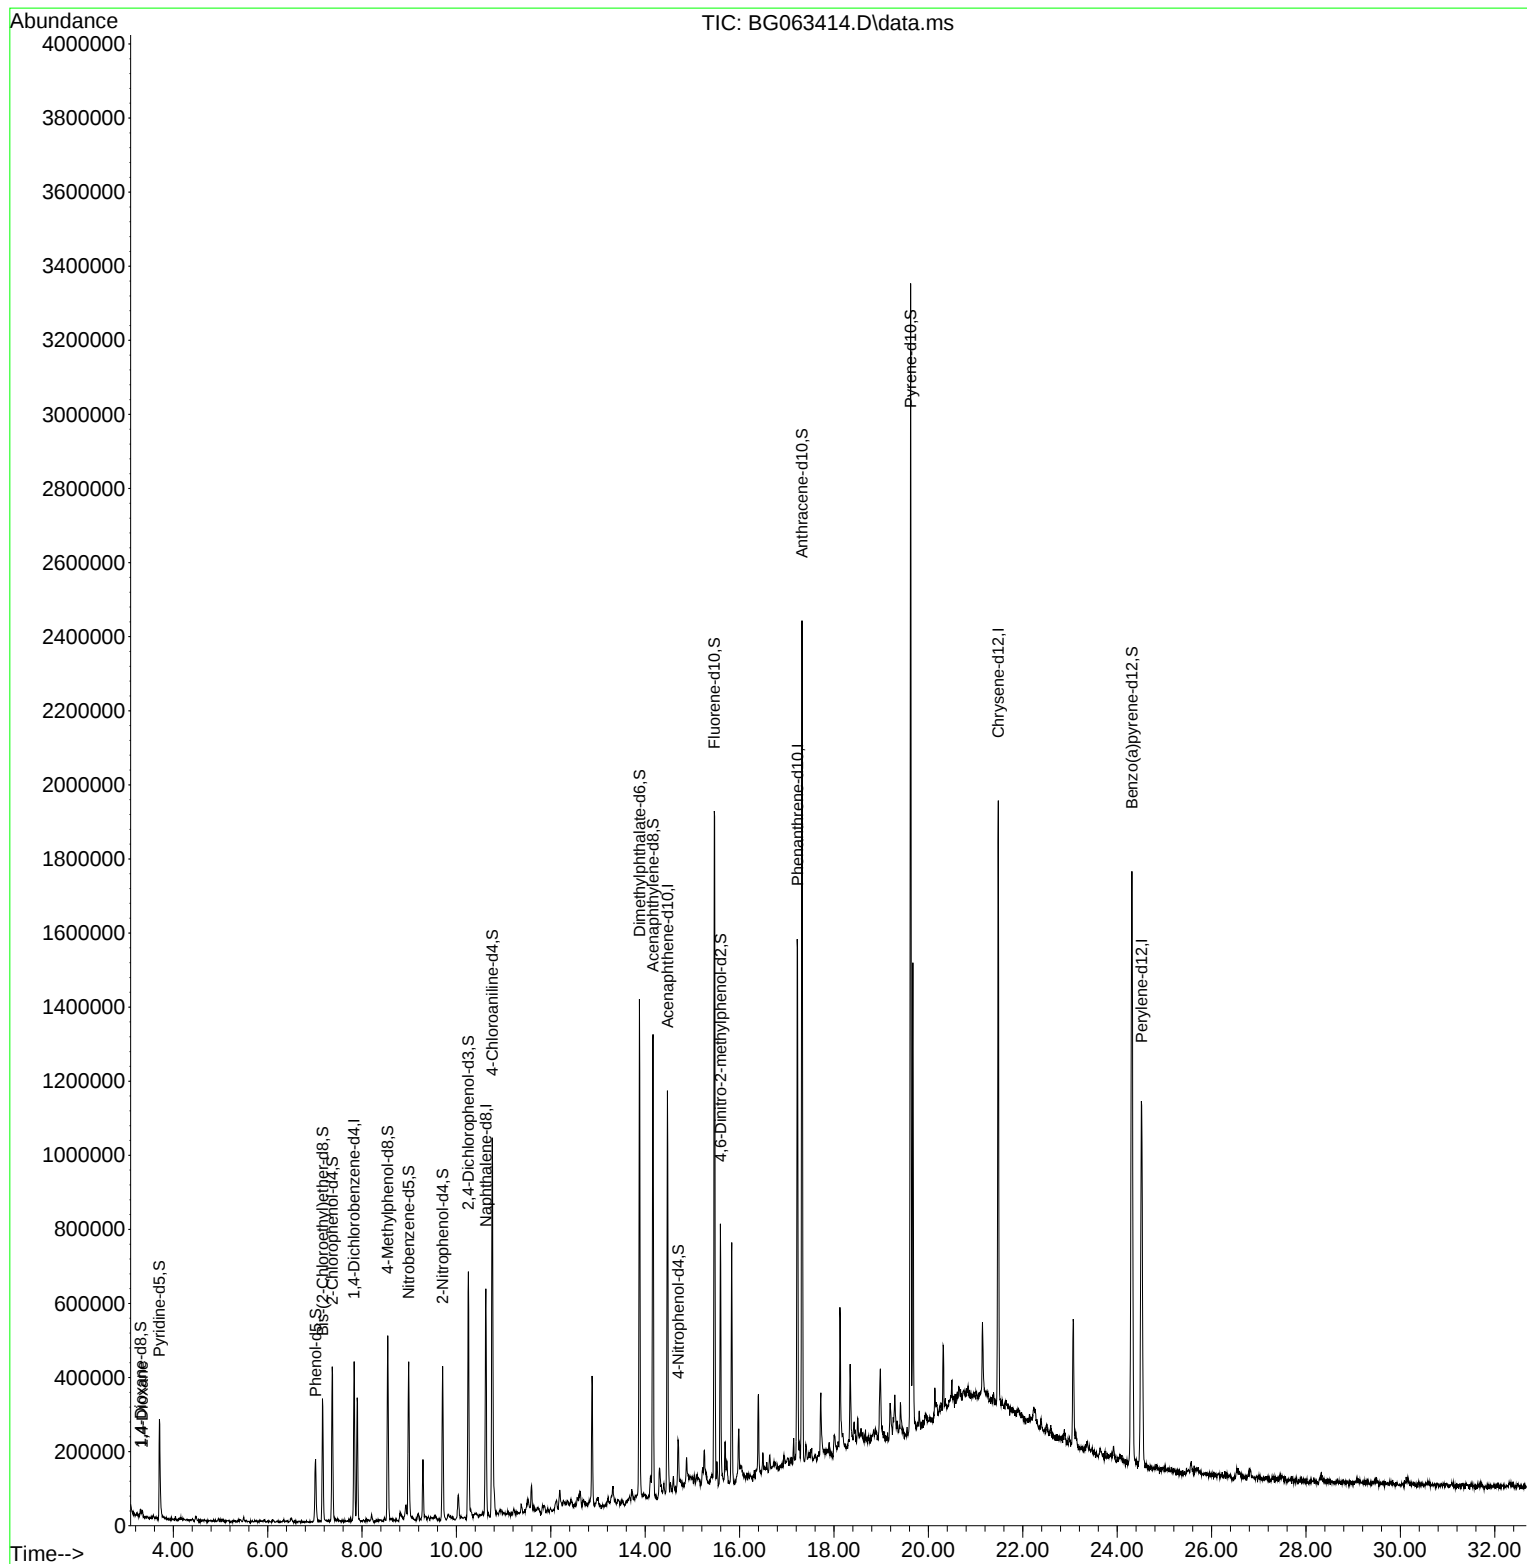

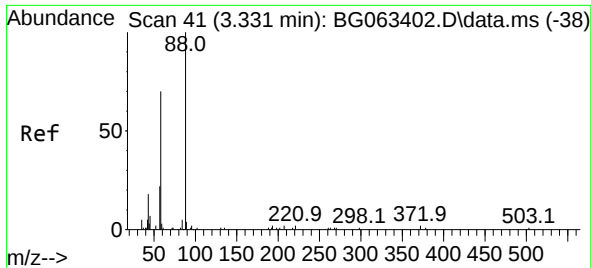

#2
1,4-Dioxane
Concen: 2.265 ng/uL
RT: 3.342 min Scan# 41
Delta R.T. 0.002 min
Lab File: BG063414.D
Acq: 15 Nov 2024 6:03

Instrument :
BNA_G
ClientSampleId :
A0AL7

Tgt Ion: 88 Resp: 7361
Ion Ratio Lower Upper
88 100
43 29.0 29.6 44.4#
58 62.8 46.5 69.7

