

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111324\
 Data File : BG063352.D
 Acq On : 13 Nov 2024 11:07
 Operator : RC/JU
 Sample : PB164920BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK920

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG063352.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.295	32	35	41	rVB2	23772	29320	0.74%	0.082%
2	3.701	99	104	115	rBV	299053	469523	11.85%	1.311%
3	4.335	210	212	217	rBV4	3686	6059	0.15%	0.017%
4	4.817	291	294	296	rVB4	5270	6458	0.16%	0.018%
5	5.017	325	328	330	rBV2	6177	6578	0.17%	0.018%
6	7.003	659	666	677	rBV	402679	660977	16.68%	1.845%
7	7.161	686	693	702	rBV	292863	477790	12.06%	1.334%
8	7.361	721	727	736	rVB	358402	617924	15.59%	1.725%
9	7.831	801	807	814	rBV	380653	624587	15.76%	1.743%
10	8.448	909	912	916	rBV2	5252	8042	0.20%	0.022%
11	8.536	921	927	936	rVV	514904	848528	21.41%	2.369%
12	8.636	942	944	950	rVB2	4856	8136	0.21%	0.023%
13	8.889	985	987	991	rVB3	5054	6493	0.16%	0.018%
14	8.983	995	1003	1011	rBV	382874	671941	16.96%	1.876%
15	9.194	1031	1039	1041	rBV7	15616	39367	0.99%	0.110%
16	9.705	1119	1126	1134	rBV	368784	627561	15.84%	1.752%
17	10.040	1181	1183	1188	rVB	4342	6866	0.17%	0.019%
18	10.246	1210	1218	1229	rBV	520610	934638	23.59%	2.609%
19	10.622	1275	1282	1291	rVB	531919	938058	23.67%	2.618%
20	10.757	1297	1305	1317	rBV	466400	895238	22.59%	2.499%
21	12.220	1550	1554	1557	rBV4	7877	12470	0.31%	0.035%
22	12.808	1652	1654	1657	rVB4	4845	5290	0.13%	0.015%
23	13.701	1804	1806	1810	rVB3	4264	5523	0.14%	0.015%
24	13.877	1829	1836	1846	rBV	1153686	1641925	41.44%	4.583%
25	14.030	1859	1862	1866	rVB2	3925	5248	0.13%	0.015%
26	14.100	1871	1874	1877	rVB2	4815	6545	0.17%	0.018%
27	14.159	1877	1884	1892	rBV	1163363	1841538	46.47%	5.140%
28	14.470	1929	1937	1944	rBV	1055471	1593209	40.21%	4.447%
29	14.682	1967	1973	1984	rBV	417894	743454	18.76%	2.075%
30	15.463	2099	2106	2115	rBV	1687770	2493201	62.92%	6.959%
31	15.593	2122	2128	2139	rBV	496031	800758	20.21%	2.235%
32	15.716	2145	2149	2152	rVB3	7887	12031	0.30%	0.034%
33	15.975	2190	2193	2196	rVB2	5633	6125	0.15%	0.017%
34	16.033	2200	2203	2208	rBV3	4451	5893	0.15%	0.016%
35	16.257	2236	2241	2243	rBV3	6879	11280	0.28%	0.031%
36	16.903	2348	2351	2353	rVB	6332	5589	0.14%	0.016%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111324\
 Data File : BG063352.D
 Acq On : 13 Nov 2024 11:07
 Operator : RC/JU
 Sample : PB164920BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK920

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
 Title : SVOA CALIBRATION

37	16.950	2357	2359	2362	rBV4	5028	5328	0.13%	0.015%
38	17.220	2399	2405	2412	rBV	1557982	2254752	56.90%	6.294%
39	17.320	2415	2422	2433	rBV	2139515	3104361	78.34%	8.665%
40	17.896	2516	2520	2523	rBV5	10162	13592	0.34%	0.038%
41	18.107	2554	2556	2559	rVB3	6508	5489	0.14%	0.015%
42	18.337	2593	2595	2600	rVB3	6832	6704	0.17%	0.019%
43	18.595	2637	2639	2641	rBV3	7399	7141	0.18%	0.020%
44	18.713	2657	2659	2661	rBV2	5182	5771	0.15%	0.016%
45	18.807	2673	2675	2679	rBV5	5131	6131	0.15%	0.017%
46	18.942	2697	2698	2701	rBV3	7265	5234	0.13%	0.015%
47	19.183	2735	2739	2745	rVB3	33065	52633	1.33%	0.147%
48	19.253	2747	2751	2757	rBV	35223	52637	1.33%	0.147%
49	19.617	2807	2813	2824	rBV	2734342	3962583	100.00%	11.061%
50	19.952	2868	2870	2874	rVB4	8202	8827	0.22%	0.025%
51	21.474	3123	3129	3138	rVB	1808571	2715710	68.53%	7.581%
52	24.300	3600	3610	3622	rBV	1420098	3770126	95.14%	10.524%
53	24.506	3636	3645	3657	rVB	1044316	2773525	69.99%	7.742%




Sum of corrected areas: 35824707

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111324\
Data File : BG063352.D
Acq On : 13 Nov 2024 11:07
Operator : RC/JU
Sample : PB164920BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK920

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

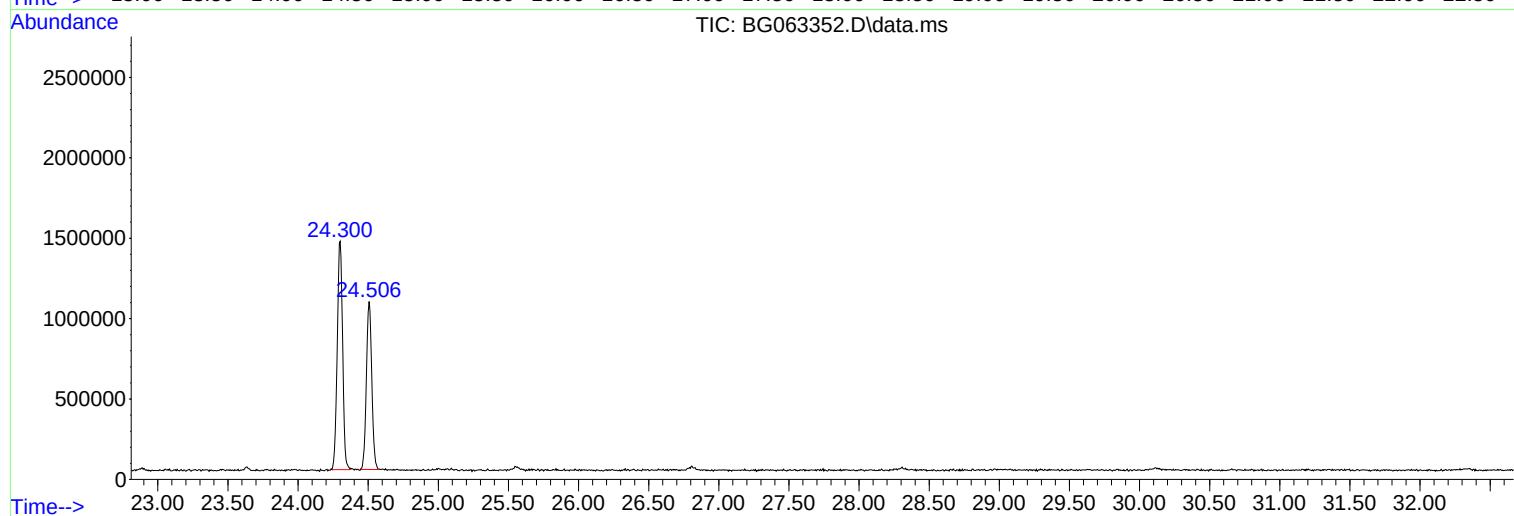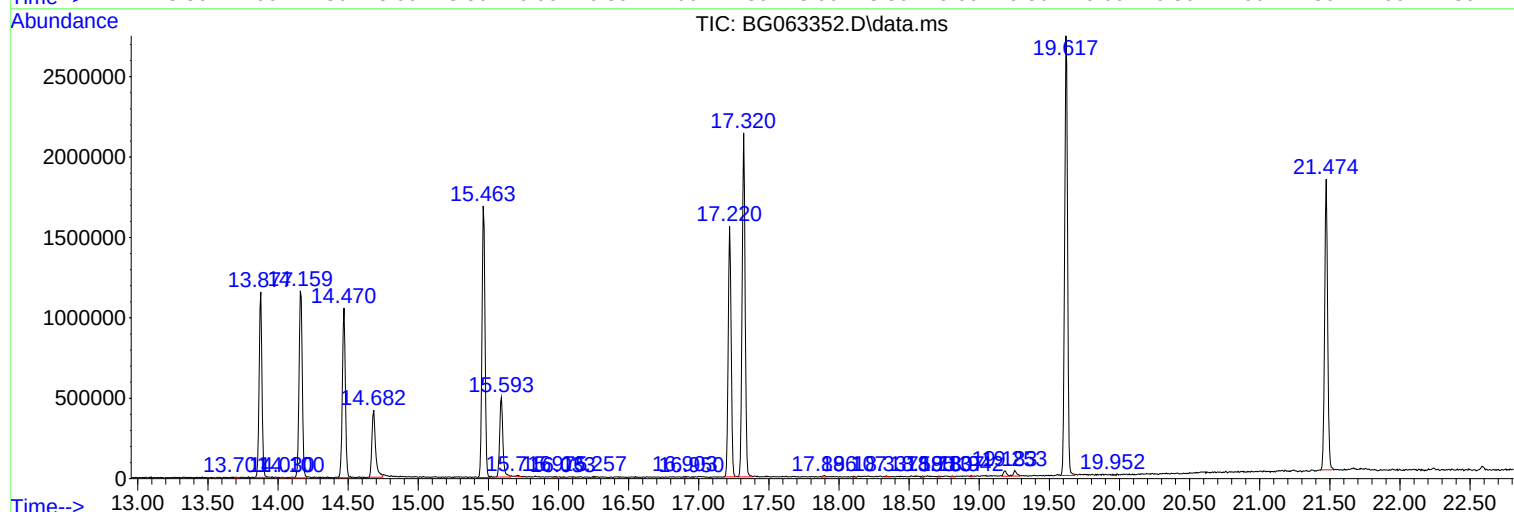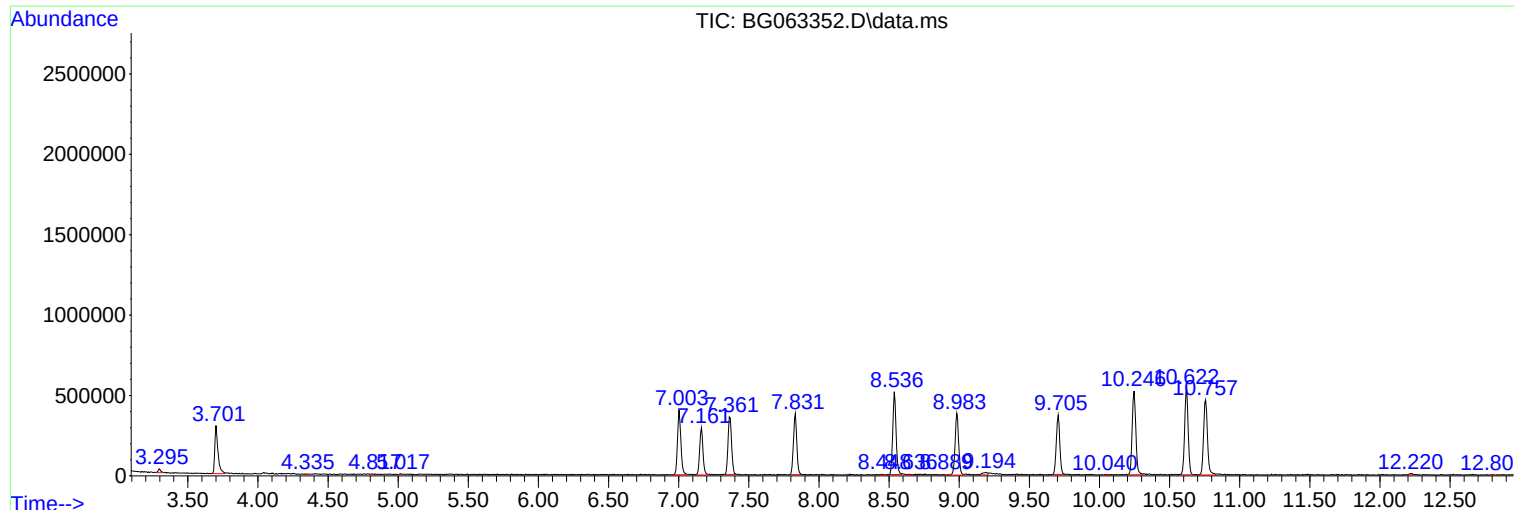

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111324\
Data File : BG063352.D
Acq On : 13 Nov 2024 11:07
Operator : RC/JU
Sample : PB164920BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK920

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111324\
Data File : BG063352.D
Acq On : 13 Nov 2024 11:07
Operator : RC/JU
Sample : PB164920BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK920

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc