

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111324\
 Data File : BG063353.D
 Acq On : 13 Nov 2024 11:45
 Operator : RC/JU
 Sample : PB164835BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK835

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG063353.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.305	33	37	41	rVB2	24327	36100	0.89%	0.100%
2	3.557	78	80	83	rBV4	5496	6804	0.17%	0.019%
3	3.704	101	105	120	rBV	315764	522559	12.82%	1.447%
4	4.039	160	162	165	rVB2	7304	7326	0.18%	0.020%
5	5.150	347	351	354	rVB5	4918	7291	0.18%	0.020%
6	5.267	370	371	375	rBV4	5205	6294	0.15%	0.017%
7	5.649	434	436	441	rVB4	5584	7682	0.19%	0.021%
8	6.272	538	542	545	rVB2	4471	7088	0.17%	0.020%
9	6.313	545	549	550	rBV3	4185	5699	0.14%	0.016%
10	6.936	650	655	657	rBV2	5465	6617	0.16%	0.018%
11	7.006	660	667	675	rBV2	403467	693866	17.02%	1.922%
12	7.165	688	694	702	rVB	300420	495473	12.15%	1.372%
13	7.365	721	728	735	rBV	399770	676765	16.60%	1.875%
14	7.418	735	737	743	rVB5	5308	5715	0.14%	0.016%
15	7.835	801	808	817	rVB	350434	597317	14.65%	1.655%
16	7.964	826	830	833	rVB3	3590	5739	0.14%	0.016%
17	8.105	850	854	858	rVB2	4697	7469	0.18%	0.021%
18	8.170	863	865	868	rBV2	5454	5509	0.14%	0.015%
19	8.540	920	928	936	rBV	529160	886475	21.75%	2.456%
20	8.986	995	1004	1011	rBV	391226	700286	17.18%	1.940%
21	9.180	1033	1037	1039	rBV3	9701	13796	0.34%	0.038%
22	9.415	1075	1077	1082	rVB4	4995	5688	0.14%	0.016%
23	9.703	1119	1126	1135	rBV	378722	671732	16.48%	1.861%
24	10.249	1211	1219	1229	rBV	524393	957997	23.50%	2.654%
25	10.620	1272	1282	1289	rBV	499668	879316	21.57%	2.436%
26	10.755	1298	1305	1316	rBV	479771	901268	22.11%	2.497%
27	11.354	1403	1407	1410	rVB2	4511	6169	0.15%	0.017%
28	11.642	1453	1456	1460	rBV2	3768	5822	0.14%	0.016%
29	11.906	1497	1501	1504	rBV2	6234	6913	0.17%	0.019%
30	13.510	1773	1774	1778	rBV	4499	5791	0.14%	0.016%
31	13.663	1798	1800	1804	rBV	3813	5755	0.14%	0.016%
32	13.875	1829	1836	1848	rVB	1179770	1682581	41.28%	4.661%
33	13.963	1848	1851	1854	rBV2	4605	5839	0.14%	0.016%
34	14.163	1878	1885	1893	rBV	1214740	1875579	46.01%	5.195%
35	14.468	1929	1937	1945	rBV	948578	1469113	36.04%	4.069%
36	14.627	1961	1964	1967	rBV2	5665	7862	0.19%	0.022%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111324\
 Data File : BG063353.D
 Acq On : 13 Nov 2024 11:45
 Operator : RC/JU
 Sample : PB164835BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK835

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
 Title : SVOA CALIBRATION

37	14.680	1967	1973	1985	rBV	437963	764879	18.76%	2.119%
38	14.926	2012	2015	2018	rVB4	5129	6654	0.16%	0.018%
39	15.132	2047	2050	2053	rVB4	5709	7377	0.18%	0.020%
40	15.467	2097	2107	2114	rBV	1658663	2547902	62.50%	7.058%
41	15.590	2121	2128	2140	rBV2	517648	827643	20.30%	2.293%
42	15.837	2166	2170	2174	rBV5	6856	8921	0.22%	0.025%
43	16.131	2217	2220	2223	rVB2	5923	6193	0.15%	0.017%
44	16.166	2223	2226	2229	rVB2	4670	6914	0.17%	0.019%
45	16.242	2236	2239	2246	rVB7	6511	10396	0.26%	0.029%
46	16.901	2347	2351	2355	rBV5	7060	8649	0.21%	0.024%
47	17.218	2398	2405	2413	rBV	1411632	2112887	51.83%	5.853%
48	17.318	2415	2422	2431	rVV2	2023027	3144846	77.15%	8.711%
49	17.735	2491	2493	2496	rVB5	4499	5499	0.13%	0.015%
50	17.776	2496	2500	2502	rBV5	6196	7137	0.18%	0.020%
51	17.888	2516	2519	2520	rBV2	7788	7809	0.19%	0.022%
52	19.180	2735	2739	2744	rBV2	36105	49261	1.21%	0.136%
53	19.251	2746	2751	2756	rBV	30194	53804	1.32%	0.149%
54	19.550	2797	2802	2806	rBV7	12871	23193	0.57%	0.064%
55	19.621	2807	2814	2823	rBV	2857617	4076457	100.00%	11.292%
56	20.261	2921	2923	2925	rBV3	8415	7174	0.18%	0.020%
57	20.385	2942	2944	2949	rVB6	11089	14964	0.37%	0.041%
58	21.472	3123	3129	3140	rBV2	1682117	2589475	63.52%	7.173%
59	24.298	3601	3610	3625	rVB	1546340	3948954	96.87%	10.939%
60	24.503	3636	3645	3659	rVB	1002769	2674838	65.62%	7.409%


Sum of corrected areas: 36101121

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111324\
Data File : BG063353.D
Acq On : 13 Nov 2024 11:45
Operator : RC/JU
Sample : PB164835BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK835

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

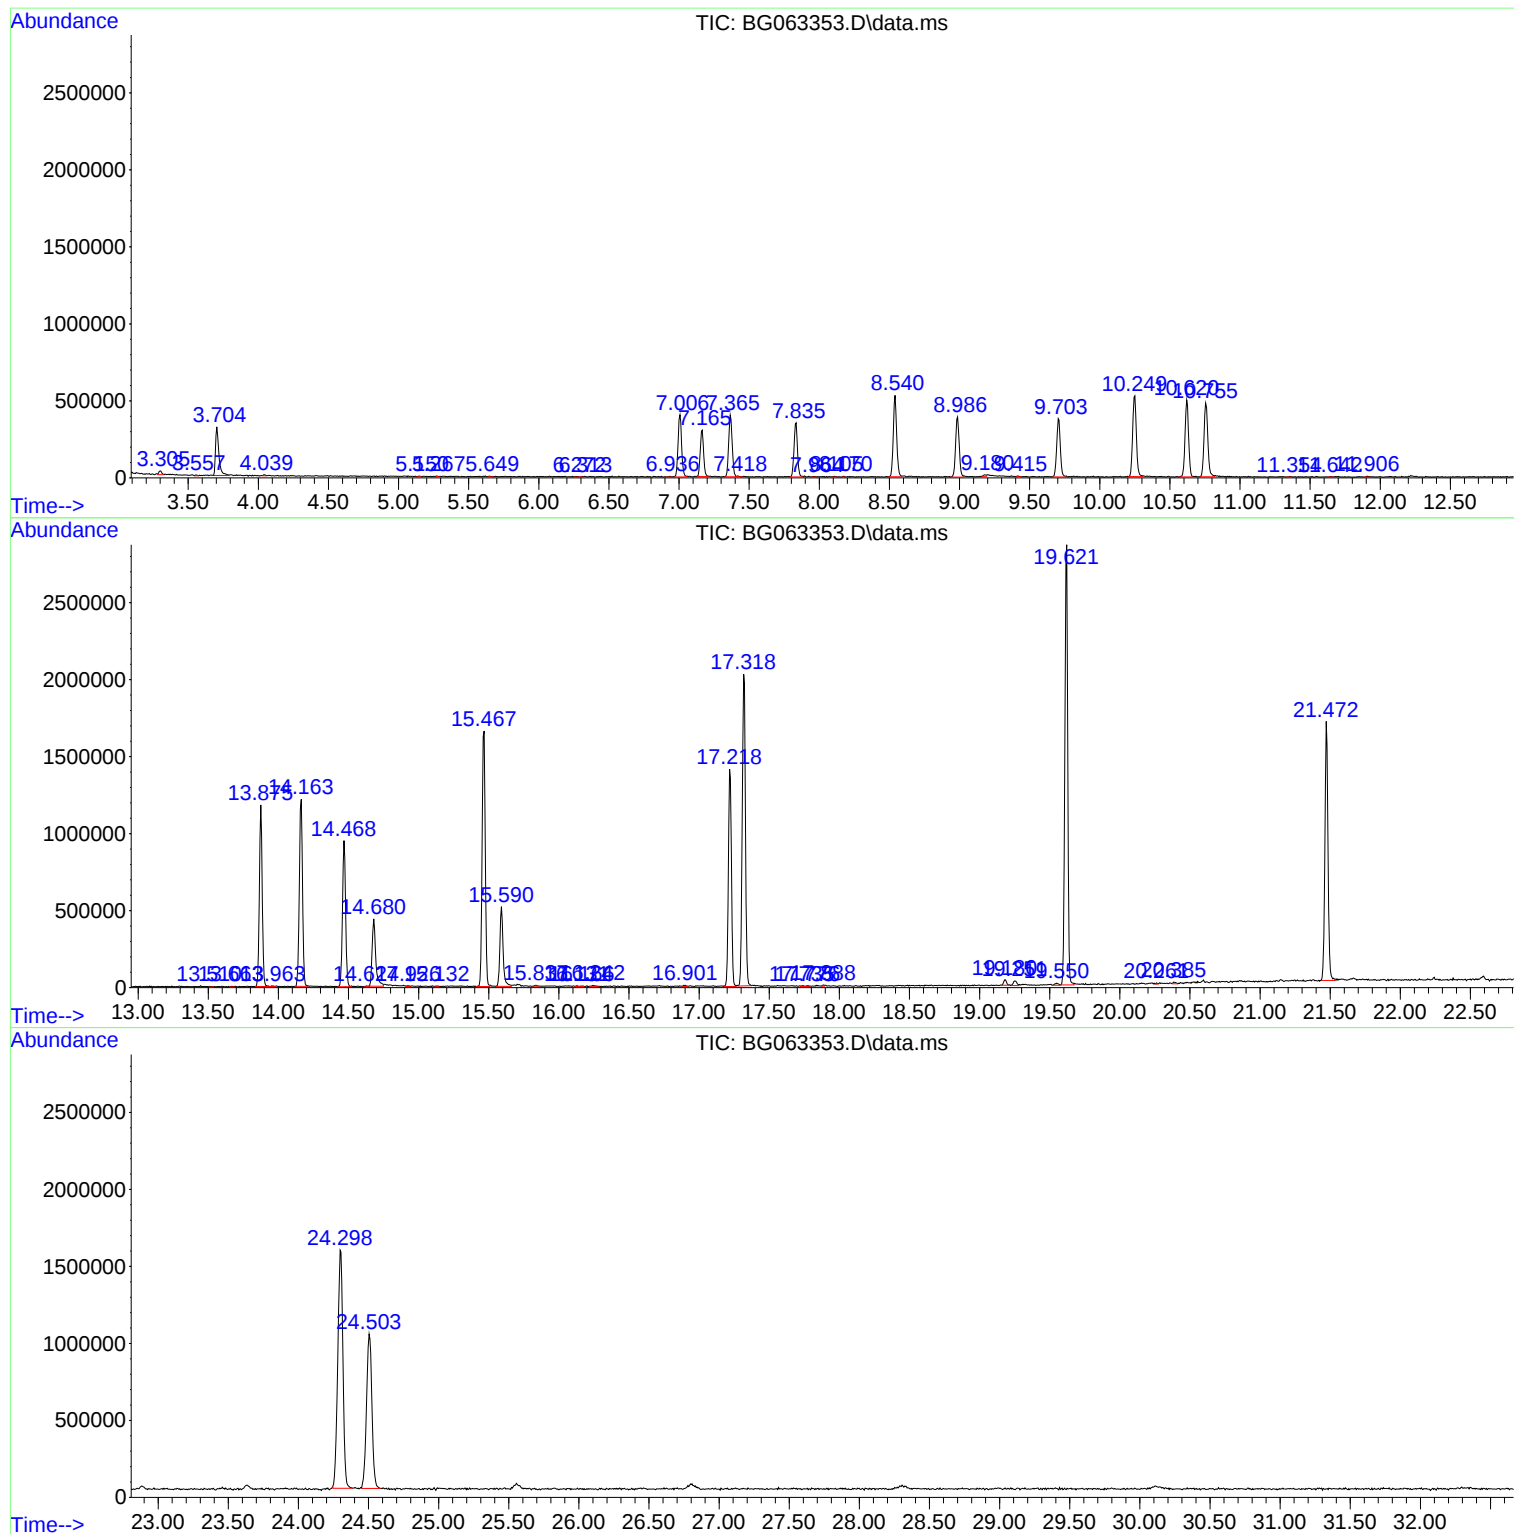

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111324\
Data File : BG063353.D
Acq On : 13 Nov 2024 11:45
Operator : RC/JU
Sample : PB164835BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK835

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111324\
Data File : BG063353.D
Acq On : 13 Nov 2024 11:45
Operator : RC/JU
Sample : PB164835BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK835

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc