

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111324\
 Data File : BG063369.D
 Acq On : 14 Nov 2024 00:24
 Operator : RC/JU
 Sample : P4801-22
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 GCPC2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG063369.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.301	33	36	41	rVB3	21071	27707	0.67%	0.079%
2	3.712	101	106	117	rBV	71192	124575	2.99%	0.354%
3	4.488	233	238	242	rBV4	7384	10955	0.26%	0.031%
4	4.547	242	248	250	rBV5	13818	18889	0.45%	0.054%
5	5.892	475	477	481	rBV3	5347	6387	0.15%	0.018%
6	7.009	660	667	674	rBV	126513	220131	5.28%	0.625%
7	7.161	687	693	703	rBV	301293	499123	11.98%	1.417%
8	7.367	721	728	737	rBV	361938	608984	14.62%	1.729%
9	7.831	799	807	814	rBV	394865	666271	15.99%	1.891%
10	8.536	921	927	937	rBV2	373924	664297	15.95%	1.886%
11	8.983	995	1003	1014	rBV	391416	721909	17.33%	2.049%
12	9.417	1071	1077	1081	rBV3	18644	29605	0.71%	0.084%
13	9.705	1119	1126	1132	rBV	367668	638341	15.32%	1.812%
14	9.799	1138	1142	1150	rVB7	3779	9493	0.23%	0.027%
15	10.246	1211	1218	1232	rBV	548909	990046	23.77%	2.811%
16	10.452	1251	1253	1259	rVB4	4230	5866	0.14%	0.017%
17	10.622	1274	1282	1292	rBV	523775	961773	23.09%	2.730%
18	10.757	1298	1305	1317	rBV	473311	864035	20.74%	2.453%
19	10.833	1317	1318	1323	rVB4	7364	7402	0.18%	0.021%
20	10.969	1339	1341	1344	rBV2	5384	6278	0.15%	0.018%
21	11.004	1344	1347	1350	rVV2	6679	8400	0.20%	0.024%
22	11.245	1384	1388	1389	rVB2	6586	6709	0.16%	0.019%
23	11.844	1486	1490	1491	rBV2	4713	5895	0.14%	0.017%
24	11.897	1496	1499	1506	rVB4	8099	14515	0.35%	0.041%
25	12.214	1550	1553	1556	rBV4	6014	7076	0.17%	0.020%
26	12.878	1663	1666	1669	rVB2	5148	7319	0.18%	0.021%
27	12.919	1669	1673	1674	rBV2	5462	6634	0.16%	0.019%
28	13.284	1731	1735	1738	rBV4	4358	6655	0.16%	0.019%
29	13.360	1743	1748	1749	rBV	5014	7879	0.19%	0.022%
30	13.871	1827	1835	1845	rBV	1121085	1649428	39.60%	4.682%
31	14.024	1858	1861	1865	rVB2	3775	6323	0.15%	0.018%
32	14.159	1874	1884	1894	rVB2	1181715	1870410	44.90%	5.310%
33	14.470	1930	1937	1944	rBV	986184	1550829	37.23%	4.403%
34	14.688	1968	1974	1982	rBV3	79615	171896	4.13%	0.488%
35	14.893	2006	2009	2011	rBV3	7410	8952	0.21%	0.025%
36	14.993	2023	2026	2029	rVB2	6887	8321	0.20%	0.024%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111324\
 Data File : BG063369.D
 Acq On : 14 Nov 2024 00:24
 Operator : RC/JU
 Sample : P4801-22
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 GCPC2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
 Title : SVOA CALIBRATION

37	15.322	2079	2082	2087	rVB6	7688	11489	0.28%	0.033%
38	15.463	2099	2106	2114	rBV	1720207	2554639	61.33%	7.252%
39	15.593	2117	2128	2137	rBV	588770	947897	22.76%	2.691%
40	15.698	2143	2146	2147	rBV2	9976	7571	0.18%	0.021%
41	15.828	2162	2168	2173	rBV2	44877	70309	1.69%	0.200%
42	16.186	2226	2229	2233	rVB5	6612	7378	0.18%	0.021%
43	16.650	2303	2308	2309	rBV3	6144	7080	0.17%	0.020%
44	16.897	2347	2350	2351	rBV2	7073	6944	0.17%	0.020%
45	17.144	2387	2392	2399	rBV3	40192	56764	1.36%	0.161%
46	17.220	2399	2405	2412	rBV	1481608	2188348	52.53%	6.212%
47	17.320	2415	2422	2432	rVB	2223071	3216571	77.22%	9.131%
48	17.890	2516	2519	2524	rVB6	11007	15863	0.38%	0.045%
49	17.990	2534	2536	2538	rBV2	5725	5937	0.14%	0.017%
50	18.125	2554	2559	2566	rBV5	45641	86064	2.07%	0.244%
51	18.307	2588	2590	2595	rVB5	8274	9898	0.24%	0.028%
52	18.413	2606	2608	2610	rBV3	8576	7774	0.19%	0.022%
53	18.548	2627	2631	2635	rBV5	22875	31895	0.77%	0.091%
54	18.759	2664	2667	2669	rBV4	6946	8406	0.20%	0.024%
55	19.183	2733	2739	2743	rBV3	38760	60158	1.44%	0.171%
56	19.253	2746	2751	2754	rBV2	36159	54072	1.30%	0.154%
57	19.282	2754	2756	2761	rVB6	24333	29705	0.71%	0.084%
58	19.406	2775	2777	2781	rVB5	12673	9317	0.22%	0.026%
59	19.617	2807	2813	2821	rBV	2989603	4165585	100.00%	11.826%
60	21.139	3068	3072	3080	rBV8	52040	89642	2.15%	0.254%
61	21.474	3122	3129	3138	rBV	1637309	2587475	62.12%	7.345%
62	24.300	3600	3610	3620	rBV	1513426	3899399	93.61%	11.070%
63	24.506	3635	3645	3659	rVB	1002739	2669903	64.09%	7.579%


Sum of corrected areas: 35225391

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111324\
Data File : BG063369.D
Acq On : 14 Nov 2024 00:24
Operator : RC/JU
Sample : P4801-22
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
GCPC2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

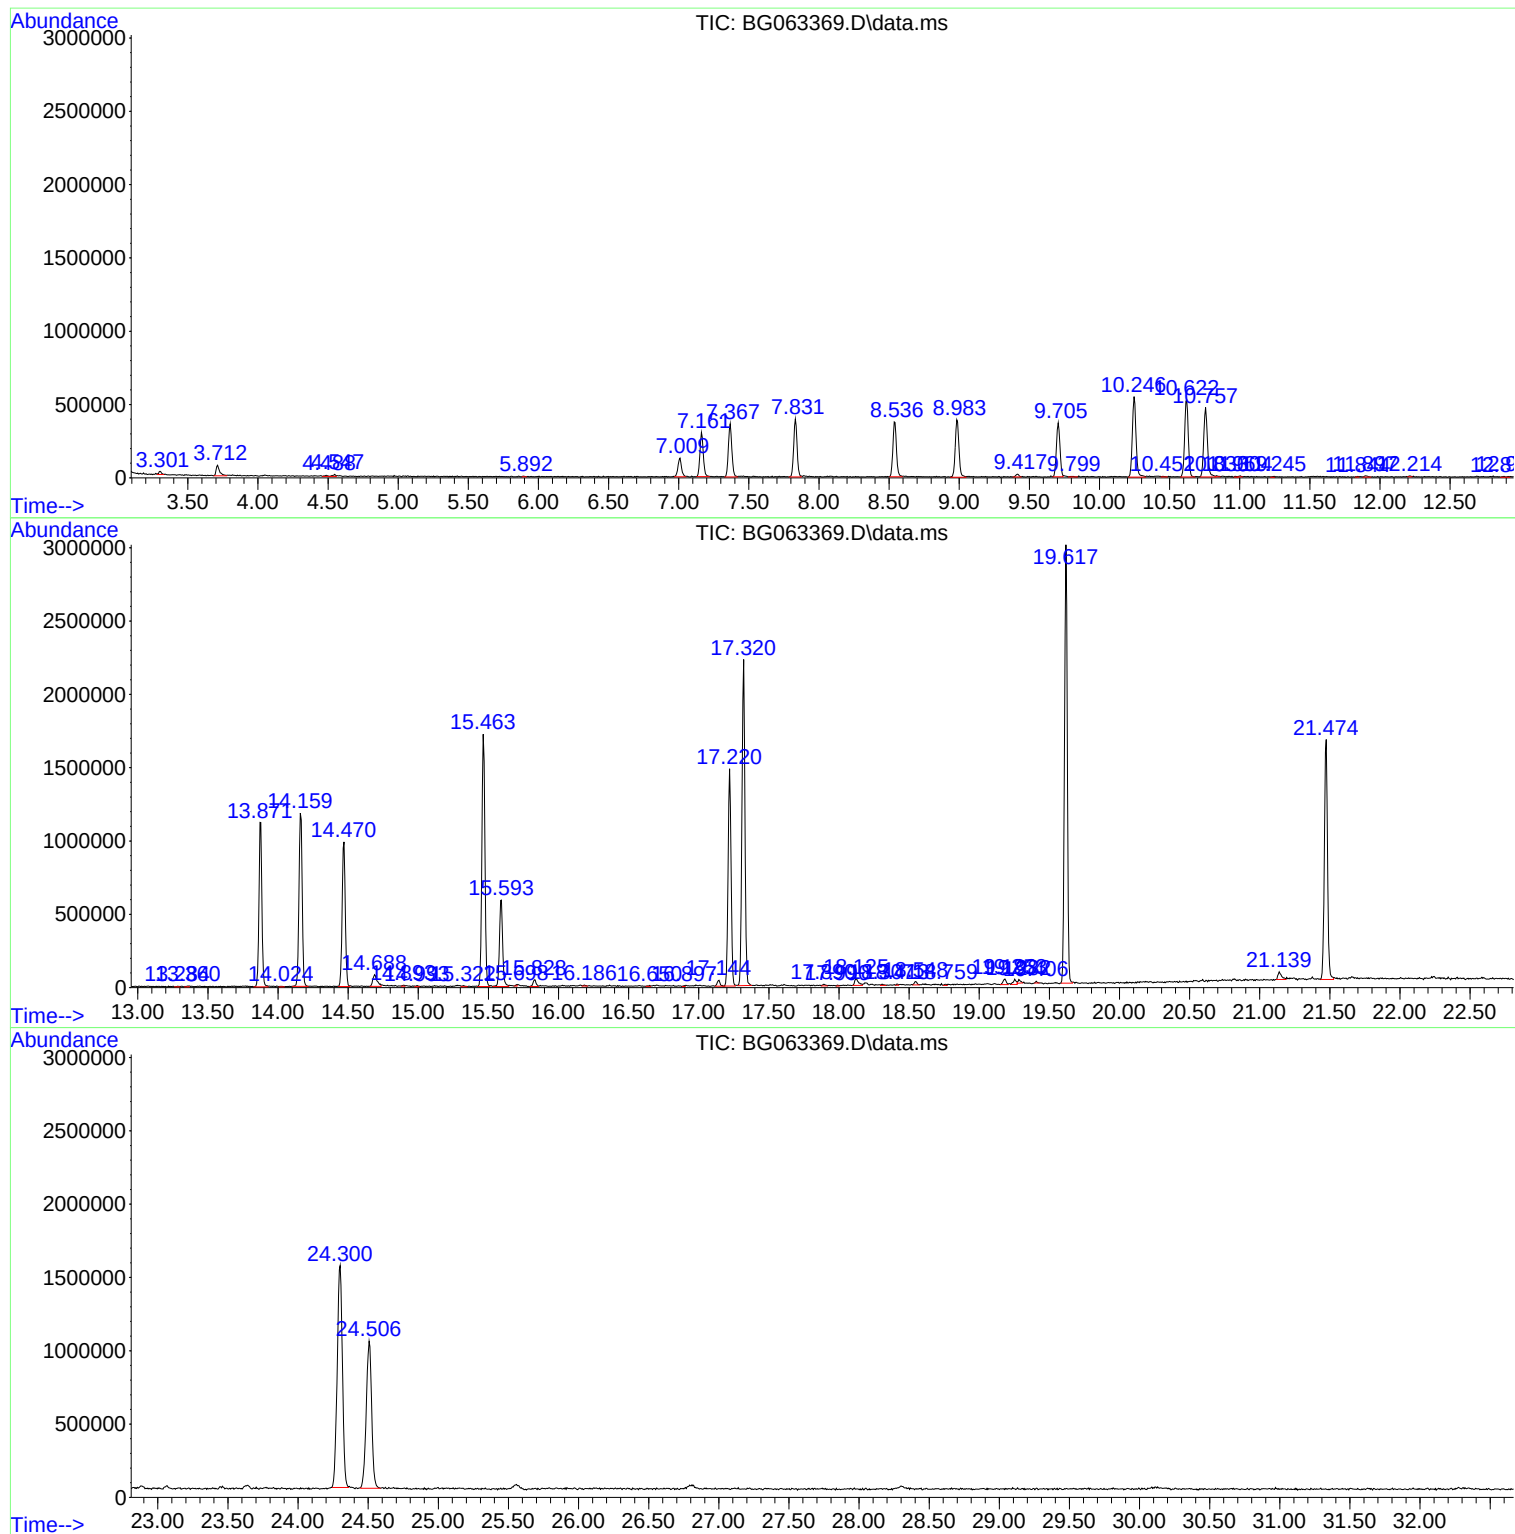

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111324\
Data File : BG063369.D
Acq On : 14 Nov 2024 00:24
Operator : RC/JU
Sample : P4801-22
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
GCPC2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111324\
Data File : BG063369.D
Acq On : 14 Nov 2024 00:24
Operator : RC/JU
Sample : P4801-22
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
GCPC2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc