

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111324\
 Data File : BG063370.D
 Acq On : 14 Nov 2024 1:01
 Operator : RC/JU
 Sample : P4802-01
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 GCPC3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG063370.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.300	28	36	42	rVB8	21555	55123	1.25%	0.155%
2	3.706	101	105	114	rBV	80012	130108	2.95%	0.366%
3	4.041	158	162	165	rVB4	7782	10595	0.24%	0.030%
4	4.399	222	223	227	rBV3	5432	6907	0.16%	0.019%
5	4.546	245	248	251	rBV5	7471	10555	0.24%	0.030%
6	5.363	383	387	388	rVB2	5585	6082	0.14%	0.017%
7	6.197	525	529	531	rVB4	6425	9080	0.21%	0.026%
8	7.002	660	666	675	rBV	131819	239186	5.43%	0.673%
9	7.160	688	693	703	rBV	298630	480834	10.92%	1.354%
10	7.366	721	728	739	rBV	343142	578076	13.13%	1.628%
11	7.830	800	807	815	rBV	364470	615717	13.98%	1.734%
12	8.541	919	928	935	rBV	401354	694681	15.78%	1.956%
13	8.982	997	1003	1011	rBV	383856	677620	15.39%	1.908%
14	9.705	1118	1126	1134	rBV	366665	646002	14.67%	1.819%
15	10.245	1211	1218	1228	rBV2	518528	950872	21.59%	2.677%
16	10.357	1234	1237	1240	rBV3	6453	7215	0.16%	0.020%
17	10.621	1275	1282	1290	rVB	520472	920004	20.89%	2.590%
18	10.756	1297	1305	1321	rBV	432913	817316	18.56%	2.301%
19	11.908	1496	1501	1504	rBV3	10227	11804	0.27%	0.033%
20	12.225	1549	1555	1559	rBV5	8809	20907	0.47%	0.059%
21	12.636	1622	1625	1630	rVB3	5184	9982	0.23%	0.028%
22	13.876	1830	1836	1844	rVB	1262357	1777365	40.36%	5.004%
23	14.158	1876	1884	1893	rBV2	1173852	1907019	43.31%	5.369%
24	14.470	1931	1937	1946	rVB	958076	1466864	33.31%	4.130%
25	14.687	1967	1974	1984	rBV3	85457	181557	4.12%	0.511%
26	14.887	2006	2008	2011	rBV3	5611	7700	0.17%	0.022%
27	15.463	2098	2106	2114	rBV	1855062	2743954	62.32%	7.726%
28	15.592	2122	2128	2140	rBV	672002	1025165	23.28%	2.886%
29	15.703	2144	2147	2152	rVB4	14034	18639	0.42%	0.052%
30	16.032	2199	2203	2206	rBV3	4610	7453	0.17%	0.021%
31	16.156	2222	2224	2226	rBV3	7553	6406	0.15%	0.018%
32	16.238	2235	2238	2244	rBV6	5971	8329	0.19%	0.023%
33	16.643	2305	2307	2309	rBV3	4981	6519	0.15%	0.018%
34	16.685	2311	2314	2317	rBV4	7468	10899	0.25%	0.031%
35	16.896	2348	2350	2354	rBV4	5829	6302	0.14%	0.018%
36	17.143	2389	2392	2399	rVB6	10867	15526	0.35%	0.044%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111324\
 Data File : BG063370.D
 Acq On : 14 Nov 2024 1:01
 Operator : RC/JU
 Sample : P4802-01
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 GCPC3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
 Title : SVOA CALIBRATION

37	17.219	2399	2405	2415	rBV	1417779	2069011	46.99%	5.825%
38	17.319	2415	2422	2434	rVV	2382508	3485578	79.16%	9.814%
39	17.836	2508	2510	2514	rBV4	4021	6113	0.14%	0.017%
40	17.889	2517	2519	2523	rVB4	15804	18835	0.43%	0.053%
41	17.965	2529	2532	2534	rBV3	6078	8319	0.19%	0.023%
42	18.054	2544	2547	2550	rBV3	6100	7675	0.17%	0.022%
43	18.124	2554	2559	2568	rBV6	39821	84162	1.91%	0.237%
44	18.336	2592	2595	2600	rBV6	10048	14832	0.34%	0.042%
45	18.547	2630	2631	2637	rVB6	12089	14089	0.32%	0.040%
46	18.618	2641	2643	2645	rVV2	8930	10418	0.24%	0.029%
47	18.665	2647	2651	2655	rBV5	5540	10064	0.23%	0.028%
48	18.876	2683	2687	2690	rVB5	7118	9421	0.21%	0.027%
49	19.182	2735	2739	2746	rVB3	36092	57201	1.30%	0.161%
50	19.252	2747	2751	2756	rBV3	36397	60126	1.37%	0.169%
51	19.405	2772	2777	2781	rBV8	19350	33476	0.76%	0.094%
52	19.616	2807	2813	2821	rBV	3051098	4403355	100.00%	12.398%
53	21.473	3123	3129	3138	rVB	1576726	2417641	54.90%	6.807%
54	24.299	3599	3610	3622	rBV	1644261	4207151	95.54%	11.846%
55	24.505	3636	3645	3657	rVB	980515	2510893	57.02%	7.070%




Sum of corrected areas: 35516723

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111324\
Data File : BG063370.D
Acq On : 14 Nov 2024 1:01
Operator : RC/JU
Sample : P4802-01
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
GCPC3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

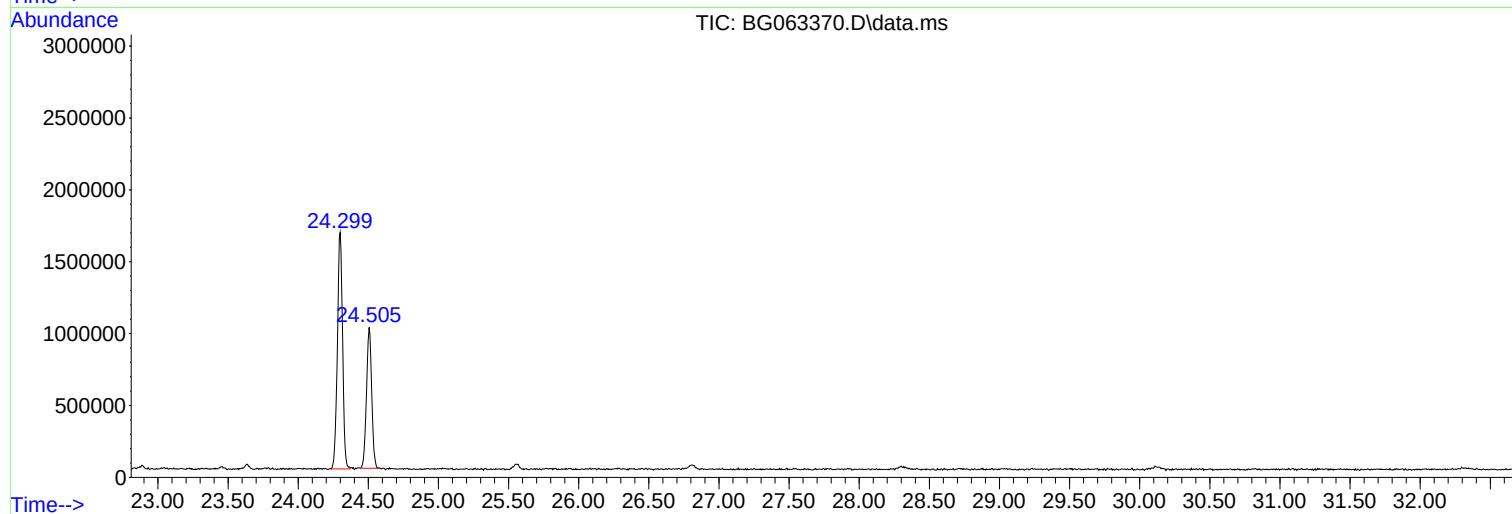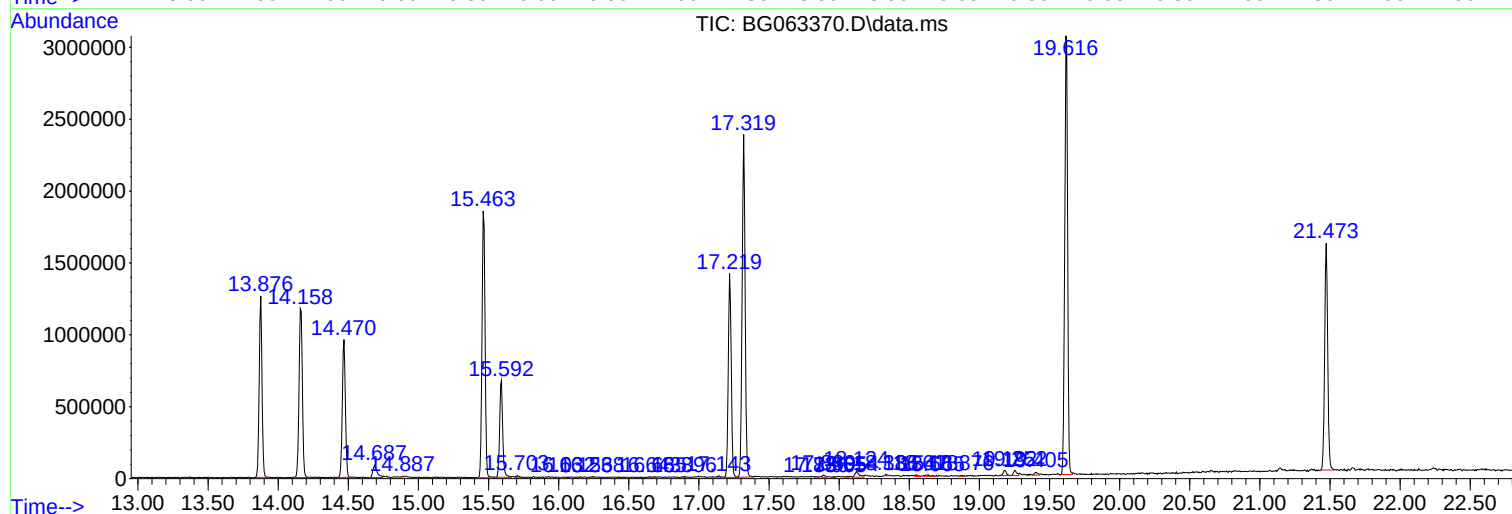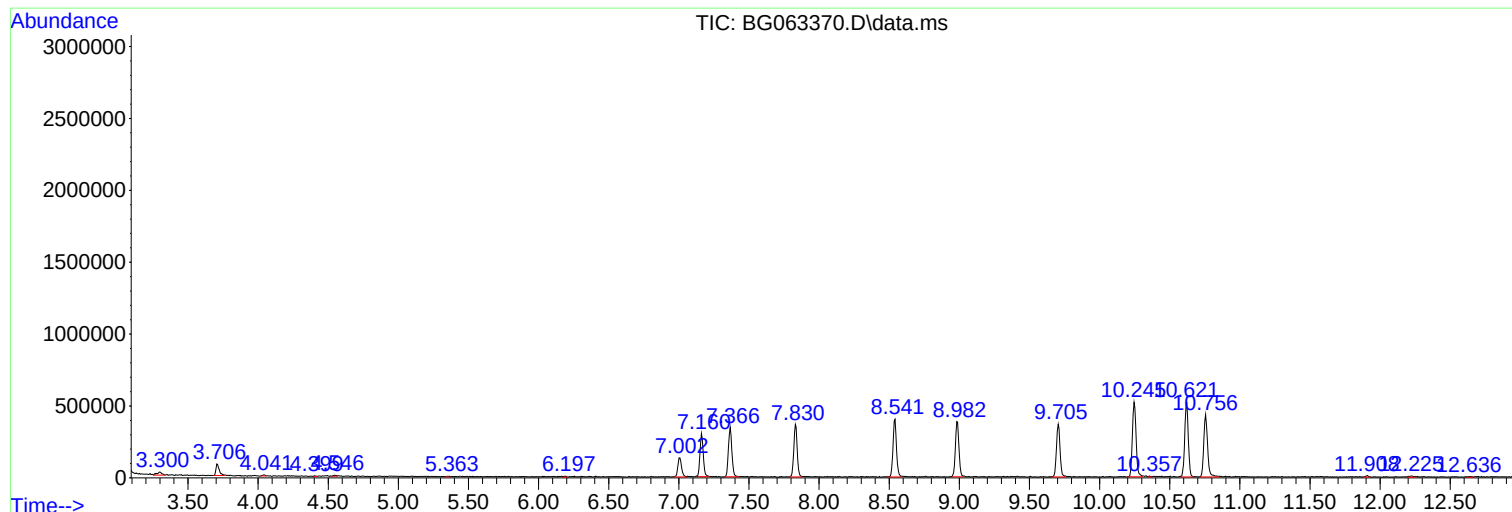

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111324\
Data File : BG063370.D
Acq On : 14 Nov 2024 1:01
Operator : RC/JU
Sample : P4802-01
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
GCPC3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111324\
Data File : BG063370.D
Acq On : 14 Nov 2024 1:01
Operator : RC/JU
Sample : P4802-01
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
GCPC3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc