

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111324\
 Data File : BG063388.D
 Acq On : 14 Nov 2024 13:00
 Operator : RC/JU
 Sample : PB164836BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK836

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG063388.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.302	33	36	43	rVB	28827	37434	0.94%	0.102%
2	3.537	75	76	79	rBV2	7289	5651	0.14%	0.015%
3	3.708	100	105	117	rBV	340413	571210	14.41%	1.550%
4	4.048	158	163	165	rVB3	11724	16372	0.41%	0.044%
5	4.483	234	237	240	rBV4	4915	7438	0.19%	0.020%
6	5.993	493	494	497	rBV2	4722	5612	0.14%	0.015%
7	6.064	505	506	512	rVB5	4573	6216	0.16%	0.017%
8	7.004	658	666	677	rBV	427306	742674	18.74%	2.016%
9	7.162	687	693	702	rVB	319733	521960	13.17%	1.417%
10	7.368	719	728	735	rBV	411608	708051	17.86%	1.922%
11	7.556	757	760	763	rBV2	4317	6013	0.15%	0.016%
12	7.832	799	807	815	rBV	390674	644928	16.27%	1.751%
13	7.926	819	823	826	rBV4	4131	6824	0.17%	0.019%
14	8.537	920	927	937	rBV	534873	958926	24.19%	2.603%
15	8.984	996	1003	1012	rBV2	420051	719315	18.15%	1.952%
16	9.184	1032	1037	1038	rBV	12249	13366	0.34%	0.036%
17	9.706	1118	1126	1135	rBV	380621	691874	17.46%	1.878%
18	9.812	1140	1144	1145	rBV2	4458	5788	0.15%	0.016%
19	10.247	1210	1218	1229	rBV2	556153	1026497	25.90%	2.786%
20	10.517	1259	1264	1267	rBV3	3766	5741	0.14%	0.016%
21	10.623	1274	1282	1290	rVB	545763	963207	24.30%	2.614%
22	10.758	1298	1305	1313	rBV	497477	934524	23.58%	2.537%
23	10.976	1337	1342	1343	rBV5	4889	7168	0.18%	0.019%
24	11.886	1494	1497	1501	rVB2	3631	5827	0.15%	0.016%
25	12.227	1551	1555	1560	rBV6	9486	16292	0.41%	0.044%
26	12.820	1651	1656	1660	rBV3	6286	12375	0.31%	0.034%
27	13.144	1706	1711	1714	rVB	4541	6754	0.17%	0.018%
28	13.878	1829	1836	1844	rBV	1189919	1681538	42.43%	4.564%
29	14.160	1878	1884	1891	rBV	1228016	1935314	48.83%	5.253%
30	14.471	1929	1937	1946	rBV	1026199	1582654	39.93%	4.296%
31	14.683	1967	1973	1984	rBV	402251	751904	18.97%	2.041%
32	15.464	2099	2106	2115	rBV	1759420	2603278	65.68%	7.066%
33	15.594	2122	2128	2143	rBV	556626	896504	22.62%	2.433%
34	15.705	2143	2147	2151	rVB6	10481	16140	0.41%	0.044%
35	16.034	2198	2203	2205	rBV2	4999	6729	0.17%	0.018%
36	16.199	2229	2231	2236	rVB3	5462	5643	0.14%	0.015%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111324\
 Data File : BG063388.D
 Acq On : 14 Nov 2024 13:00
 Operator : RC/JU
 Sample : PB164836BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK836

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
 Title : SVOA CALIBRATION

37	16.246	2238	2239	2243	rVB2	6033	6575	0.17%	0.018%
38	16.510	2281	2284	2288	rBV3	4146	6665	0.17%	0.018%
39	16.640	2302	2306	2308	rBV2	4839	7319	0.18%	0.020%
40	17.221	2399	2405	2414	rBV	1513770	2206431	55.67%	5.989%
41	17.321	2415	2422	2433	rVB2	2114326	3166553	79.89%	8.595%
42	17.527	2453	2457	2460	rVB5	4192	5683	0.14%	0.015%
43	17.568	2460	2464	2467	rBV4	4613	5768	0.15%	0.016%
44	17.891	2515	2519	2520	rBV3	8756	7195	0.18%	0.020%
45	19.184	2735	2739	2746	rVB2	30387	48333	1.22%	0.131%
46	19.254	2746	2751	2761	rBV	33970	52997	1.34%	0.144%
47	19.618	2807	2813	2825	rBV	2927942	3963436	100.00%	10.758%
48	19.947	2865	2869	2870	rBV4	7428	8441	0.21%	0.023%
49	20.212	2910	2914	2915	rBV4	7998	9632	0.24%	0.026%
50	21.475	3122	3129	3139	rBV2	1697244	2688646	67.84%	7.298%
51	24.301	3600	3610	3621	rVB	1486744	3812042	96.18%	10.347%
52	24.507	3636	3645	3656	rVB2	1003392	2717578	68.57%	7.376%




Sum of corrected areas: 36841035

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111324\
Data File : BG063388.D
Acq On : 14 Nov 2024 13:00
Operator : RC/JU
Sample : PB164836BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK836

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

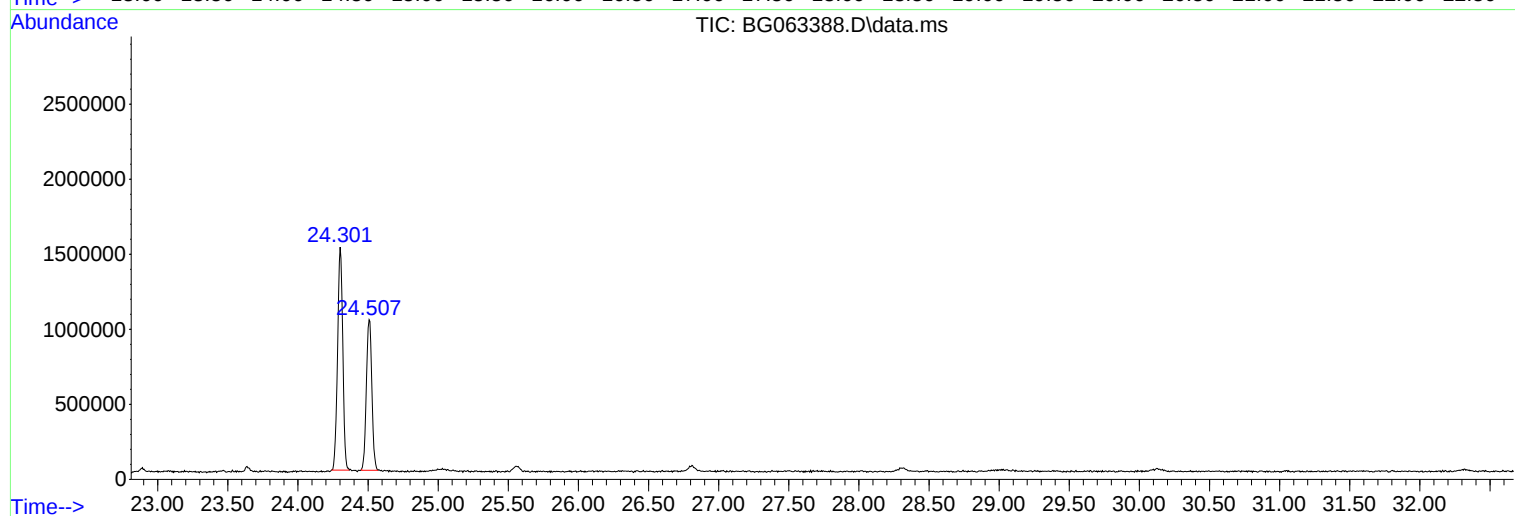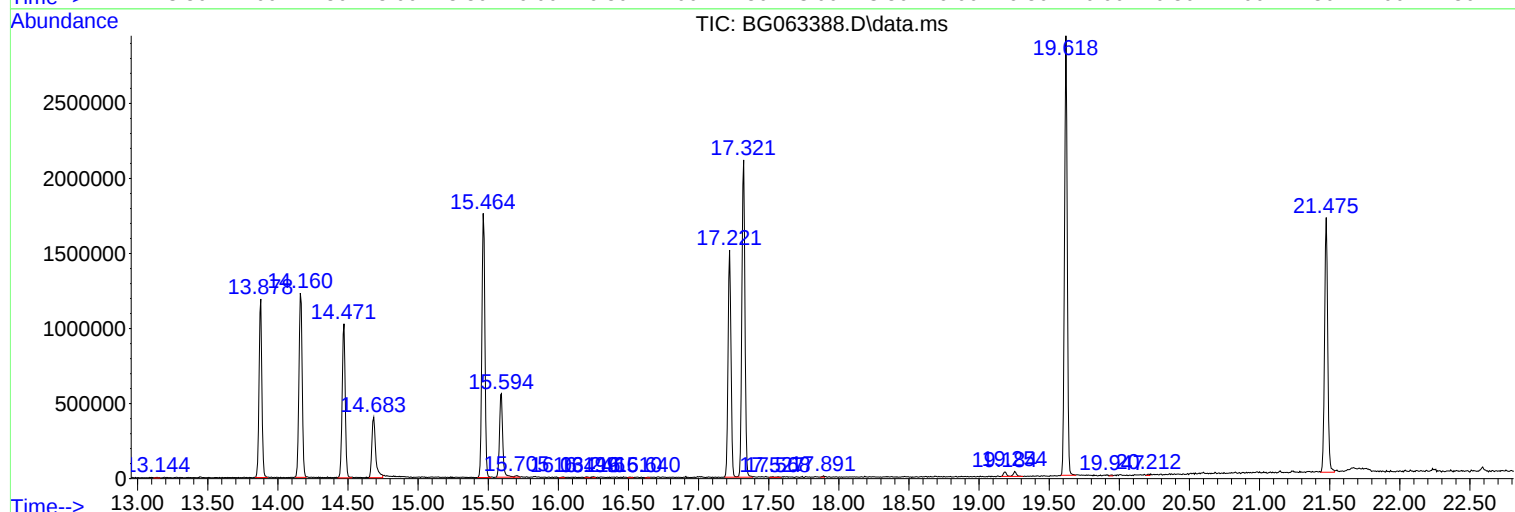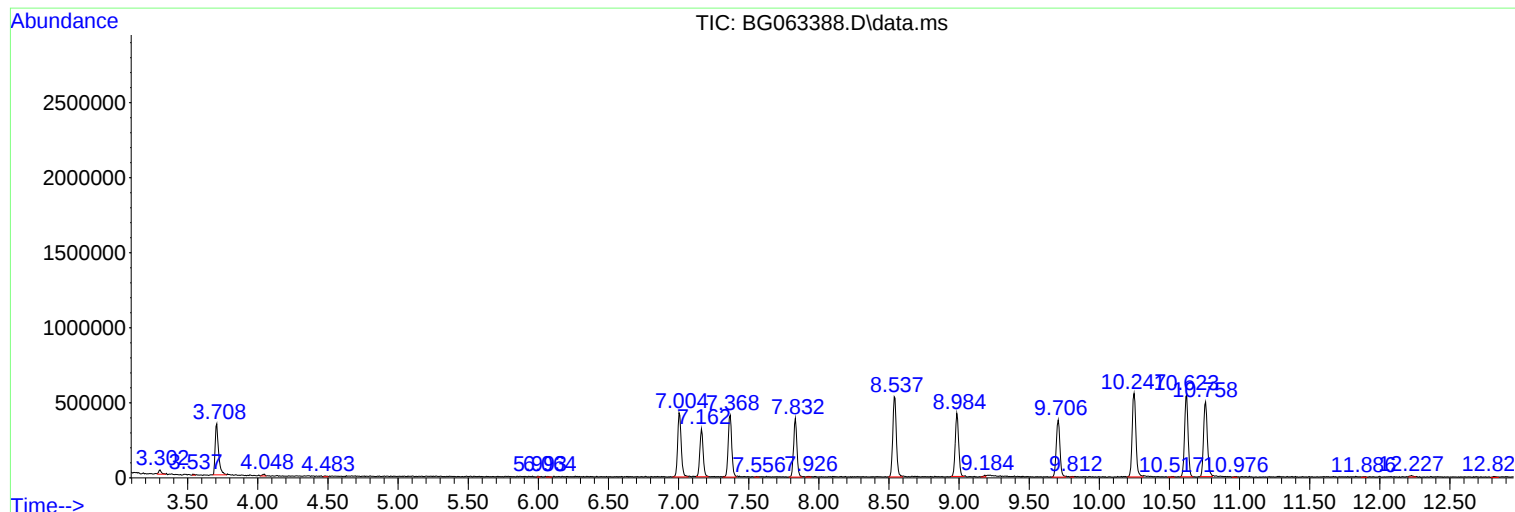

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111324\
Data File : BG063388.D
Acq On : 14 Nov 2024 13:00
Operator : RC/JU
Sample : PB164836BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK836

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111324\
Data File : BG063388.D
Acq On : 14 Nov 2024 13:00
Operator : RC/JU
Sample : PB164836BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK836

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc