

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111324\
 Data File : BG063389.D
 Acq On : 14 Nov 2024 13:38
 Operator : RC/JU
 Sample : PB164838BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK838

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG063389.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.298	34	36	42	rVB3	25837	36650	0.96%	0.101%
2	3.545	76	78	80	rVB2	7441	7147	0.19%	0.020%
3	3.704	101	105	123	rVB	353952	621212	16.20%	1.711%
4	3.909	138	140	145	rBV4	5101	6296	0.16%	0.017%
5	4.855	298	301	303	rBV3	4817	5133	0.13%	0.014%
6	4.908	308	310	313	rBV3	4028	5387	0.14%	0.015%
7	5.983	490	493	496	rVB3	5184	5943	0.15%	0.016%
8	6.136	513	519	520	rBV3	4615	7457	0.19%	0.021%
9	7.006	660	667	675	rBV	458420	779630	20.33%	2.147%
10	7.076	678	679	684	rVB3	6319	6533	0.17%	0.018%
11	7.164	687	694	702	rBV	353223	570690	14.88%	1.572%
12	7.364	722	728	736	rVB	434467	741503	19.33%	2.042%
13	7.834	800	808	817	rBV	381796	647131	16.87%	1.782%
14	8.539	920	928	937	rBV	595059	995442	25.95%	2.741%
15	8.721	956	959	961	rBV3	4868	6986	0.18%	0.019%
16	8.986	995	1004	1018	rBV	408999	737433	19.23%	2.031%
17	9.191	1034	1039	1040	rBV3	9765	12691	0.33%	0.035%
18	9.221	1042	1044	1047	rVV4	7367	8764	0.23%	0.024%
19	9.703	1119	1126	1138	rBV	388896	699072	18.22%	1.925%
20	9.820	1143	1146	1148	rVB2	6912	7086	0.18%	0.020%
21	10.249	1210	1219	1228	rBV	567358	1032012	26.90%	2.842%
22	10.390	1240	1243	1246	rBV3	4537	6083	0.16%	0.017%
23	10.619	1275	1282	1292	rVB	547589	944817	24.63%	2.602%
24	10.754	1299	1305	1315	rBV	513192	933876	24.35%	2.572%
25	11.013	1346	1349	1352	rBV2	4839	7194	0.19%	0.020%
26	11.154	1371	1373	1376	rBV	4507	5355	0.14%	0.015%
27	11.236	1385	1387	1390	rBV2	4874	5551	0.14%	0.015%
28	12.217	1550	1554	1556	rBV3	10863	15256	0.40%	0.042%
29	13.874	1828	1836	1848	rBV	1186147	1720794	44.86%	4.739%
30	14.162	1878	1885	1894	rVB	1229482	1967631	51.30%	5.419%
31	14.468	1930	1937	1948	rVB	971981	1517231	39.55%	4.178%
32	14.679	1966	1973	1984	rBV	384490	726519	18.94%	2.001%
33	14.844	2000	2001	2004	rVB3	6776	5358	0.14%	0.015%
34	14.896	2004	2010	2011	rBV5	6367	10359	0.27%	0.029%
35	15.466	2099	2107	2115	rBV	1727221	2608186	68.00%	7.183%
36	15.590	2122	2128	2140	rBV2	567359	876564	22.85%	2.414%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111324\
 Data File : BG063389.D
 Acq On : 14 Nov 2024 13:38
 Operator : RC/JU
 Sample : PB164838BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK838

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
 Title : SVOA CALIBRATION

37	15.831	2167	2169	2175	rVB3	6155	6825	0.18%	0.019%
38	15.919	2180	2184	2185	rVB	6449	5923	0.15%	0.016%
39	15.948	2185	2189	2192	rBV2	6413	8591	0.22%	0.024%
40	16.495	2279	2282	2284	rBV2	5277	5473	0.14%	0.015%
41	16.753	2324	2326	2330	rBV2	4711	6656	0.17%	0.018%
42	17.012	2365	2370	2371	rBV	5246	5856	0.15%	0.016%
43	17.223	2399	2406	2412	rBV	1389875	2060524	53.72%	5.675%
44	17.317	2415	2422	2429	rBV2	2056147	3083804	80.40%	8.493%
45	17.546	2458	2461	2467	rBV6	3613	5496	0.14%	0.015%
46	17.664	2480	2481	2486	rVB5	5567	6212	0.16%	0.017%
47	17.899	2517	2521	2523	rVB5	6750	8449	0.22%	0.023%
48	18.116	2555	2558	2561	rBV2	5128	6884	0.18%	0.019%
49	18.551	2631	2632	2637	rVB2	6563	8821	0.23%	0.024%
50	18.880	2685	2688	2690	rBV3	5095	5192	0.14%	0.014%
51	19.003	2707	2709	2713	rVB3	5340	6162	0.16%	0.017%
52	19.186	2734	2740	2744	rBV3	33779	47546	1.24%	0.131%
53	19.256	2748	2752	2759	rVB	31224	47104	1.23%	0.130%
54	19.620	2807	2814	2820	rBV	2676315	3835790	100.00%	10.564%
55	20.484	2959	2961	2962	rBV2	8235	5468	0.14%	0.015%
56	21.060	3056	3059	3061	rBV3	11981	16418	0.43%	0.045%
57	21.477	3122	3130	3141	rBV	1503935	2481907	64.70%	6.835%
58	23.445	3463	3465	3470	rBV6	15803	27085	0.71%	0.075%
59	24.303	3601	3611	3626	rVB	1462136	3759219	98.00%	10.353%
60	24.509	3636	3646	3657	rBV	994220	2569149	66.98%	7.075%


Sum of corrected areas: 36311526

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111324\
Data File : BG063389.D
Acq On : 14 Nov 2024 13:38
Operator : RC/JU
Sample : PB164838BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK838

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

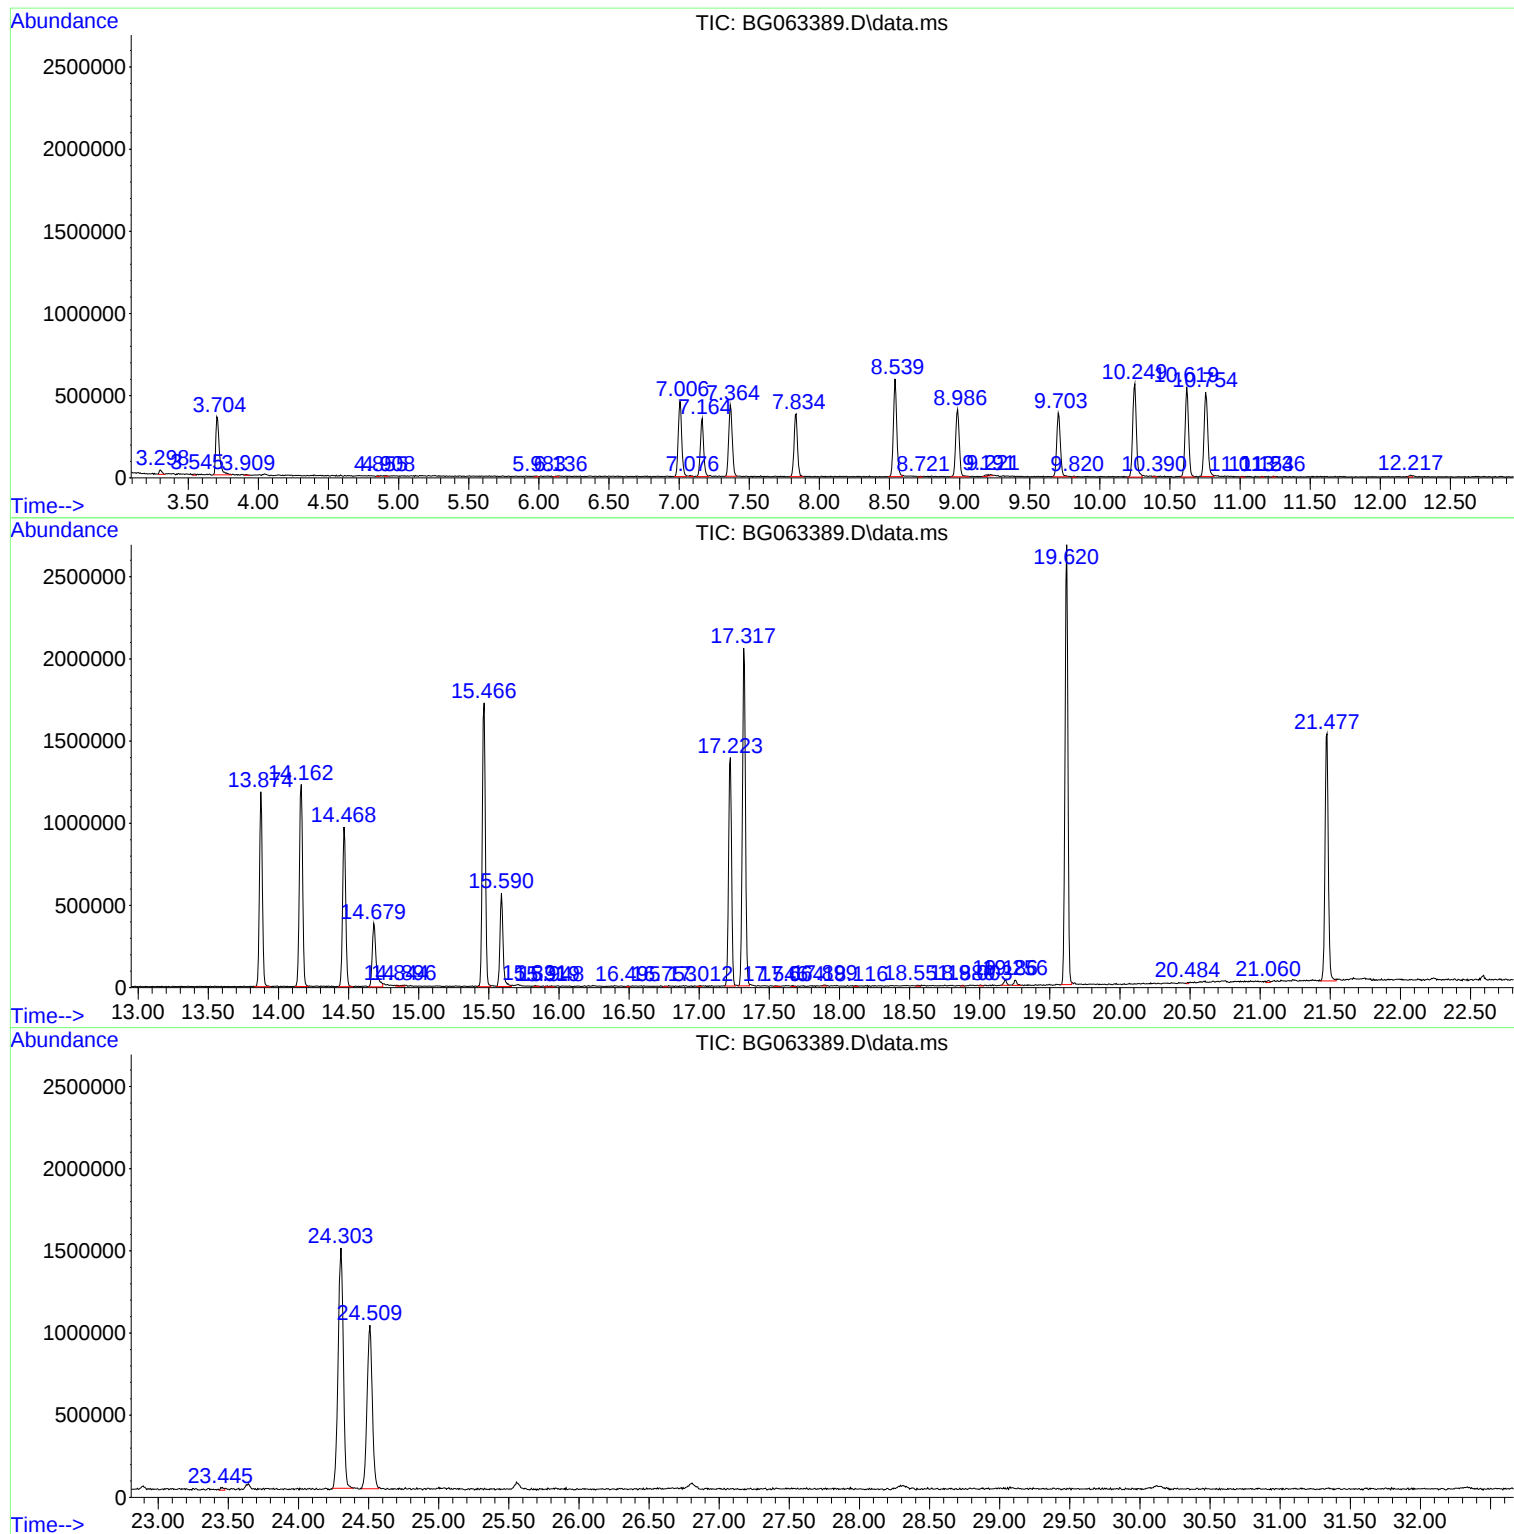

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111324\
Data File : BG063389.D
Acq On : 14 Nov 2024 13:38
Operator : RC/JU
Sample : PB164838BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK838

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111324\
Data File : BG063389.D
Acq On : 14 Nov 2024 13:38
Operator : RC/JU
Sample : PB164838BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK838

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc