

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111324\
 Data File : BG063403.D
 Acq On : 14 Nov 2024 23:06
 Operator : RC/JU
 Sample : PB164842BL
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK842

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG063403.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.299	32	36	44	rBV3	32038	59549	1.38%	0.151%
2	3.705	101	105	113	rBV	366875	617078	14.33%	1.567%
3	3.887	134	136	139	rVB3	6848	6146	0.14%	0.016%
4	4.950	315	317	319	rBV3	5214	6353	0.15%	0.016%
5	5.097	341	342	347	rVB4	4466	6263	0.15%	0.016%
6	5.144	347	350	352	rBV4	5023	6866	0.16%	0.017%
7	5.261	366	370	373	rVB5	4109	6236	0.14%	0.016%
8	6.143	517	520	522	rBV3	4999	6524	0.15%	0.017%
9	6.813	632	634	636	rBV2	6317	6462	0.15%	0.016%
10	7.007	661	667	682	rVB	515026	846619	19.66%	2.149%
11	7.165	686	694	701	rBV	367501	602859	14.00%	1.530%
12	7.365	722	728	737	rBV	469768	803347	18.66%	2.039%
13	7.829	800	807	816	rBV	389818	669112	15.54%	1.699%
14	8.246	873	878	879	rVB4	5500	7140	0.17%	0.018%
15	8.540	921	928	937	rBV2	613955	1043568	24.24%	2.649%
16	8.781	965	969	971	rBV3	5326	7446	0.17%	0.019%
17	8.987	996	1004	1015	rBV	465526	829088	19.26%	2.105%
18	9.204	1037	1041	1046	rBV6	13460	27720	0.64%	0.070%
19	9.709	1116	1127	1137	rBV	427964	779404	18.10%	1.979%
20	10.250	1211	1219	1230	rBV	624202	1145282	26.60%	2.907%
21	10.620	1275	1282	1291	rBV	548641	981924	22.81%	2.493%
22	10.755	1297	1305	1315	rBV	583510	1062181	24.67%	2.697%
23	11.631	1448	1454	1457	rBV5	4801	6301	0.15%	0.016%
24	12.224	1551	1555	1559	rBV4	9452	17452	0.41%	0.044%
25	12.682	1629	1633	1637	rVB2	4649	6934	0.16%	0.018%
26	13.687	1799	1804	1805	rVB4	4932	7025	0.16%	0.018%
27	13.875	1829	1836	1845	rBV	1257675	1843514	42.82%	4.680%
28	14.163	1876	1885	1895	rBV	1403506	2149190	49.92%	5.456%
29	14.468	1931	1937	1944	rBV	1047748	1577957	36.65%	4.006%
30	14.680	1967	1973	1989	rBV	427501	814187	18.91%	2.067%
31	14.886	2006	2008	2015	rVB8	5671	7293	0.17%	0.019%
32	15.291	2073	2077	2081	rBV2	5035	8531	0.20%	0.022%
33	15.467	2100	2107	2119	rBV	1898989	2827093	65.67%	7.177%
34	15.591	2123	2128	2140	rBV	634421	950695	22.08%	2.414%
35	15.708	2145	2148	2155	rVB7	14045	22939	0.53%	0.058%
36	15.826	2164	2168	2171	rBV5	5945	9274	0.22%	0.024%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111324\
 Data File : BG063403.D
 Acq On : 14 Nov 2024 23:06
 Operator : RC/JU
 Sample : PB164842BL
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK842

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
 Title : SVOA CALIBRATION

37	16.249	2238	2240	2244	rVB5	9645	10985	0.26%	0.028%
38	16.907	2348	2352	2353	rVB4	5829	6703	0.16%	0.017%
39	17.218	2398	2405	2415	rBV	1461392	2208333	51.29%	5.606%
40	17.318	2415	2422	2435	rVV	2188566	3394568	78.85%	8.618%
41	17.594	2468	2469	2472	rBV3	5121	5865	0.14%	0.015%
42	17.894	2518	2520	2523	rVB4	7374	6972	0.16%	0.018%
43	18.000	2536	2538	2541	rVB2	6606	5966	0.14%	0.015%
44	18.023	2541	2542	2545	rBV	5621	6110	0.14%	0.016%
45	18.417	2608	2609	2611	rBV2	6855	6573	0.15%	0.017%
46	19.186	2734	2740	2746	rVB2	38449	70484	1.64%	0.179%
47	19.257	2748	2752	2755	rVB2	30490	46215	1.07%	0.117%
48	19.621	2807	2814	2824	rBV	3051522	4305233	100.00%	10.930%
49	20.032	2882	2884	2886	rBV3	8044	6853	0.16%	0.017%
50	20.162	2904	2906	2908	rBV3	6649	6334	0.15%	0.016%
51	21.278	3094	3096	3098	rBV2	13718	10237	0.24%	0.026%
52	21.478	3123	3130	3139	rBV2	1667281	2639338	61.31%	6.700%
53	24.304	3601	3611	3624	rBV	1655241	4167180	96.79%	10.579%
54	24.510	3636	3646	3658	rBV	1011373	2711129	62.97%	6.883%




Sum of corrected areas: 39390630

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111324\
Data File : BG063403.D
Acq On : 14 Nov 2024 23:06
Operator : RC/JU
Sample : PB164842BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK842

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

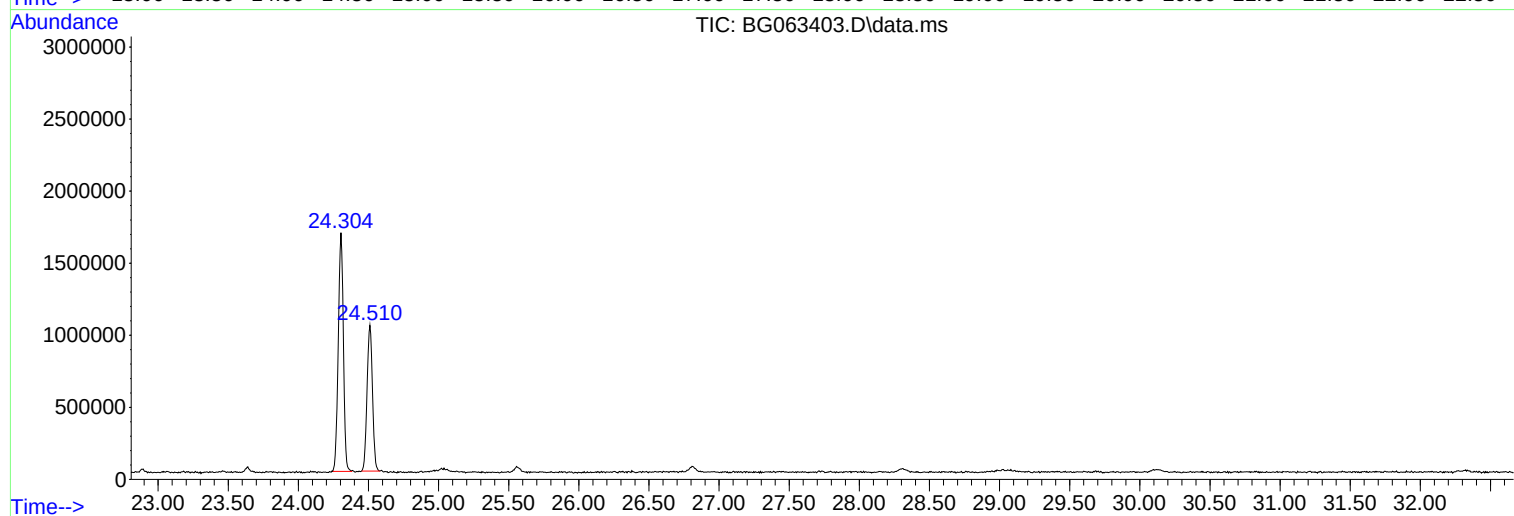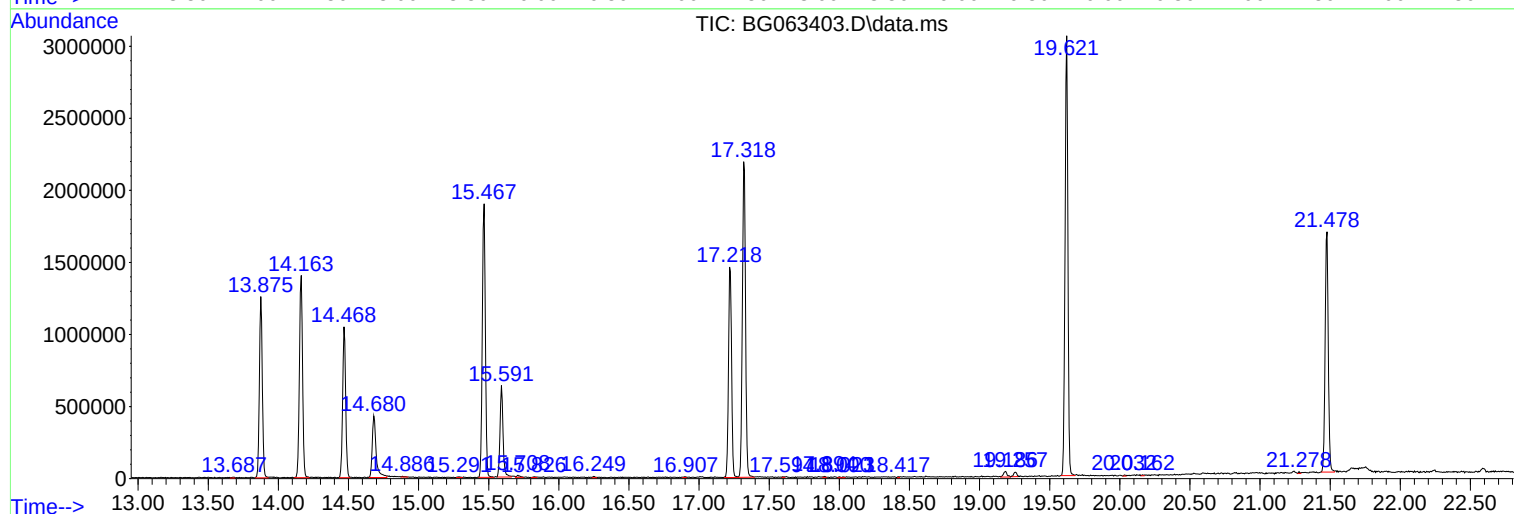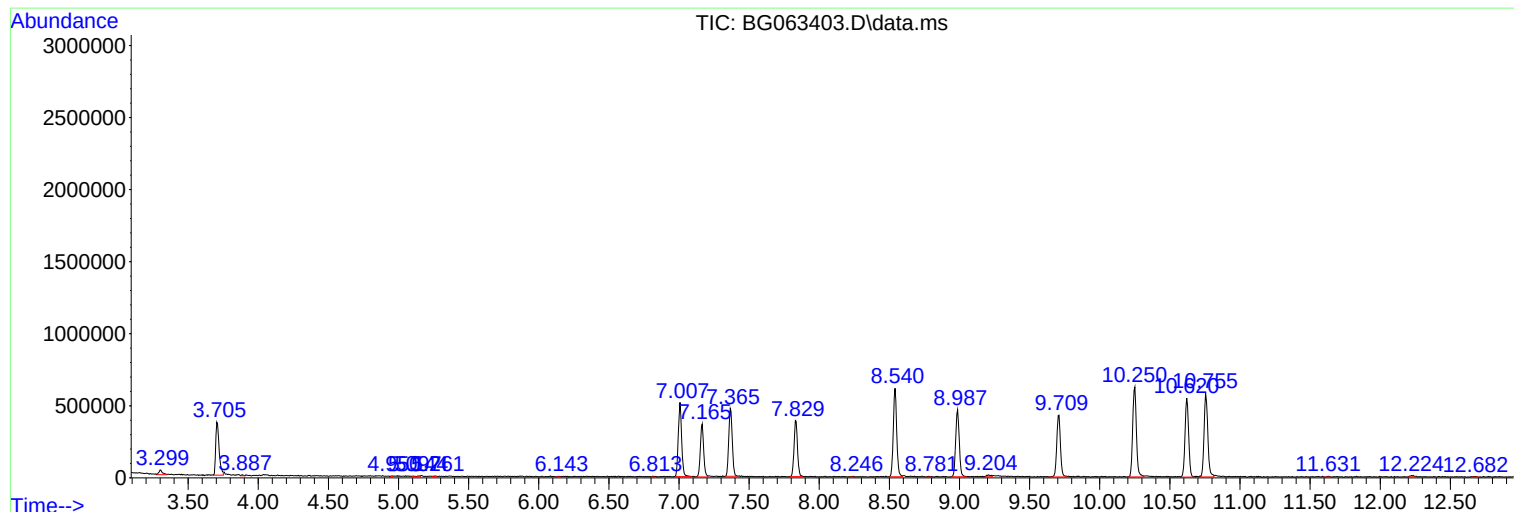

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111324\
Data File : BG063403.D
Acq On : 14 Nov 2024 23:06
Operator : RC/JU
Sample : PB164842BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK842

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111324\
Data File : BG063403.D
Acq On : 14 Nov 2024 23:06
Operator : RC/JU
Sample : PB164842BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK842

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------