

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111324\
 Data File : BG063404.D
 Acq On : 14 Nov 2024 23:44
 Operator : RC/JU
 Sample : PB164840BL
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK840

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG063404.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.305	33	37	46	rVB3	29053	49917	1.22%	0.129%
2	3.710	101	106	115	rBV	377259	635211	15.57%	1.638%
3	3.898	134	138	139	rVB3	8886	5927	0.15%	0.015%
4	4.045	160	163	166	rBV4	11175	12293	0.30%	0.032%
5	4.421	223	227	228	rBV3	4157	5960	0.15%	0.015%
6	4.791	289	290	295	rVB4	5100	6627	0.16%	0.017%
7	7.006	658	667	676	rBV	503895	866068	21.23%	2.233%
8	7.100	681	683	686	rVB4	5703	5760	0.14%	0.015%
9	7.165	688	694	702	rVV	376160	611949	15.00%	1.578%
10	7.247	705	708	709	rBV3	7153	6837	0.17%	0.018%
11	7.364	721	728	737	rBV	477544	837989	20.54%	2.160%
12	7.829	800	807	818	rBV	411257	700777	17.17%	1.807%
13	8.281	879	884	887	rVB3	3350	6176	0.15%	0.016%
14	8.540	921	928	939	rBV2	623999	1080958	26.49%	2.787%
15	8.898	986	989	992	rBV3	3857	5721	0.14%	0.015%
16	8.986	996	1004	1013	rVV	481849	826356	20.25%	2.130%
17	9.209	1041	1042	1046	rBV4	6411	7620	0.19%	0.020%
18	9.709	1119	1127	1135	rBV	428873	782137	19.17%	2.016%
19	10.249	1212	1219	1230	rBV	632447	1136468	27.85%	2.930%
20	10.619	1275	1282	1293	rBV	583429	1007582	24.69%	2.598%
21	10.755	1298	1305	1321	rBV	565377	1100801	26.98%	2.838%
22	12.223	1552	1555	1562	rVB6	8857	17410	0.43%	0.045%
23	13.875	1830	1836	1846	rBV	1300626	1849904	45.34%	4.769%
24	14.162	1876	1885	1895	rBV	1381859	2165274	53.07%	5.582%
25	14.468	1929	1937	1947	rVB	1046479	1609614	39.45%	4.150%
26	14.679	1967	1973	1986	rBV	407058	773991	18.97%	1.995%
27	15.285	2073	2076	2079	rBV5	4438	6630	0.16%	0.017%
28	15.467	2099	2107	2119	rBV	1865237	2849217	69.83%	7.346%
29	15.590	2121	2128	2136	rBV	609861	916714	22.47%	2.363%
30	15.708	2146	2148	2151	rVB3	8796	9776	0.24%	0.025%
31	16.043	2198	2205	2206	rBV4	4704	5986	0.15%	0.015%
32	16.624	2298	2304	2308	rBV3	5002	9504	0.23%	0.025%
33	16.683	2312	2314	2316	rBV3	5186	5614	0.14%	0.014%
34	16.765	2323	2328	2329	rBV2	4734	5995	0.15%	0.015%
35	17.006	2365	2369	2372	rBV5	6954	12478	0.31%	0.032%
36	17.224	2397	2406	2412	rBV	1451220	2150821	52.71%	5.545%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111324\
 Data File : BG063404.D
 Acq On : 14 Nov 2024 23:44
 Operator : RC/JU
 Sample : PB164840BL
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK840

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
 Title : SVOA CALIBRATION

37	17.318	2415	2422	2433	rVV2	2151887	3311776	81.16%	8.538%
38	17.470	2443	2448	2450	rVB4	5648	8848	0.22%	0.023%
39	17.500	2450	2453	2455	rBV3	3822	5613	0.14%	0.014%
40	17.893	2516	2520	2521	rBV3	7761	9812	0.24%	0.025%
41	18.187	2567	2570	2573	rBV4	4758	6599	0.16%	0.017%
42	18.716	2657	2660	2662	rBV2	5509	7691	0.19%	0.020%
43	19.180	2735	2739	2744	rBV3	41796	52053	1.28%	0.134%
44	19.256	2748	2752	2758	rVB	31420	49288	1.21%	0.127%
45	19.450	2783	2785	2788	rBV3	4824	6620	0.16%	0.017%
46	19.621	2807	2814	2824	rBV	2892055	4080376	100.00%	10.520%
47	19.956	2867	2871	2872	rBV4	5955	7301	0.18%	0.019%
48	20.373	2940	2942	2945	rBV4	8176	12047	0.30%	0.031%
49	20.555	2969	2973	2976	rBV5	9970	17187	0.42%	0.044%
50	21.477	3123	3130	3144	rBV	1627706	2537846	62.20%	6.543%
51	21.742	3173	3175	3176	rBV	13450	7430	0.18%	0.019%
52	24.303	3600	3611	3625	rBV	1530299	4035533	98.90%	10.404%
53	24.509	3637	3646	3660	rVB	945125	2543511	62.34%	6.558%


Sum of corrected areas: 38787593

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111324\
Data File : BG063404.D
Acq On : 14 Nov 2024 23:44
Operator : RC/JU
Sample : PB164840BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK840

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

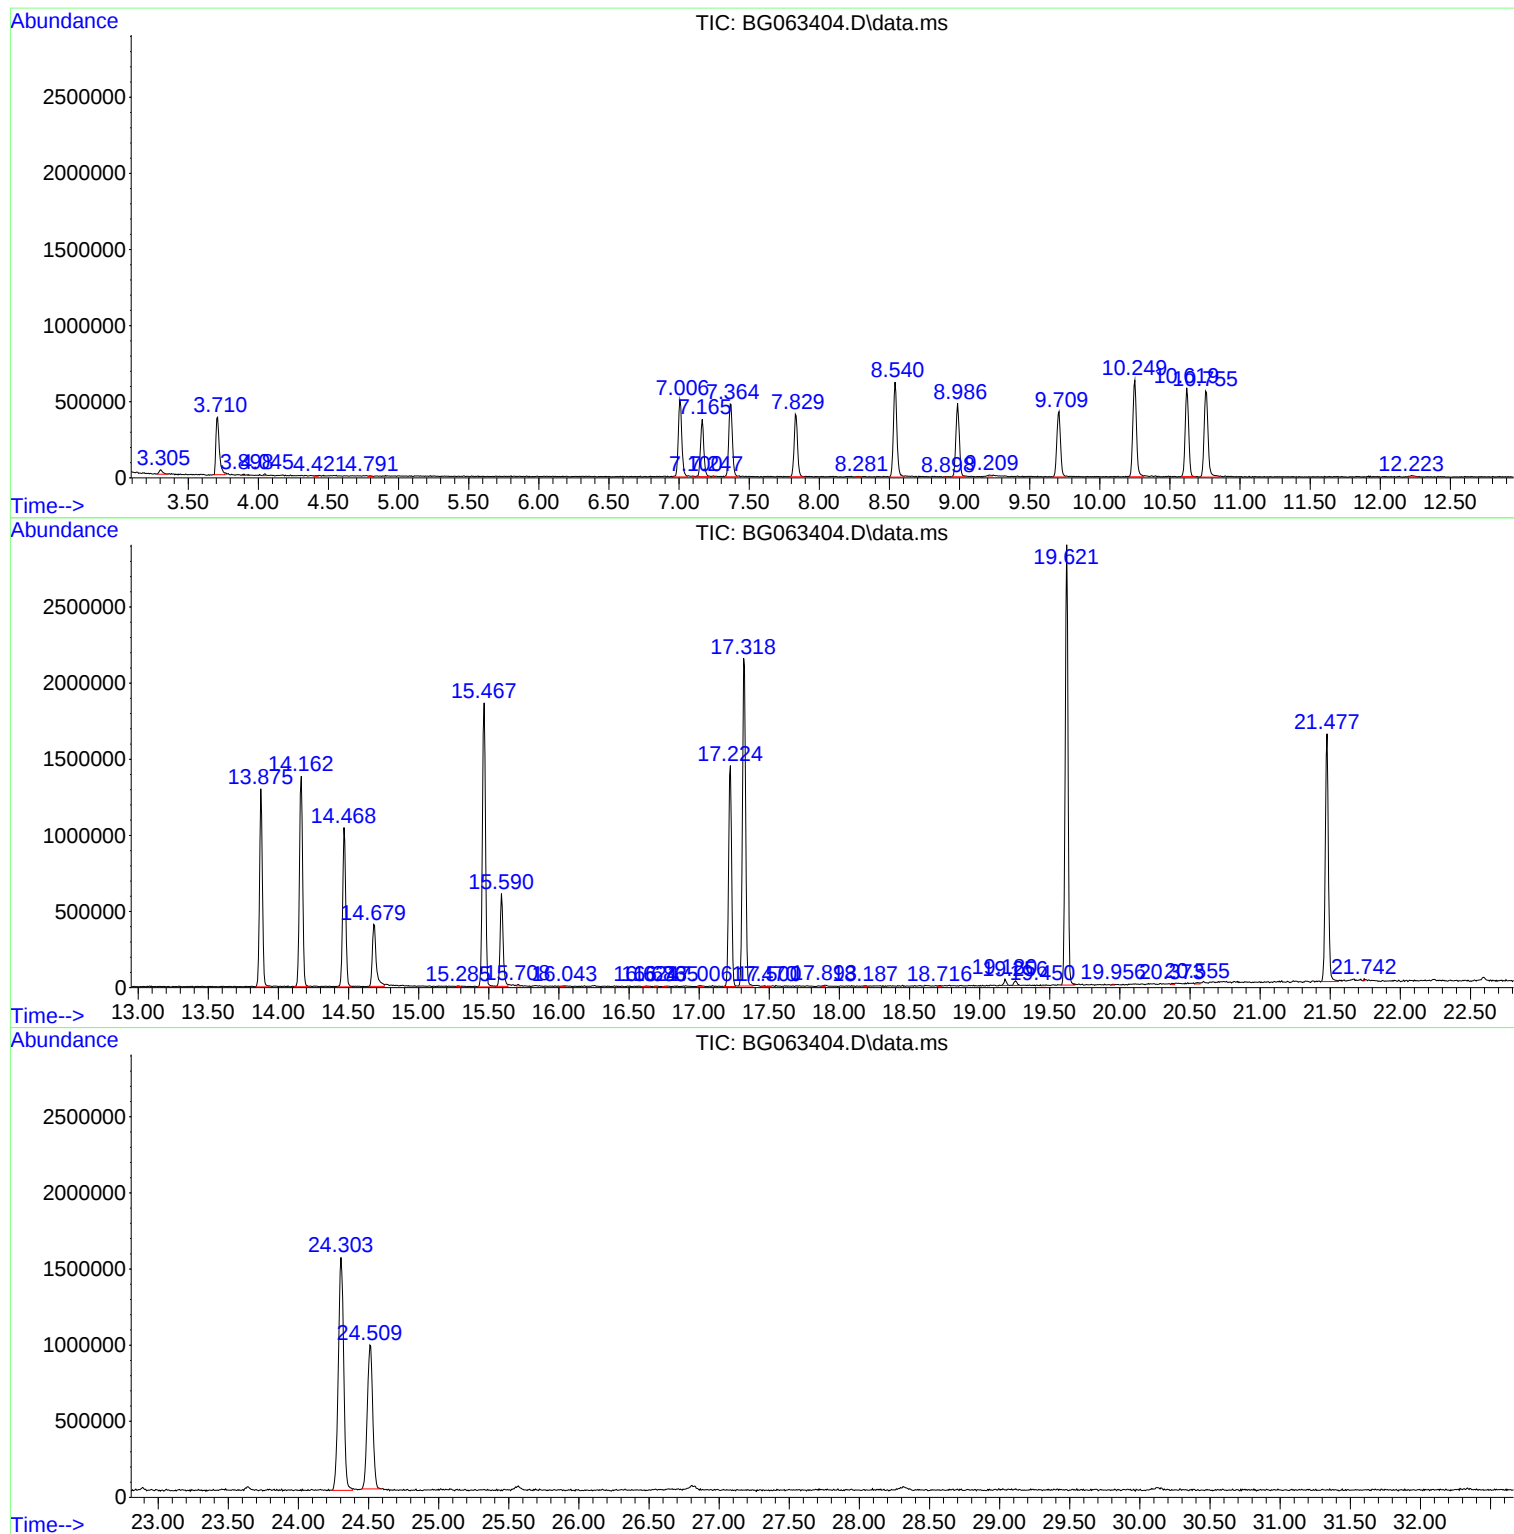

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111324\
Data File : BG063404.D
Acq On : 14 Nov 2024 23:44
Operator : RC/JU
Sample : PB164840BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK840

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111324\
Data File : BG063404.D
Acq On : 14 Nov 2024 23:44
Operator : RC/JU
Sample : PB164840BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK840

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc