

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111324\
 Data File : BG063406.D
 Acq On : 15 Nov 2024 1:00
 Operator : RC/JU
 Sample : P4761-08
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 A0AM8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG063406.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.303	33	36	42	rVB3	24834	36623	0.77%	0.089%
2	3.714	102	106	114	rBV	124918	214786	4.52%	0.520%
3	3.920	140	141	145	rVB4	6098	7416	0.16%	0.018%
4	4.666	265	268	271	rBV4	5176	7569	0.16%	0.018%
5	4.948	313	316	321	rVB5	8429	10057	0.21%	0.024%
6	5.917	477	481	488	rBV3	14694	27405	0.58%	0.066%
7	7.004	659	666	675	rBV	156260	282996	5.96%	0.685%
8	7.163	686	693	703	rBV	439694	709292	14.93%	1.717%
9	7.369	722	728	739	rBV	511823	860750	18.11%	2.083%
10	7.833	800	807	814	rBV	444371	740338	15.58%	1.792%
11	8.074	844	848	850	rBV4	15721	19697	0.41%	0.048%
12	8.538	919	927	937	rBV	485464	841002	17.70%	2.036%
13	8.984	996	1003	1015	rVB	562394	971233	20.44%	2.351%
14	9.707	1117	1126	1135	rBV	517940	910350	19.16%	2.203%
15	10.248	1210	1218	1232	rBV	759348	1332333	28.04%	3.225%
16	10.624	1274	1282	1290	rBV	609147	1099951	23.15%	2.662%
17	10.759	1297	1305	1315	rBV	610765	1136661	23.92%	2.751%
18	12.057	1525	1526	1531	rBV	4951	7251	0.15%	0.018%
19	12.216	1547	1553	1556	rBV5	12776	23593	0.50%	0.057%
20	12.427	1586	1589	1592	rBV2	7497	11697	0.25%	0.028%
21	12.662	1626	1629	1632	rBV3	4686	6578	0.14%	0.016%
22	13.879	1829	1836	1844	rBV	1429380	2105670	44.31%	5.097%
23	14.161	1873	1884	1897	rBV	1533819	2443243	51.42%	5.914%
24	14.472	1929	1937	1947	rBV2	1109049	1992655	41.94%	4.823%
25	14.689	1968	1974	1985	rBV2	90210	201721	4.25%	0.488%
26	14.966	2020	2021	2025	rBV3	6010	6937	0.15%	0.017%
27	15.130	2044	2049	2052	rBV3	5221	7076	0.15%	0.017%
28	15.465	2097	2106	2114	rBV	2171702	3194909	67.24%	7.733%
29	15.588	2121	2127	2136	rBV	701324	1089399	22.93%	2.637%
30	16.164	2221	2225	2232	rBV4	18084	36071	0.76%	0.087%
31	16.252	2237	2240	2244	rVB5	7677	9114	0.19%	0.022%
32	16.893	2346	2349	2352	rBV5	7849	10749	0.23%	0.026%
33	17.222	2398	2405	2415	rBV	1561798	2256727	47.49%	5.462%
34	17.322	2415	2422	2432	rVV	2599647	3780759	79.57%	9.151%
35	17.604	2466	2470	2472	rBV3	6468	8352	0.18%	0.020%
36	18.127	2557	2559	2562	rVB3	7967	7998	0.17%	0.019%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111324\
Data File : BG063406.D
Acq On : 15 Nov 2024 1:00
Operator : RC/JU
Sample : P4761-08
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
A0AM8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Title : SVOA CALIBRATION

37	18.315	2586	2591	2593	rBV5	6394	11262	0.24%	0.027%
38	18.614	2639	2642	2646	rBV4	9166	10037	0.21%	0.024%
39	19.184	2734	2739	2744	rBV2	43169	66636	1.40%	0.161%
40	19.255	2747	2751	2757	rBV	42334	60298	1.27%	0.146%
41	19.548	2799	2801	2805	rBV5	8786	7926	0.17%	0.019%
42	19.619	2807	2813	2819	rBV	3320175	4751607	100.00%	11.501%
43	21.476	3123	3129	3137	rBV	1783831	2646815	55.70%	6.406%
44	24.308	3601	3611	3625	rVB	1804136	4593469	96.67%	11.118%
45	24.513	3637	3646	3658	rVB	1053669	2758017	58.04%	6.676%




Sum of corrected areas: 41315025

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111324\
Data File : BG063406.D
Acq On : 15 Nov 2024 1:00
Operator : RC/JU
Sample : P4761-08
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
A0AM8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

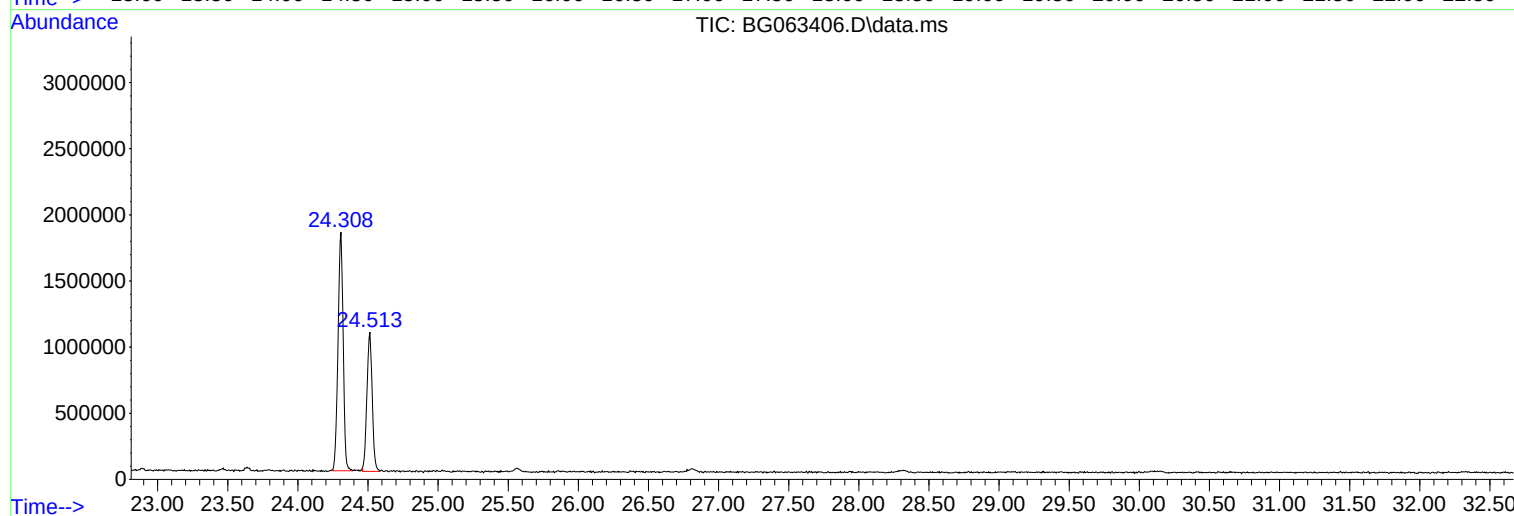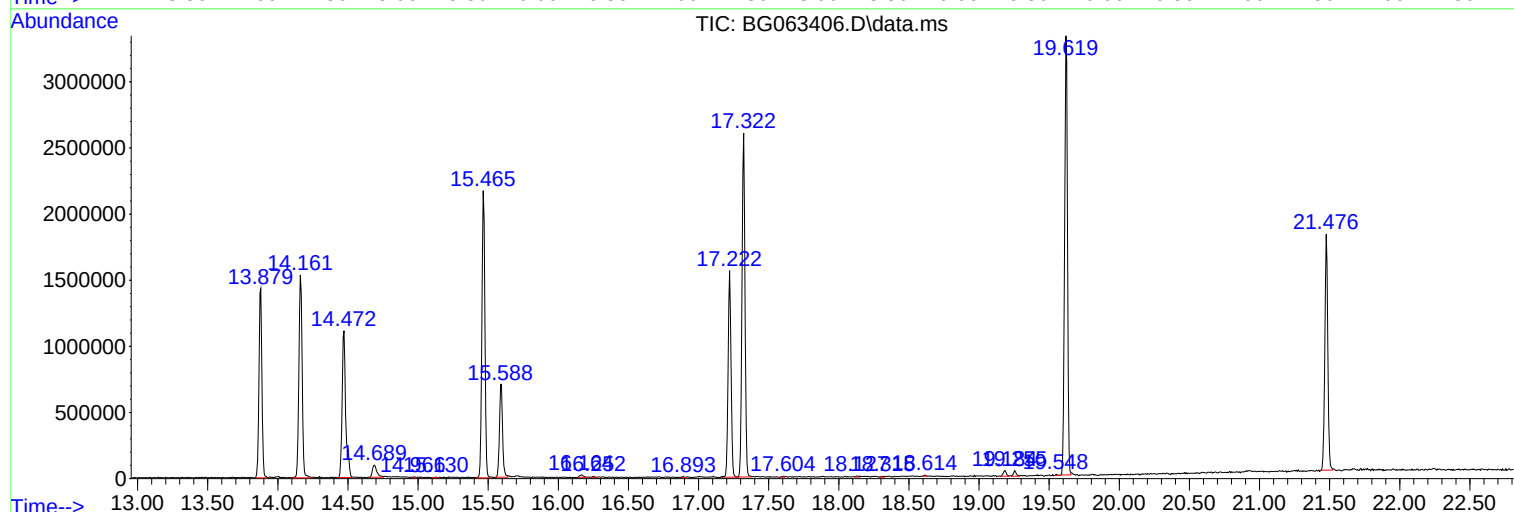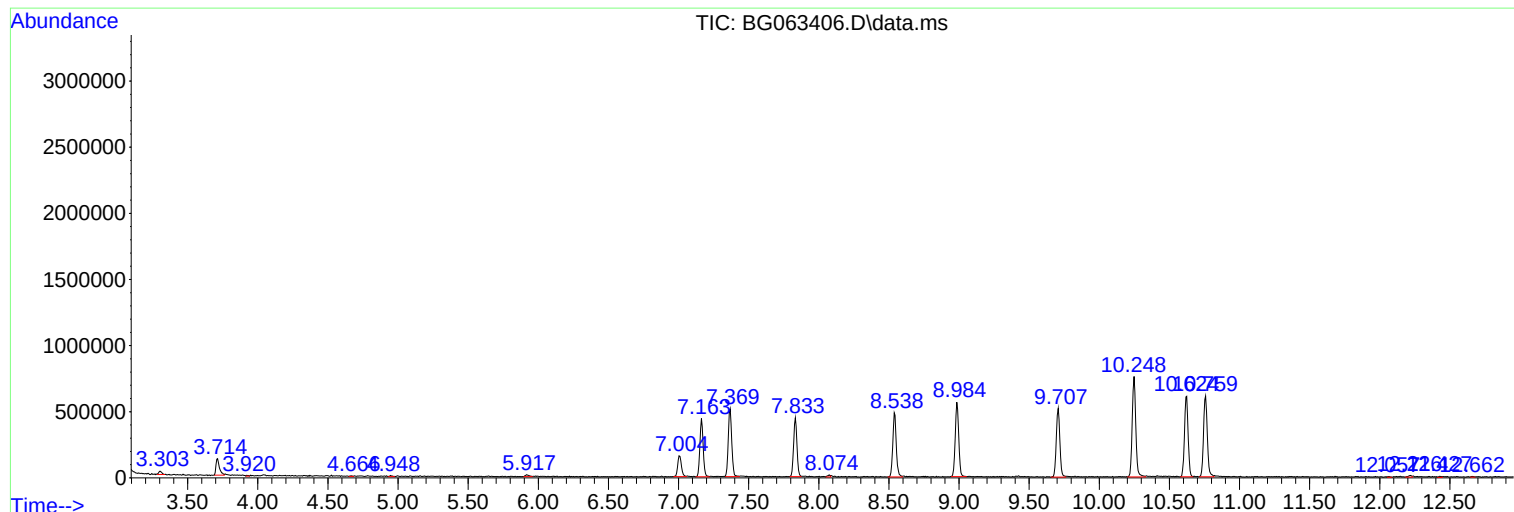

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111324\
Data File : BG063406.D
Acq On : 15 Nov 2024 1:00
Operator : RC/JU
Sample : P4761-08
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
A0AM8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111324\
Data File : BG063406.D
Acq On : 15 Nov 2024 1:00
Operator : RC/JU
Sample : P4761-08
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
A0AM8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc