
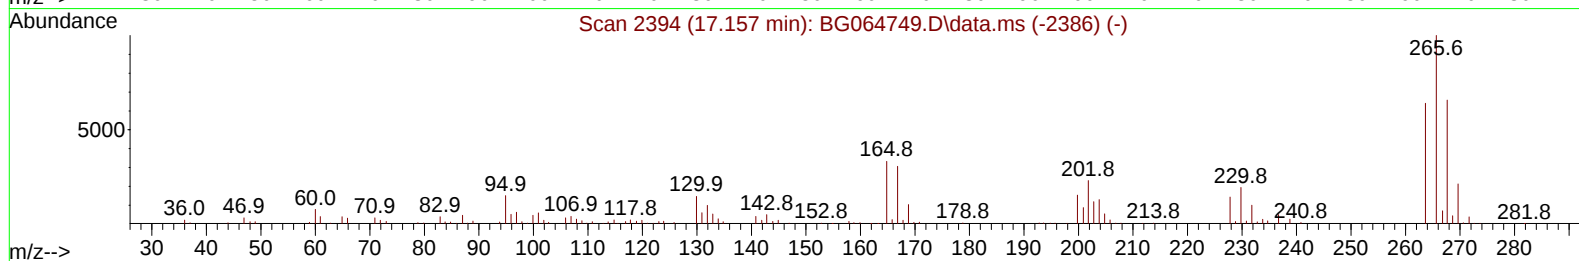
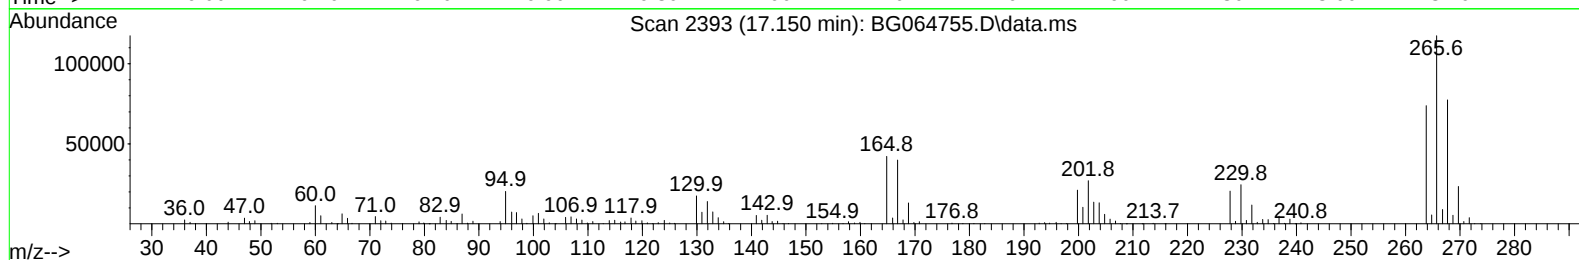


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111325\
Data File : BG064755.D
Acq On : 13 Nov 2025 13:54
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 13 15:48:14 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 12 17:10:56 2025
Response via : Initial Calibration

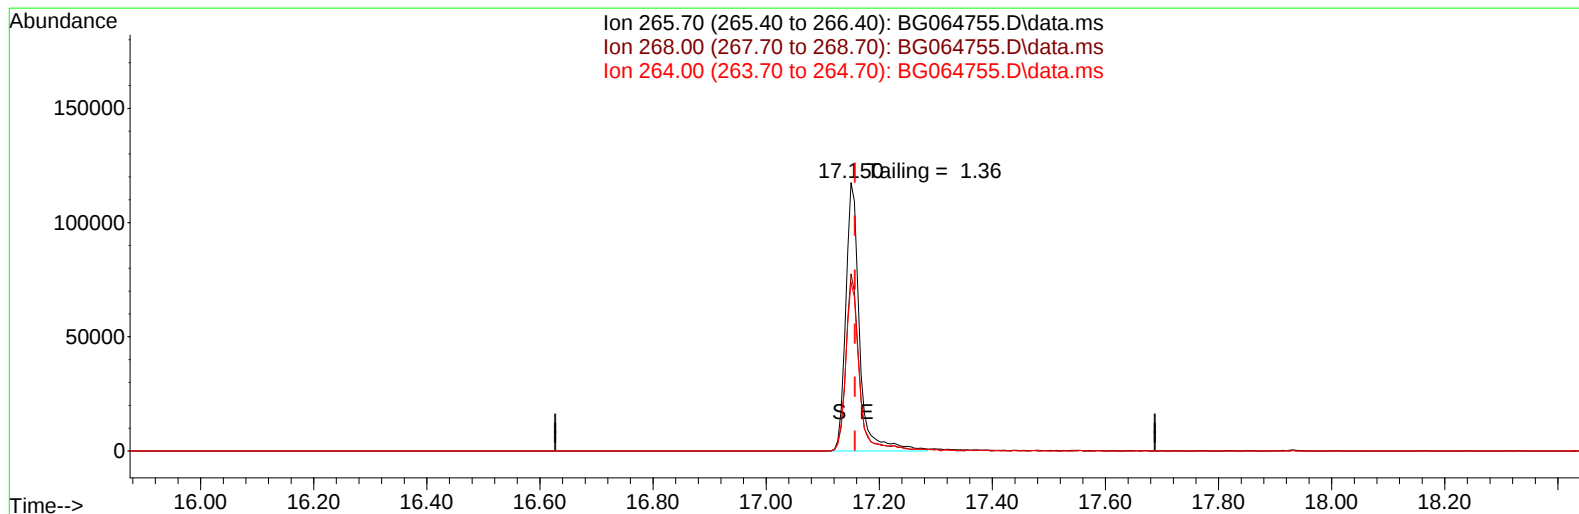

TIC: BG064755.D\data.ms

(70) Pentachlorophenol (C)




17.150min (-0.007) 321859.64 ng

response 200225

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	70.10	70.63
264.00	64.00	62.86
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111325\
Data File : BG064755.D
Acq On : 13 Nov 2025 13:54
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 13 15:48:14 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 12 17:10:56 2025
Response via : Initial Calibration

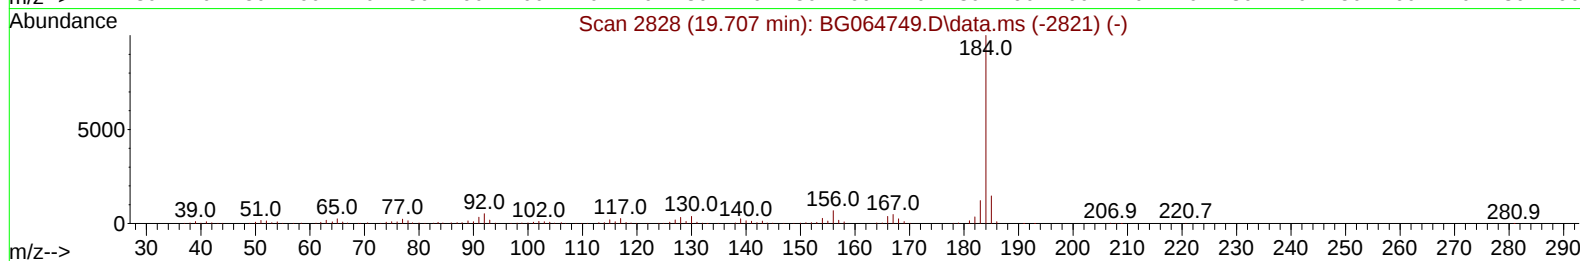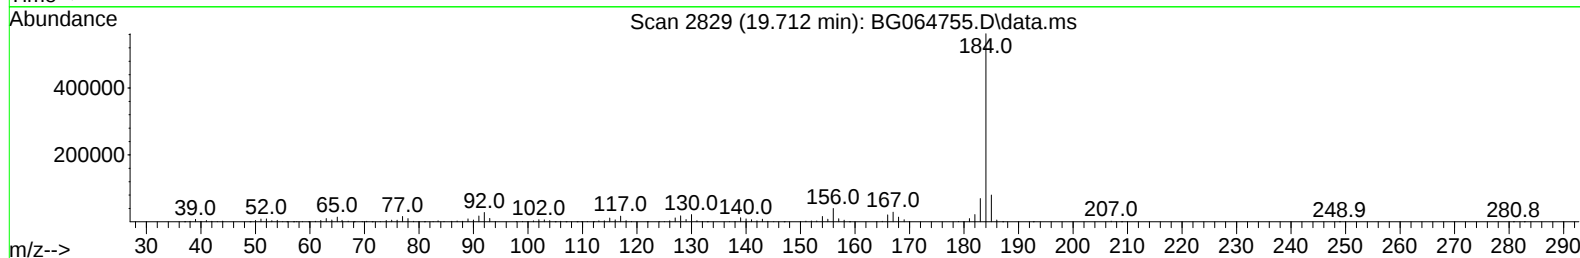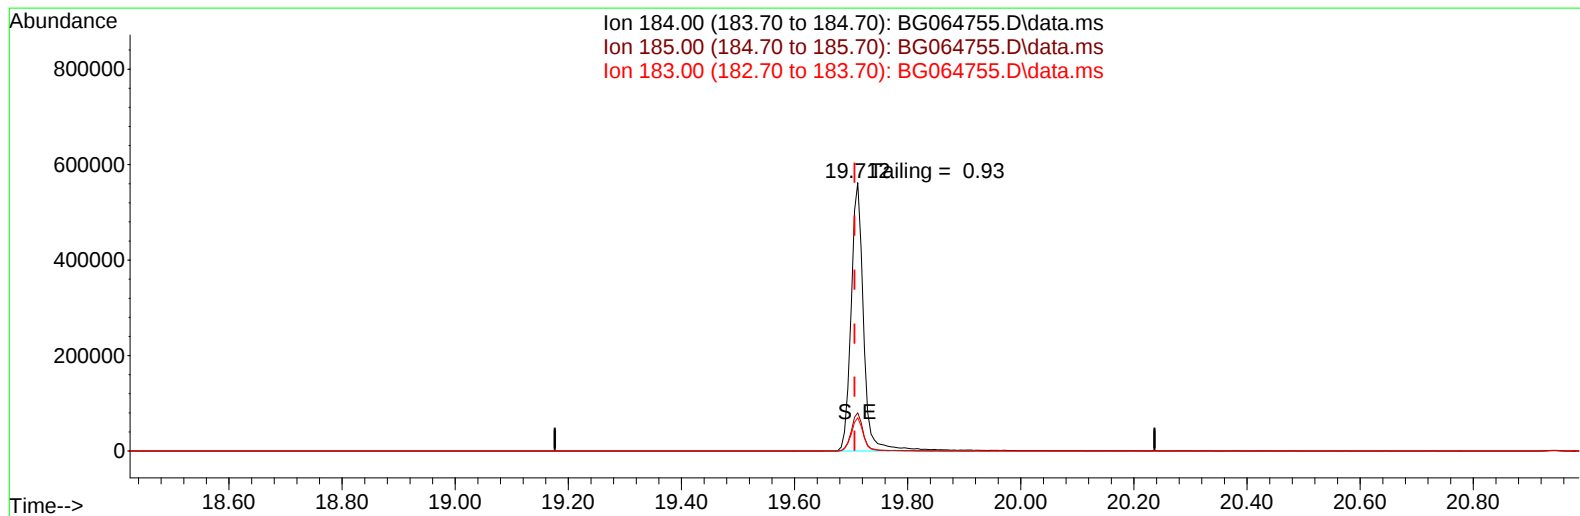

TIC: BG064755.D\data.ms

(77) Benzidine

19.712min (+ 0.005) 16479.67 ng

response 867643

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.24
183.00	12.20	12.39
0.00	0.00	0.00