

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111325\
 Data File : BG064760.D
 Acq On : 13 Nov 2025 17:22
 Operator : RC/JU
 Sample : Q3609-13
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 AU-713-COMP-05

Quant Time: Nov 14 05:01:20 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111225.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 12 17:10:56 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.165	152	32026	20.000	ng	0.00
21) Naphthalene-d8	10.979	136	119447	20.000	ng	# 0.00
39) Acenaphthene-d10	14.775	164	93146	20.000	ng	0.00
64) Phenanthrene-d10	17.501	188	235739	20.000	ng	0.00
76) Chrysene-d12	21.755	240	324228	20.000	ng	0.00
86) Perylene-d12	25.010	264	339738	20.000	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.703	112	158731	86.548	ng	0.00
7) Phenol-d6	7.307	99	211175	86.571	ng	0.00
23) Nitrobenzene-d5	9.328	82	130699	54.100	ng	0.00
42) 2,4,6-Tribromophenol	16.250	330	162303	89.343	ng	0.00
45) 2-Fluorobiphenyl	13.406	172	365640	54.773	ng	0.00
79) Terphenyl-d14	20.092	244	965500	58.577	ng	0.00


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111325\
Data File : BG064760.D
Acq On : 13 Nov 2025 17:22
Operator : RC/JU
Sample : Q3609-13
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
AU-713-COMP-05

Quant Time: Nov 14 05:01:20 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 12 17:10:56 2025
Response via : Initial Calibration




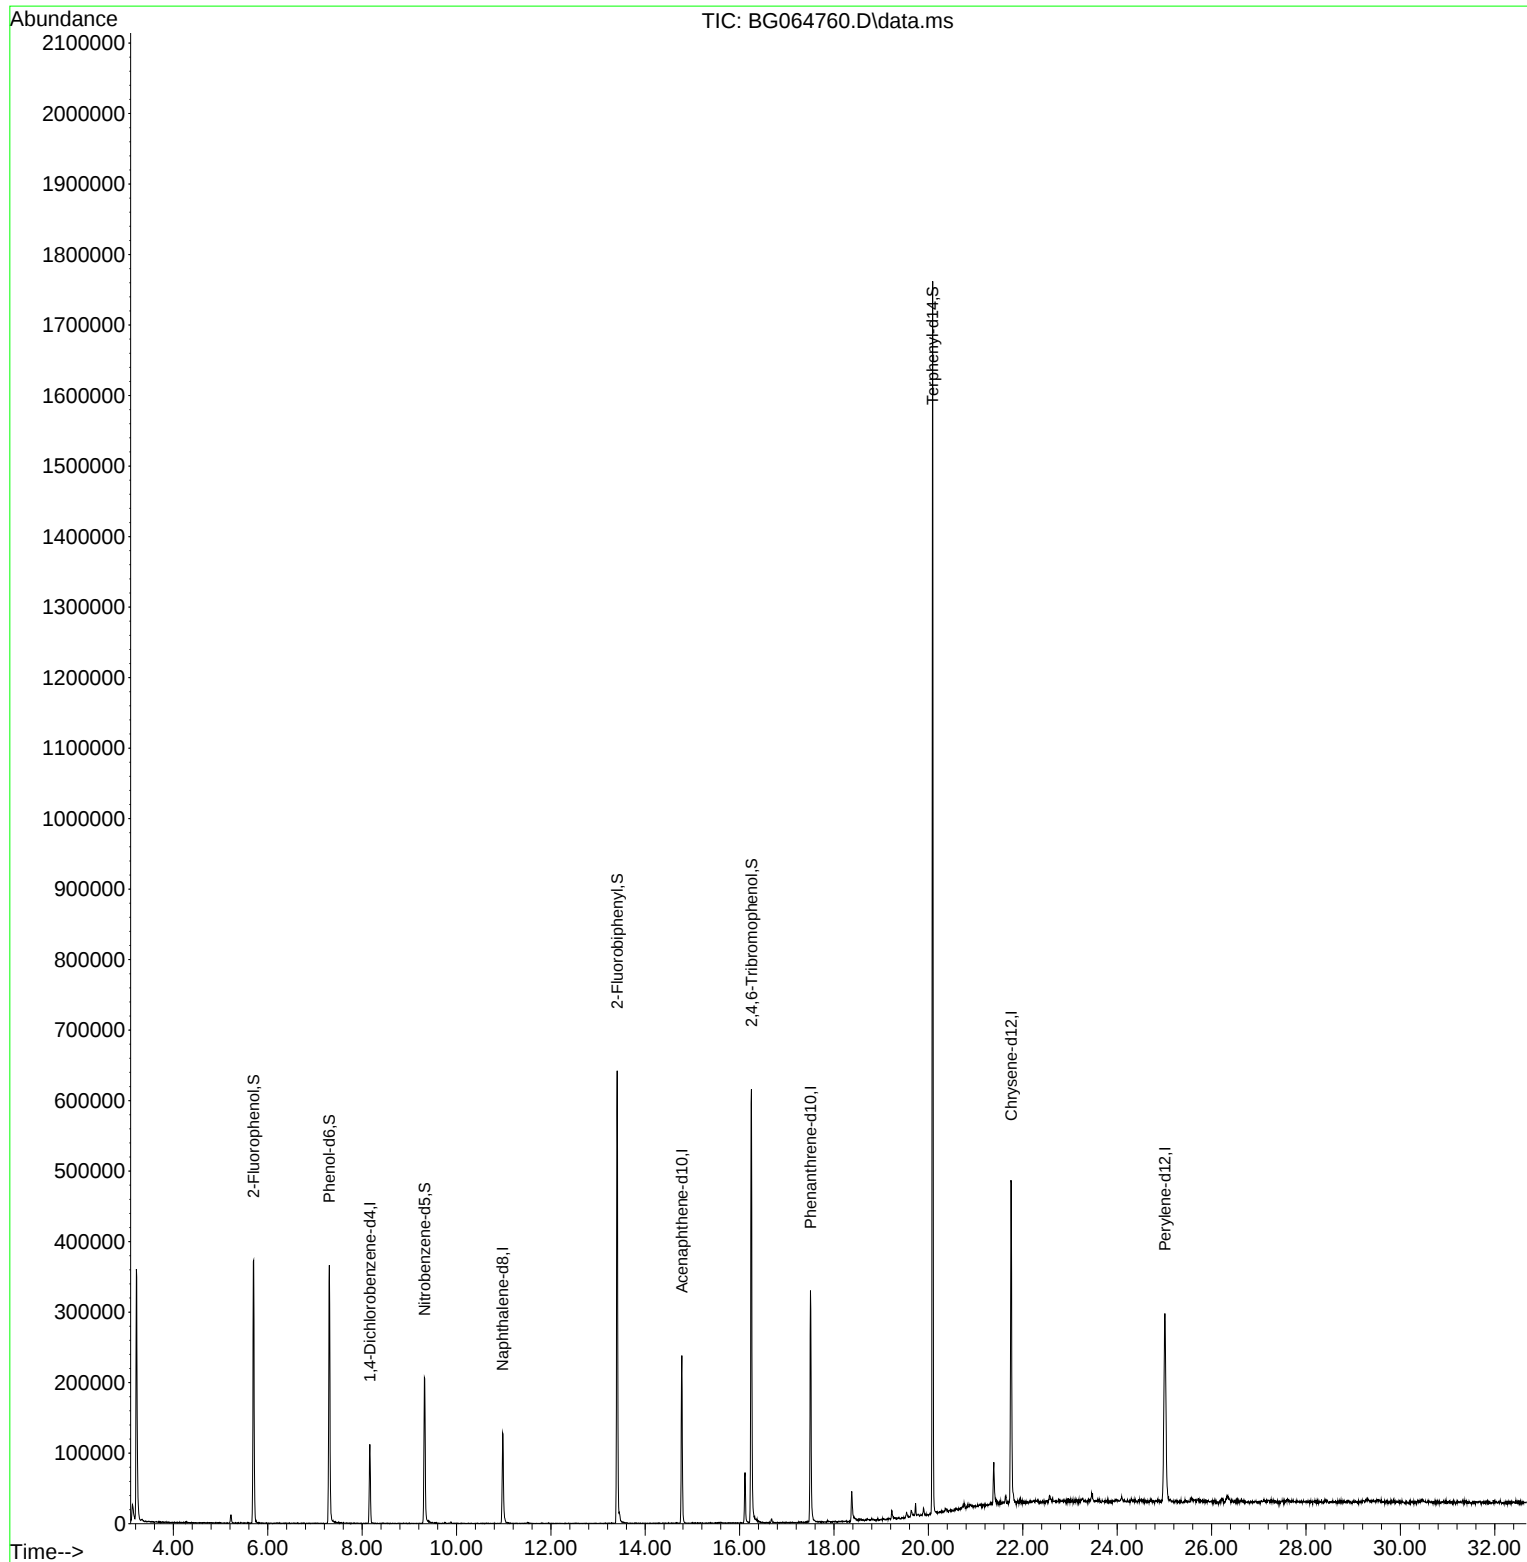


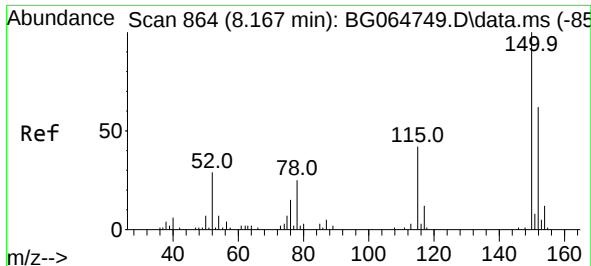

#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.165 min Scan# 80
Delta R.T. -0.002 min
Lab File: BG064760.D
Acq: 13 Nov 2025 17:22




Instrument :
BNA_G
ClientSampleId :
AU-713-COMP-05


Tgt Ion:152 Resp: 32026
Ion Ratio Lower Upper
152 100
150 152.9 129.2 193.8
115 56.2 53.7 80.5

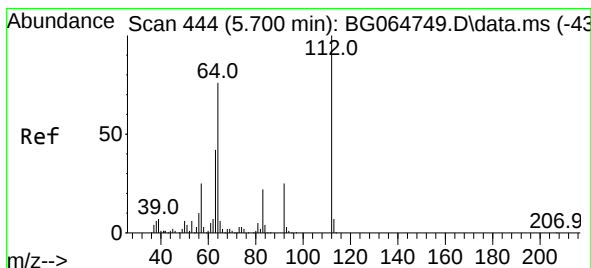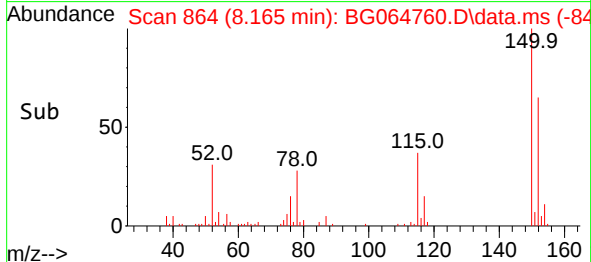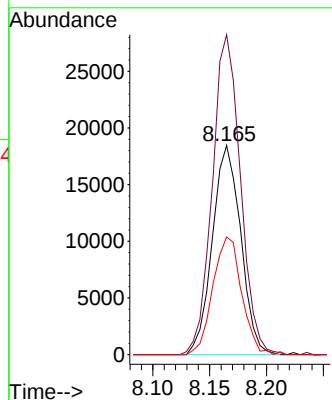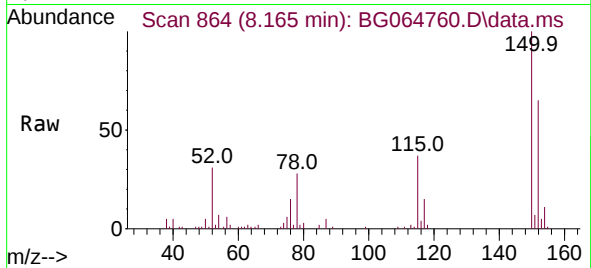

#5
2-Fluorophenol
Concen: 86.548 ng
RT: 5.703 min Scan# 445
Delta R.T. 0.003 min
Lab File: BG064760.D
Acq: 13 Nov 2025 17:22


Tgt Ion:112 Resp: 158731
Ion Ratio Lower Upper
112 100
64 75.4 61.0 91.4
63 42.5 33.3 49.9

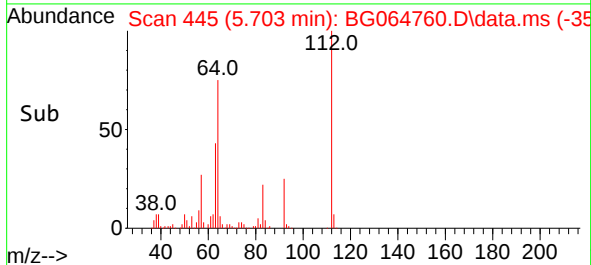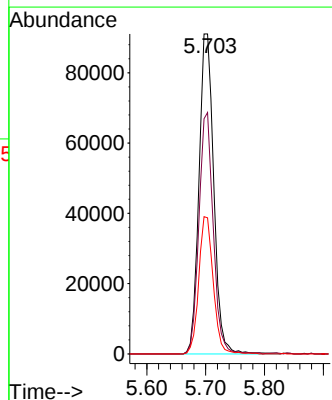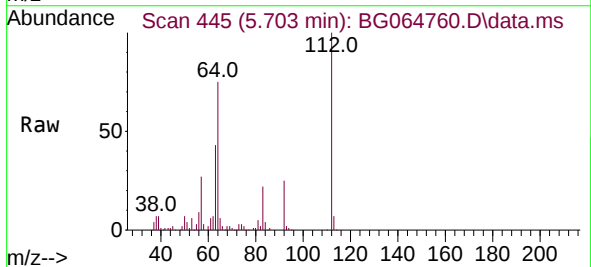

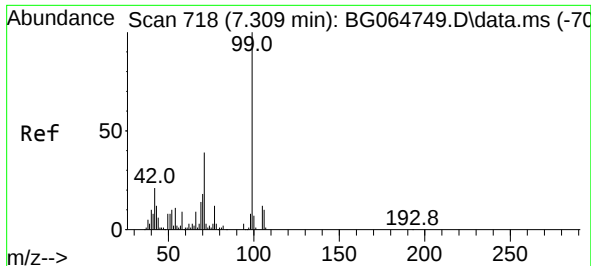




#7
Phenol-d6
Concen: 86.571 ng
RT: 7.307 min Scan# 718
Delta R.T. -0.002 min
Lab File: BG064760.D
Acq: 13 Nov 2025 17:22

Instrument :
BNA_G
ClientSampleId :
AU-713-COMP-05

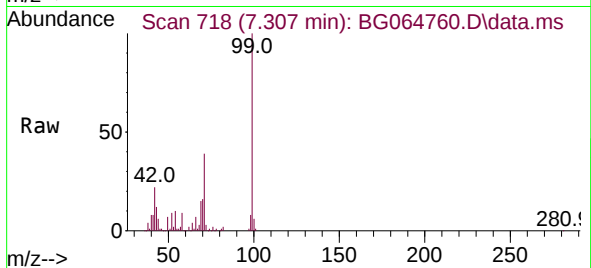

Tgt Ion: 99 Resp: 211175




Ion	Ratio	Lower	Upper
99	100		
42	21.6	16.8	25.2
71	39.5	31.1	46.7

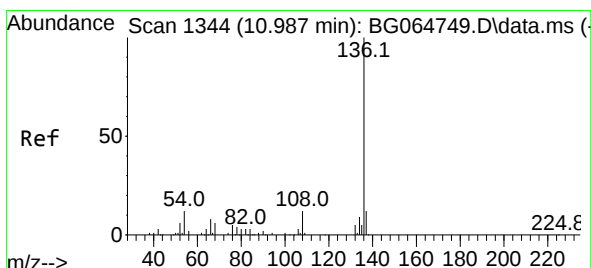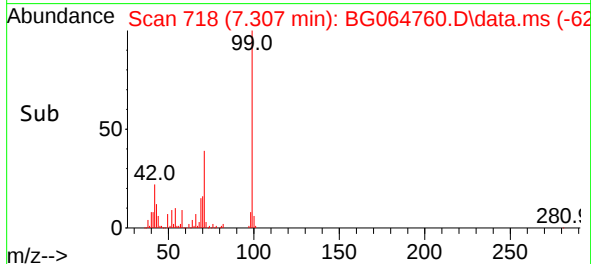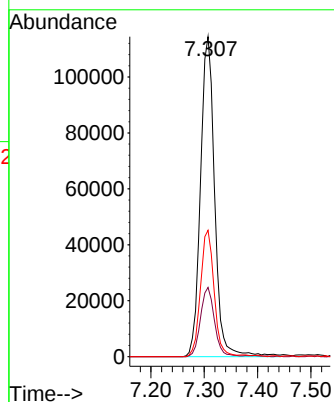


#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.979 min Scan# 1343
Delta R.T. -0.008 min
Lab File: BG064760.D
Acq: 13 Nov 2025 17:22

Tgt Ion: 136 Resp: 119447

Ion	Ratio	Lower	Upper
136	100		
137	10.7	9.3	13.9
54	12.9	9.3	13.9
68	4.7	5.0	7.6

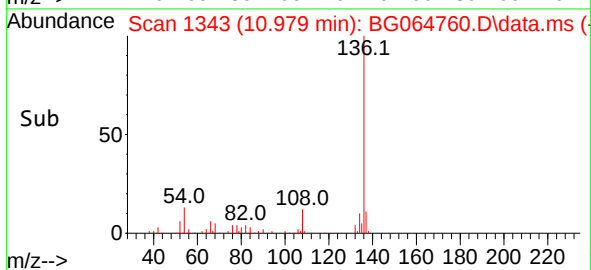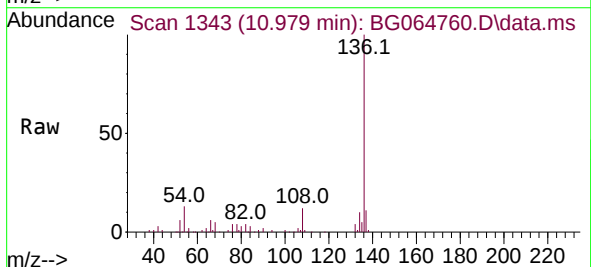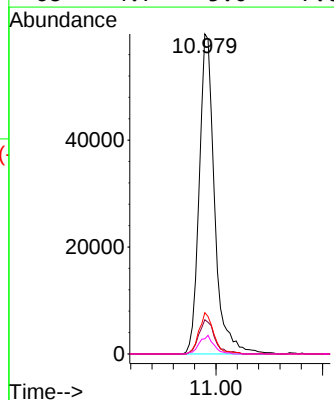

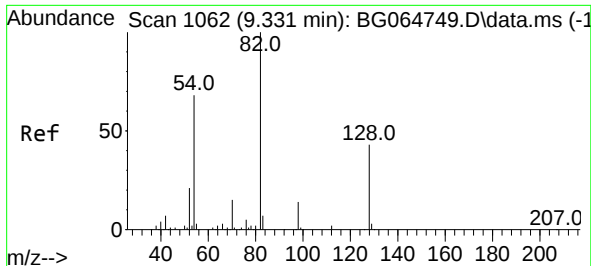

#23

Nitrobenzene-d5

Concen: 54.100 ng

RT: 9.328 min Scan# 1062

Delta R.T. -0.002 min

Lab File: BG064760.D

Acq: 13 Nov 2025 17:22

Instrument :

BNA_G

ClientSampleId :

AU-713-COMP-05





Tgt Ion: 82 Resp: 130699

Ion Ratio Lower Upper

82 100

128 39.7 34.1 51.1

54 65.0 54.3 81.5

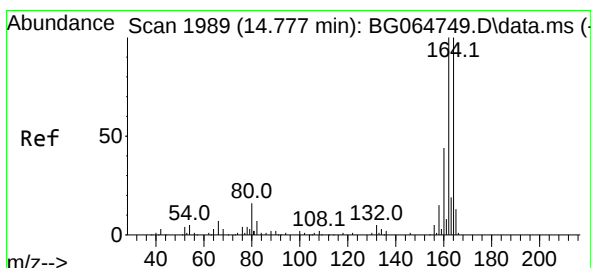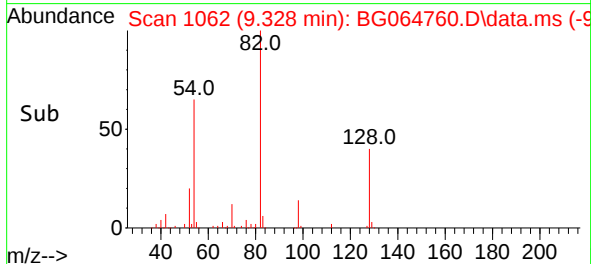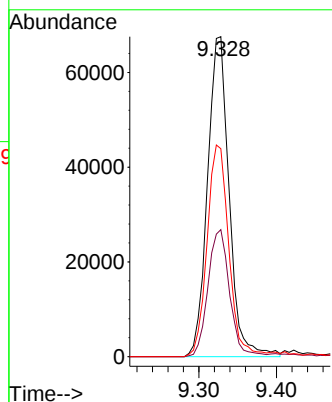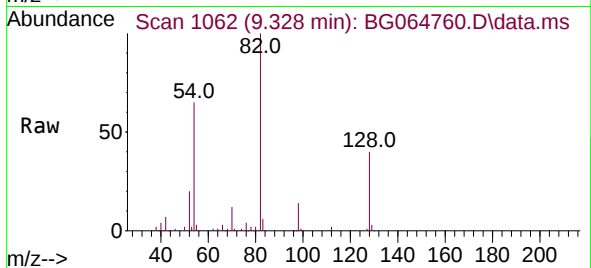

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 14.775 min Scan# 1989

Delta R.T. -0.002 min

Lab File: BG064760.D

Acq: 13 Nov 2025 17:22




Tgt Ion: 164 Resp: 93146


Ion Ratio Lower Upper

164 100

162 103.3 79.8 119.6


160 46.8 34.9 52.3

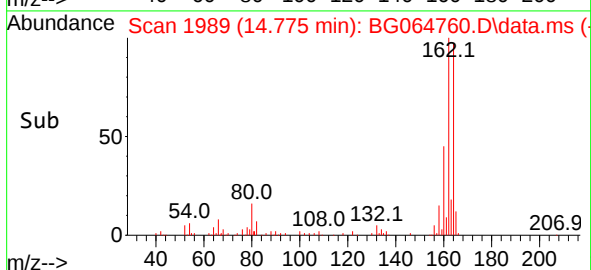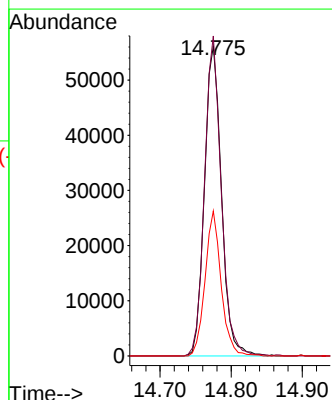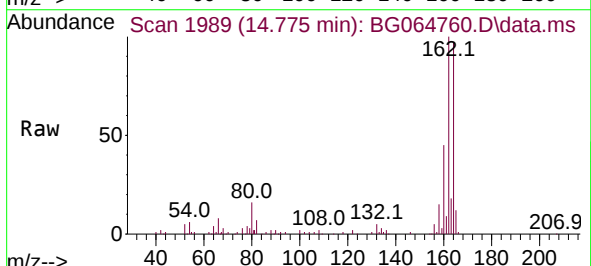



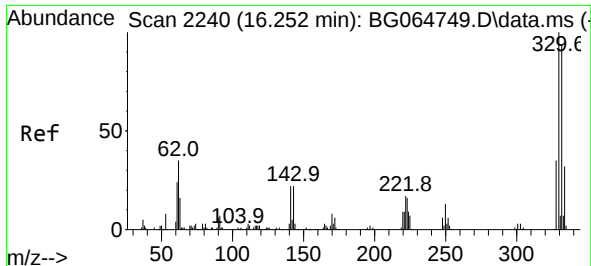


#42
2,4,6-Tribromophenol
Concen: 89.343 ng
RT: 16.250 min Scan# 21
Delta R.T. -0.002 min
Lab File: BG064760.D
Acq: 13 Nov 2025 17:22


Instrument :
BNA_G
ClientSampleId :
AU-713-COMP-05

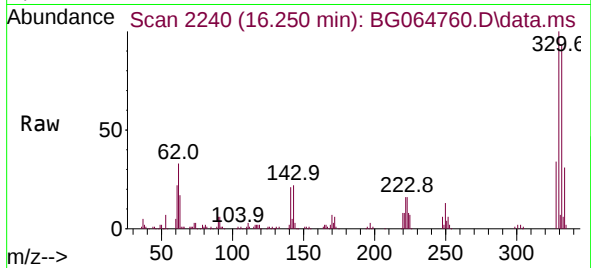



Tgt Ion:330 Resp: 162303
Ion Ratio Lower Upper
330 100
332 93.5 77.0 115.6
141 22.3 18.2 27.2

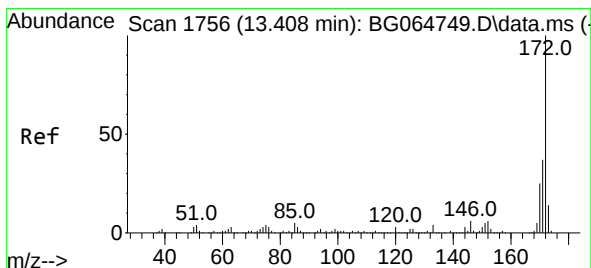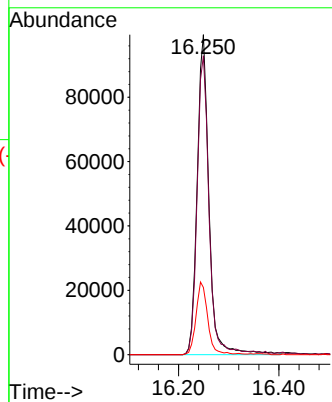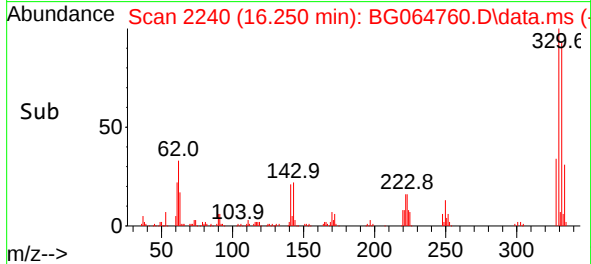


#45
2-Fluorobiphenyl
Concen: 54.773 ng
RT: 13.406 min Scan# 1756
Delta R.T. -0.002 min
Lab File: BG064760.D
Acq: 13 Nov 2025 17:22

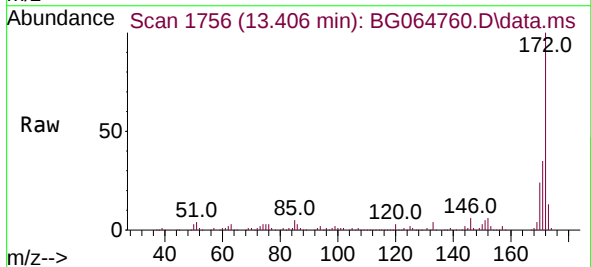

Tgt Ion:172 Resp: 365640
Ion Ratio Lower Upper
172 100
171 34.9 29.9 44.9
170 24.0 19.8 29.6



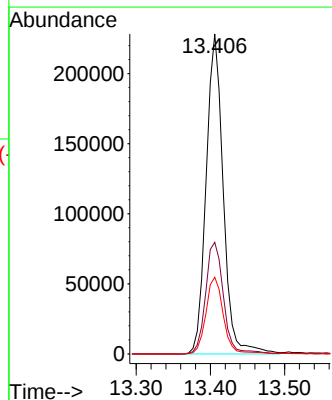
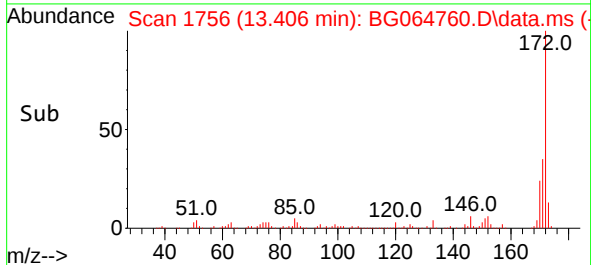


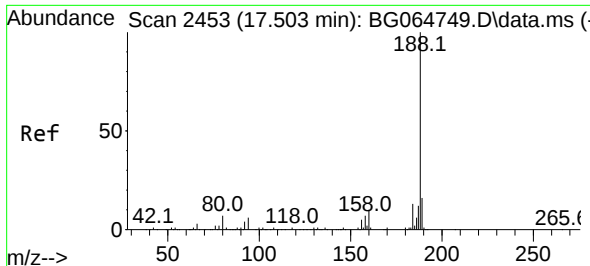

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.501 min Scan# 2453
Delta R.T. -0.002 min
Lab File: BG064760.D
Acq: 13 Nov 2025 17:22




Instrument :
BNA_G
ClientSampleId :
AU-713-COMP-05


Tgt Ion:188 Resp: 235739
Ion Ratio Lower Upper
188 100
94 5.6 4.7 7.1
80 6.0 5.4 8.2

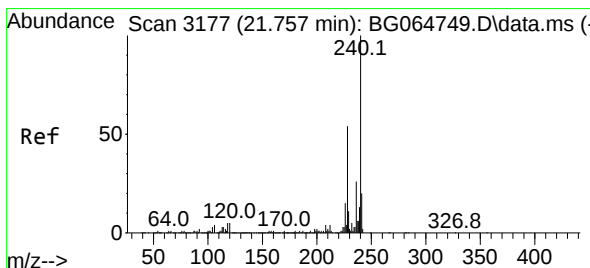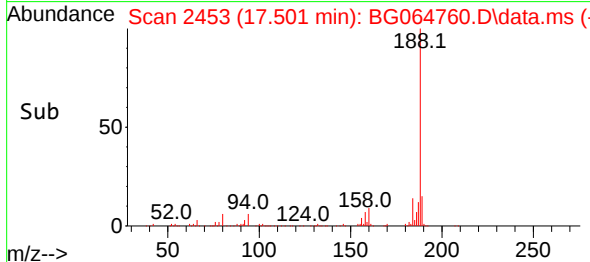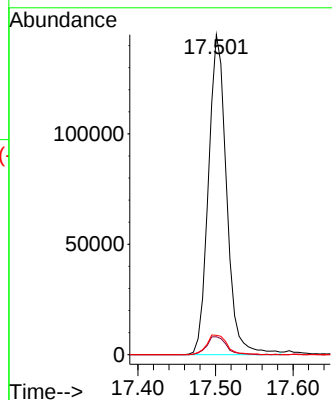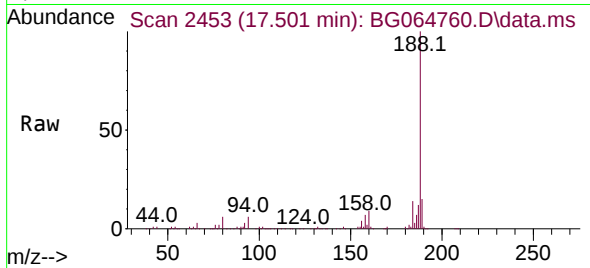

#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.755 min Scan# 3177
Delta R.T. -0.002 min
Lab File: BG064760.D
Acq: 13 Nov 2025 17:22

Tgt Ion:240 Resp: 324228
Ion Ratio Lower Upper
240 100
120 5.2 4.2 6.4
236 25.1 20.8 31.2


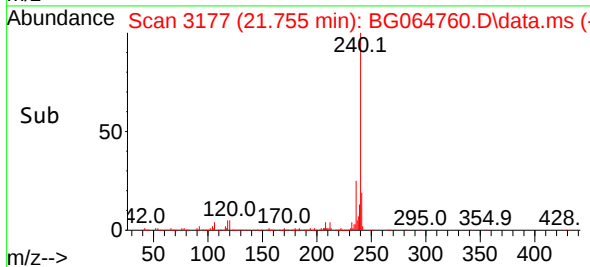
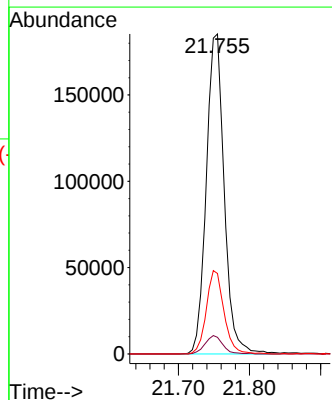
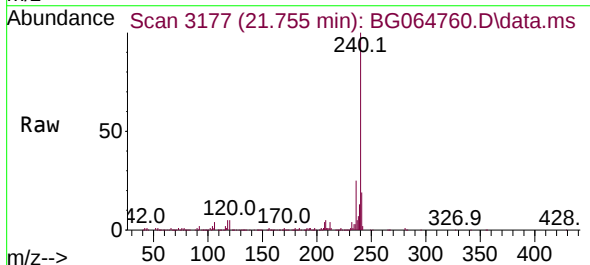


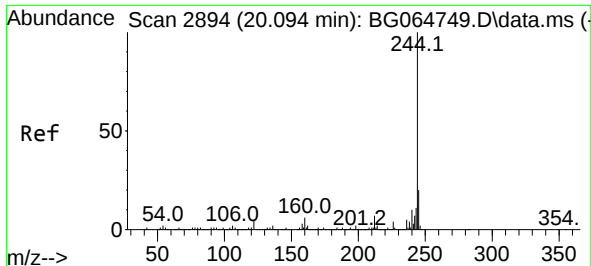

#79
Terphenyl-d14
Concen: 58.577 ng
RT: 20.092 min Scan# 2894
Delta R.T. -0.002 min
Lab File: BG064760.D
Acq: 13 Nov 2025 17:22

Instrument :
BNA_G
ClientSampleId :
AU-713-COMP-05

Tgt Ion:244 Resp: 965500
Ion Ratio Lower Upper
244 100
212 6.9 5.8 8.6
122 5.0 4.3 6.5

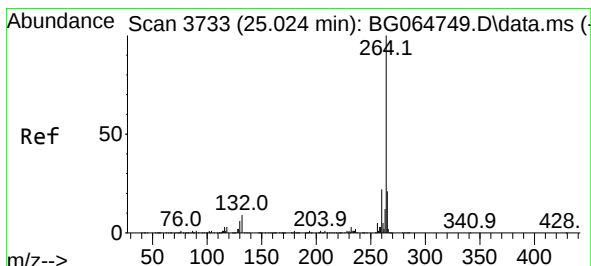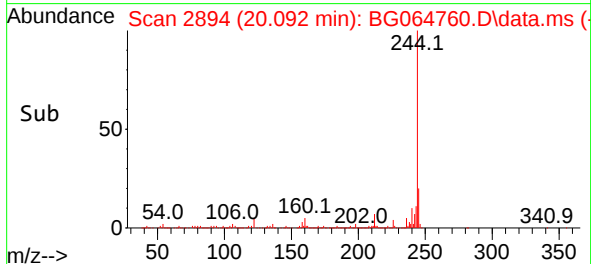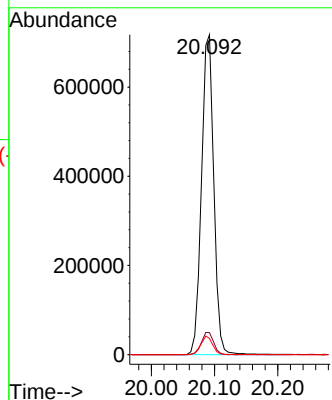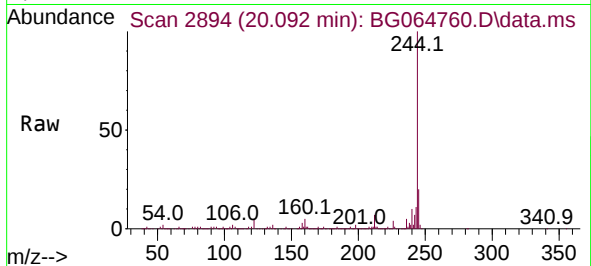

#86
Perylene-d12
Concen: 20.000 ng
RT: 25.010 min Scan# 3731
Delta R.T. -0.014 min
Lab File: BG064760.D
Acq: 13 Nov 2025 17:22

Tgt Ion:264 Resp: 339738
Ion Ratio Lower Upper
264 100
260 24.9 17.2 25.8
265 23.0 16.6 25.0

