

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG111419\
 Data File : BG043644.D
 Acq On : 14 Nov 2019 21:45
 Operator : JU
 Sample : K5806-01
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 STOCK-PILE

Quant Time: Nov 15 01:01:18 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG102119.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 04 15:22:15 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.00	152	39313	20.00	ng	-0.01
21) Naphthalene-d8	10.80	136	152815	20.00	ng	-0.02
39) Acenaphthene-d10	14.62	164	104493	20.00	ng	-0.02
64) Phenanthrene-d10	17.37	188	238555	20.00	ng	-0.02
76) Chrysene-d12	21.64	240	258252	20.00	ng	-0.02
87) Perylene-d12	24.82	264	304634	20.00	ng	-0.03

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
5) 2-Fluorophenol	5.59	112	194556	90.69	ng	0.00
7) Phenol-d6	7.20	99	271453	87.94	ng	0.00
23) Nitrobenzene-d5	9.16	82	160920	54.29	ng	-0.02
42) 2,4,6-Tribromophenol	16.12	330	146325	73.59	ng	-0.02
45) 2-Fluorobiphenyl	13.25	172	447326	59.15	ng	-0.02
79) Terphenyl-d14	19.98	244	775422	56.33	ng	-0.02


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
10) Phenol	7.22	94	9271	3.287	ng	91
19) n-Nitroso-di-n-propylamine	9.16	70	22492	11.277	ng	# 82
50) Dimethylphthalate	14.08	163	42172	5.210	ng	98
56) 4-Nitrophenol	15.03	139	3170	2.786	ng	# 1
57) 2,4-Dinitrotoluene	14.62	165	15337	6.103	ng	# 28
58) Fluorene	15.68	166	17396	2.228	ng	96
67) 4-Bromophenyl-phenylether	16.12	248	9834	3.063	ng	# 1
71) Phenanthrene	17.42	178	241581	19.776	ng	99
72) Anthracene	17.42	178	241581	19.766	ng	98
73) Carbazole	17.79	167	24208	2.187	ng	97
75) Fluoranthene	19.42	202	474697	29.807	ng	99
77) Benzidine	19.98	184	12626	2.429	ng	# 93
78) Pvrene	19.79	202	428303	26.793	ng	99
81) Benzo(a)anthracene	21.62	228	251573	15.552	ng	100
83) Chrysene	21.68	228	239308	14.889	ng	98
86) Indeno(1,2,3-cd)pyrene	28.46	276	213570	10.586	ng	# 97
88) Benzo(b)fluoranthene	23.81	252	358610	20.785	ng	97
89) Benzo(k)fluoranthene	23.81	252	358610	20.646	ng	96
90) Benzo(a)pvrene	24.67	252	275484	16.720	ng	98
91) Dibenzo(a,h)anthracene	28.48	278	34089	2.023	ng	99
92) Benzo(g,h,i)perylene	29.58	276	211951	12.750	ng	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG111419\
Data File : BG043644.D
Acq On : 14 Nov 2019 21:45
Operator : JU
Sample : K5806-01
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
STOCK-PILE

Quant Time: Nov 15 01:01:18 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG102119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 04 15:22:15 2019
Response via : Initial Calibration






#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.00 min Scan# 835
Delta R.T. -0.01 min
Lab File: BG043644.D
Acq: 14 Nov 2019 21:45

Instrument :
BNA_G
ClientSampleId :
STOCK-PILE

Tot Ion:152 Resp: 39313
Ion Ratio Lower Upper
152 100
150 150.5 129.4 194.0
115 60.9 48.8 73.2




Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

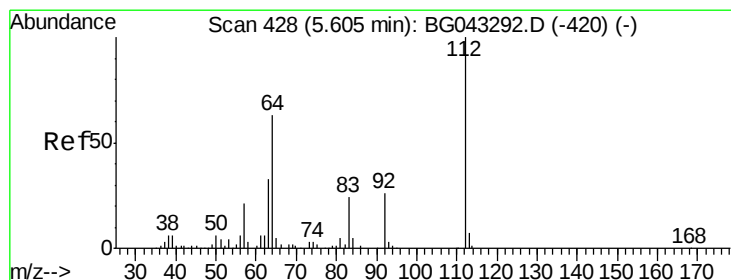



#5


2-Fluorophenol
Concen: 90.686 ng
RT: 5.59 min Scan# 426
Delta R.T. 0.00 min
Lab File: BG043644.D
Acq: 14 Nov 2019 21:45

Tgt Ion:112 Resp: 194556
Ion Ratio Lower Upper
112 100
64 60.8 50.0 75.0
63 36.1 26.6 40.0



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BG
Ion 63.00 (62.70 to 63.70): BG





#7

Phenol-d6

Concen: 87.943 ng

RT: 7.20 min Scan# 699

Delta R.T. 0.00 min

Lab File: BG043644.D

Acq: 14 Nov 2019 21:45

Instrument :

BNA_G

ClientSampleId :

STOCK-PILE


Tot Ion: 99 Resp: 271453

Ion Ratio Lower Upper




99 100

42 17.8 14.6 21.8

71 39.8 32.5 48.7



Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC



#10

Phenol

Concen: 3.287 ng

RT: 7.22 min Scan# 703

Delta R.T. 0.00 min

Lab File: BG043644.D

Acq: 14 Nov 2019 21:45


Tgt Ion: 94 Resp: 9271

Ion Ratio Lower Upper



94 100


65 27.4 12.6 52.6

66 56.4 30.7 70.7



Abundance Ion 94.00 (93.70 to 94.70): BGC
Ion 65.00 (64.70 to 65.70): BGC
Ion 66.00 (65.70 to 66.70): BGC





#19

n-Nitroso-di-n-propylamine

Concen: 11.277 ng

RT: 9.16 min Scan# 1033

Delta R.T. 0.35 min

Lab File: BG043644.D

Acq: 14 Nov 2019 21:45

Instrument :

BNA_G

ClientSampleId :

STOCK-PILE

Tot Ion: 70 Resp: 22492





Ion Ratio Lower Upper

70 100

42 48.5 41.4 62.2

101 0.0 7.9 11.9#

130 3.1 19.0 28.4#



#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.80 min Scan# 1312

Delta R.T. -0.02 min

Lab File: BG043644.D

Acq: 14 Nov 2019 21:45

Tgt Ion: 136 Resp: 152815




Ion Ratio Lower Upper


136 100

137 12.0 8.7 13.1

54 8.4 5.4 8.2#

68 4.4 3.0 4.4









#23
Nitrobenzene-d5
Concen: 54.289 ng
RT: 9.16 min Scan# 1033
Delta R.T. -0.02 min
Lab File: BG043644.D
Acq: 14 Nov 2019 21:45




Instrument :
BNA_G
ClientSampleId :
STOCK-PILE


Tot Ion: 82 Resp: 160920
Ion Ratio Lower Upper
82 100
128 40.9 35.0 52.6
54 52.4 40.2 60.2



#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.62 min Scan# 1963
Delta R.T. -0.02 min
Lab File: BG043644.D
Acq: 14 Nov 2019 21:45

Tgt Ion: 164 Resp: 104493
Ion Ratio Lower Upper
164 100
162 101.8 83.5 125.3
160 45.0 36.5 54.7




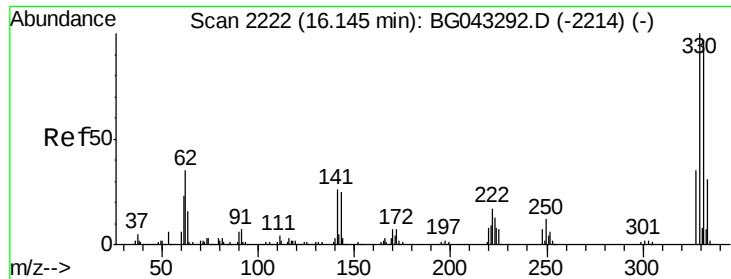

#42
 2,4,6-Tribromophenol
 Concen: 73.585 ng
 RT: 16.12 min Scan# 2217
 Delta R.T. -0.02 min
 Lab File: BG043644.D
 Acq: 14 Nov 2019 21:45




Instrument :
 BNA_G
 ClientSampleId :
 STOCK-PILE

Tot Ion	Ratio	Lower	Upper
330	100		
332	98.5	77.4	116.0
141	29.7	22.8	34.2




Abundance

Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E





#45
 2-Fluorobiphenyl
 Concen: 59.154 ng
 RT: 13.25 min Scan# 1729
 Delta R.T. -0.02 min
 Lab File: BG043644.D
 Acq: 14 Nov 2019 21:45


Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.3	28.9	43.3
170	22.3	18.5	27.7



Abundance

Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E





#50

Dimethylphthalate

Concen: 5.210 ng

RT: 14.08 min Scan# 1870

Delta R.T. -0.02 min

Lab File: BG043644.D

Acq: 14 Nov 2019 21:45

Instrument :

BNA_G

ClientSampleId :

STOCK-PILE


Tot Ion:163 Resp: 42172

Ion Ratio Lower Upper

163 100

194 4.1 3.8 5.6




164 10.2 8.9 13.3



Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E



#56

4-Nitrophenol

Concen: 2.786 ng

RT: 15.03 min Scan# 2032

Delta R.T. 0.15 min

Lab File: BG043644.D

Acq: 14 Nov 2019 21:45


Tgt Ion:139 Resp: 3170

Ion Ratio Lower Upper

139 100

109 0.0 87.2 127.2#



65 0.0 83.8 123.8#




Abundance Ion 139.00 (138.70 to 139.70): E

Ion 109.00 (108.70 to 109.70): E

Ion 65.00 (64.70 to 65.70): BGC






#57
2,4-Dinitrotoluene
Concen: 6.103 ng
RT: 14.62 min Scan# 1963
Delta R.T. -0.38 min
Lab File: BG043644.D
Acq: 14 Nov 2019 21:45

Instrument :
BNA_G
ClientSampleId :
STOCK-PILE

Tot Ion	Ratio	Lower	Upper
165	100		
63	1.5	33.2	49.8#
89	2.3	52.2	78.4#
182	0.0	2.0	3.0#






Abundance

Ion 165.00 (164.70 to 165.70): E

Ion 63.00 (62.70 to 63.70): BGC


Ion 89.00 (88.70 to 89.70): BGC

Ion 182.00 (181.70 to 182.70): E



#58
Fluorene
Concen: 2.228 ng
RT: 15.68 min Scan# 2142
Delta R.T. -0.01 min
Lab File: BG043644.D
Acq: 14 Nov 2019 21:45

Tgt Ion	Ratio	Lower	Upper
166	100		
165	94.7	79.0	118.6
167	14.5	10.5	15.7






Abundance

Ion 166.00 (165.70 to 166.70): E

Ion 165.00 (164.70 to 165.70): E

Ion 167.00 (166.70 to 167.70): E





#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.37 min Scan# 2431

Delta R.T. -0.02 min

Lab File: BG043644.D

Acq: 14 Nov 2019 21:45

Instrument :

BNA_G

ClientSampleId :

STOCK-PILE


Tot Ion:188 Resp: 238555

Ion Ratio Lower Upper

188 100

94 5.6 4.2 6.4




80 5.7 4.5 6.7



Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BGC

Ion 80.00 (79.70 to 80.70): BGC



#67

4-Bromophenyl-phenylether

Concen: 3.063 ng

RT: 16.12 min Scan# 2218

Delta R.T. -0.45 min

Lab File: BG043644.D

Acq: 14 Nov 2019 21:45


Tgt Ion:248 Resp: 9834

Ion Ratio Lower Upper

248 100

250 194.1 77.0 115.4#



141 387.4 47.5 71.3#




Abundance Ion 248.00 (247.70 to 248.70): E

Ion 250.00 (249.70 to 250.70): E

Ion 141.00 (140.70 to 141.70): E









#71
Phenanthrene
Concen: 19.776 ng
RT: 17.42 min Scan# 2438
Delta R.T. -0.02 min
Lab File: BG043644.D
Acq: 14 Nov 2019 21:45




Instrument :
BNA_G
ClientSampleId :
STOCK-PILE


Tot Ion:178 Resp: 241581
Ion Ratio Lower Upper
178 100
176 18.7 15.4 23.0
179 16.2 13.0 19.6



#72
Anthracene
Concen: 19.766 ng
RT: 17.42 min Scan# 2438
Delta R.T. -0.10 min
Lab File: BG043644.D
Acq: 14 Nov 2019 21:45

Tgt Ion:178 Resp: 241581
Ion Ratio Lower Upper
178 100
176 18.7 15.5 23.3
179 16.2 13.7 20.5









#73
 Carbazole
 Concen: 2.187 ng
 RT: 17.79 min Scan# 2501
 Delta R.T. -0.01 min
 Lab File: BG043644.D
 Acq: 14 Nov 2019 21:45




Instrument :
 BNA_G
 ClientSampleId :
 STOCK-PILE


Tot Ion	Ratio	Lower	Upper
167	100		
166	21.8	18.7	28.1
139	13.4	10.0	15.0



#75
 Fluoranthene
 Concen: 29.807 ng
 RT: 19.42 min Scan# 2780
 Delta R.T. -0.02 min
 Lab File: BG043644.D
 Acq: 14 Nov 2019 21:45

Tgt Ion	Ratio	Lower	Upper
202	100		
101	6.1	0.0	26.3
203	18.1	0.0	37.9









#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.64 min Scan# 3157
Delta R.T. -0.02 min
Lab File: BG043644.D
Acq: 14 Nov 2019 21:45

Instrument :
BNA_G
ClientSampleId :
STOCK-PILE

Tot Ion:240 Resp: 258252
Ion Ratio Lower Upper
240 100
120 6.1 4.6 6.8
236 25.0 19.8 29.8




Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E






#77
Benzidine
Concen: 2.429 ng
RT: 19.98 min Scan# 2875
Delta R.T. 0.36 min
Lab File: BG043644.D
Acq: 14 Nov 2019 21:45

Tgt Ion:184 Resp: 12626
Ion Ratio Lower Upper
184 100
185 13.8 11.0 16.4
183 6.5 10.0 15.0#



Abundance Ion 184.00 (183.70 to 184.70): E
Ion 185.00 (184.70 to 185.70): E
Ion 183.00 (182.70 to 183.70): E









#78
Pvrene
Concen: 26.793 ng
RT: 19.79 min Scan# 2842
Delta R.T. -0.01 min
Lab File: BG043644.D
Acq: 14 Nov 2019 21:45




Instrument :
BNA_G
ClientSampleId :
STOCK-PILE


Tot Ion	Ratio	Lower	Upper
202	100		
200	21.4	17.0	25.4
203	17.9	14.7	22.1



#79
Terphenyl-d14
Concen: 56.330 ng
RT: 19.98 min Scan# 2875
Delta R.T. -0.02 min
Lab File: BG043644.D
Acq: 14 Nov 2019 21:45

Tgt Ion	Ratio	Lower	Upper
244	100		
212	7.4	5.8	8.6
122	6.6	5.4	8.2





#81

Benzo(a)anthracene

Concen: 15.552 ng

RT: 21.62 min Scan# 3153

Delta R.T. -0.02 min

Lab File: BG043644.D

Acq: 14 Nov 2019 21:45

Instrument :

BNA_G

ClientSampleId :

STOCK-PILE


Tot Ion:228 Resp: 251573

Ion Ratio Lower Upper

228 100

226 27.5 22.2 33.2




229 21.3 17.0 25.4



Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E



#83

Chrysene

Concen: 14.889 ng

RT: 21.68 min Scan# 3164

Delta R.T. -0.02 min

Lab File: BG043644.D

Acq: 14 Nov 2019 21:45


Tgt Ion:228 Resp: 239308

Ion Ratio Lower Upper

228 100

226 31.9 25.1 37.7



229 23.0 17.0 25.4




Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E









#86
 Indeno(1,2,3-cd)pyrene
 Concen: 10.586 ng
 RT: 28.46 min Scan# 4317
 Delta R.T. -0.04 min
 Lab File: BG043644.D
 Acq: 14 Nov 2019 21:45




Instrument :
 BNA_G
 ClientSampleId :
 STOCK-PILE


Tot Ion:276 Resp: 213570
 Ion Ratio Lower Upper
 276 100
 138 12.3 6.8 10.2#
 277 26.3 20.9 31.3



#87
 Perylene-d12
 Concen: 20.000 ng
 RT: 24.82 min Scan# 3699
 Delta R.T. -0.03 min
 Lab File: BG043644.D
 Acq: 14 Nov 2019 21:45

Tgt Ion:264 Resp: 304634
 Ion Ratio Lower Upper
 264 100
 260 24.4 17.5 26.3
 265 21.9 17.4 26.0









#88
Benzo(b)fluoranthene
Concen: 20.785 ng
RT: 23.81 min Scan# 3527
Delta R.T. -0.03 min
Lab File: BG043644.D
Acq: 14 Nov 2019 21:45




Instrument :
BNA_G
ClientSampleId :
STOCK-PILE


Tot Ion:252 Resp: 358610
Ion Ratio Lower Upper
252 100
253 23.8 17.7 26.5
125 5.6 4.5 6.7



#89
Benzo(k)fluoranthene
Concen: 20.646 ng
RT: 23.81 min Scan# 3527
Delta R.T. -0.09 min
Lab File: BG043644.D
Acq: 14 Nov 2019 21:45

Tgt Ion:252 Resp: 358610
Ion Ratio Lower Upper
252 100
253 23.8 17.3 25.9
125 5.6 4.6 6.8





#90

Benzo(a)pyrene

Concen: 16.720 ng

RT: 24.67 min Scan# 3673

Delta R.T. -0.03 min

Lab File: BG043644.D

Acq: 14 Nov 2019 21:45

Instrument :

BNA_G

ClientSampleId :

STOCK-PILE





Tot Ion:252 Resp: 275484

Ion Ratio Lower Upper

252 100

253 23.2 17.8 26.8

125 6.3 5.4 8.2



#91

Dibenzo(a,h)anthracene

Concen: 2.023 ng

RT: 28.48 min Scan# 4321

Delta R.T. -0.08 min

Lab File: BG043644.D

Acq: 14 Nov 2019 21:45




Tgt Ion:278 Resp: 34089


Ion Ratio Lower Upper

278 100

139 9.9 7.4 11.0

279 24.4 19.1 28.7





#92
 Benzo(a,h,i)perylene
 Concen: 12.750 ng
 RT: 29.58 min Scan# 4509
 Delta R.T. -0.05 min
 Lab File: BG043644.D
 Acq: 14 Nov 2019 21:45

Instrument :
 BNA_G
 ClientSampleId :
 STOCK-PILE

Tot Ion	Ratio	Lower	Upper
276	100		
277	22.5	18.9	28.3
138	11.4	8.9	13.3

