

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG111419\
 Data File : BG043638.D
 Acq On : 14 Nov 2019 17:52
 Operator : JU
 Sample : K5832-10
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 8-(8-10)

Quant Time: Nov 15 03:23:14 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG102119.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 04 15:22:15 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.99	152	28995	20.00	ng	-0.01
21) Naphthalene-d8	10.80	136	111970	20.00	ng	-0.01
39) Acenaphthene-d10	14.63	164	84688	20.00	ng	-0.01
64) Phenanthrene-d10	17.37	188	201680	20.00	ng	-0.02
76) Chrysene-d12	21.64	240	211943	20.00	ng	-0.02
87) Perylene-d12	24.82	264	250533	20.00	ng	-0.03
System Monitoring Compounds						
5) 2-Fluorophenol	5.59	112	237221	149.92	ng	0.00
7) Phenol-d6	7.20	99	336859	147.97	ng	0.00
23) Nitrobenzene-d5	9.16	82	202030	93.02	ng	-0.01
42) 2,4,6-Tribromophenol	16.12	330	192878	119.68	ng	-0.01
45) 2-Fluorobiphenyl	13.25	172	521879	85.15	ng	-0.01
79) Terphenyl-d14	19.99	244	977640	86.54	ng	-0.01
Target Compounds						
10) Phenol	7.22	94	10170	4.889	ng	Qvalue # 72
50) Dimethylphthalate	14.08	163	85342	13.010	ng	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG111419\
Data File : BG043638.D
Acq On : 14 Nov 2019 17:52
Operator : JU
Sample : K5832-10
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
8-(8-10)

Quant Time: Nov 15 03:23:14 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG102119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 04 15:22:15 2019
Response via : Initial Calibration

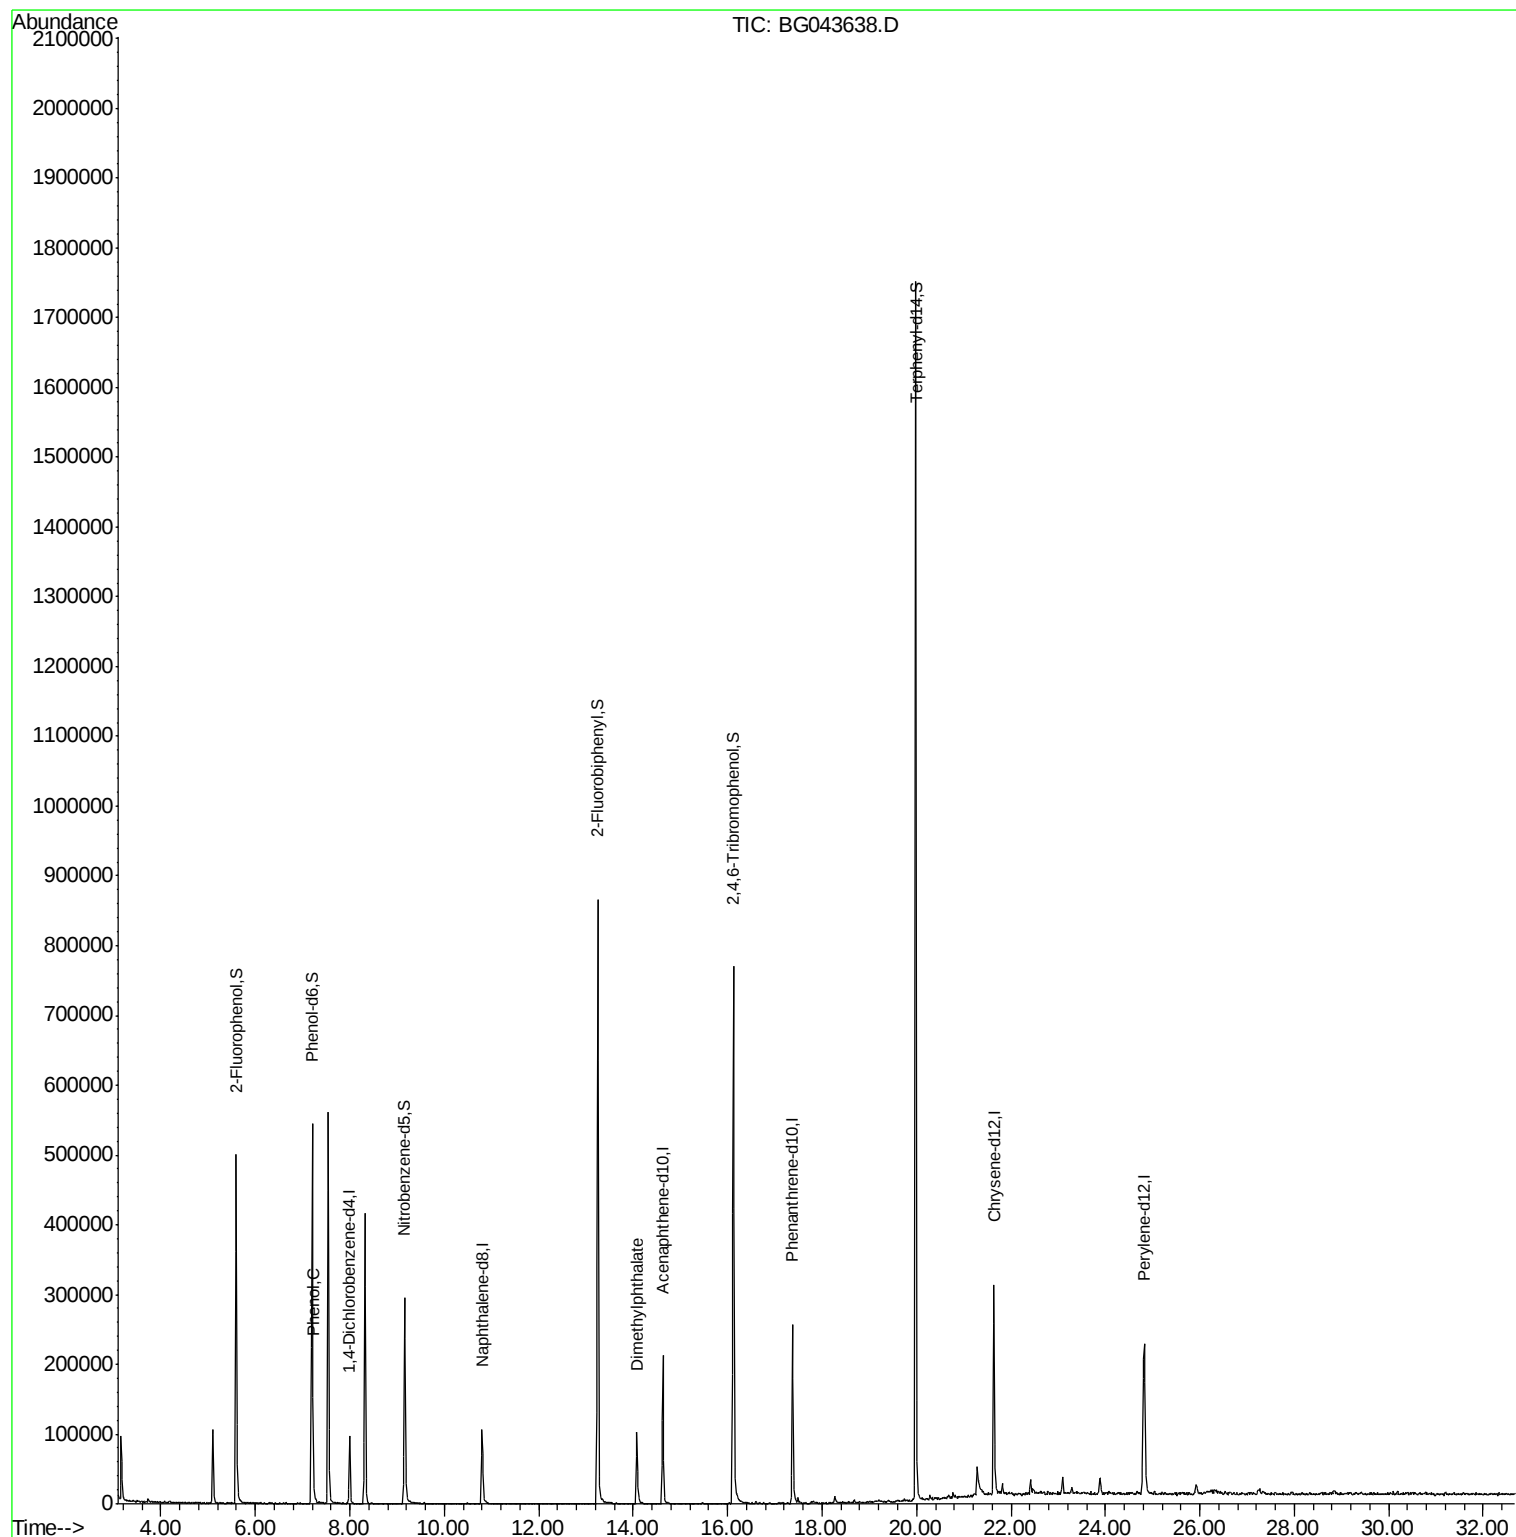




#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.99 min Scan# 835
Delta R.T. -0.01 min
Lab File: BG043638.D
Acq: 14 Nov 2019 17:52

Instrument :
BNA_G
ClientSampleId :
8-(8-10)

Tot Ion:152 Resp: 28995
Ion Ratio Lower Upper
152 100
150 140.4 129.4 194.0
115 61.9 48.8 73.2

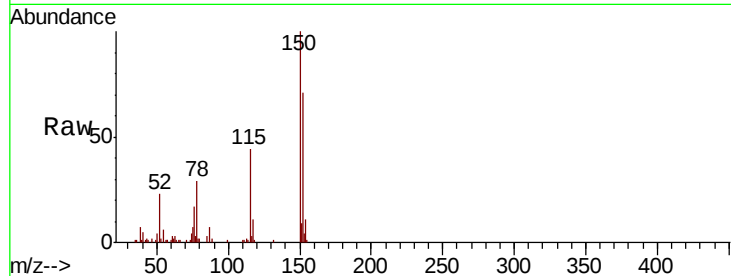


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

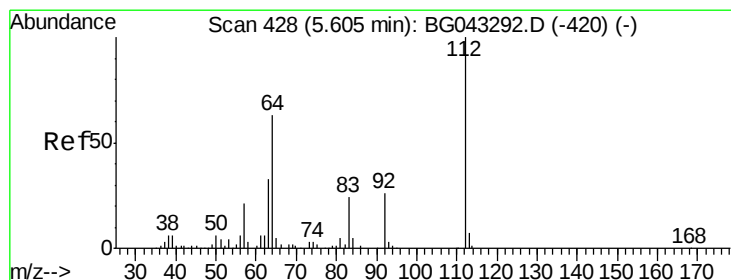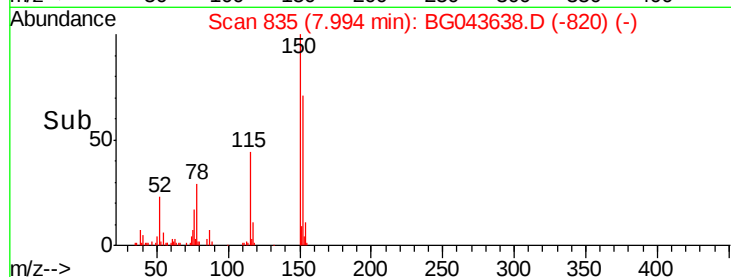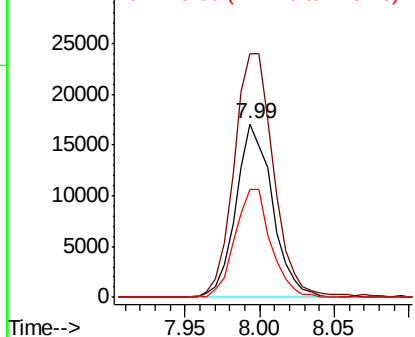



#5


2-Fluorophenol
Concen: 149.921 ng
RT: 5.59 min Scan# 426
Delta R.T. -0.00 min
Lab File: BG043638.D
Acq: 14 Nov 2019 17:52

Tgt Ion:112 Resp: 237221
Ion Ratio Lower Upper
112 100
64 59.9 50.0 75.0
63 36.0 26.6 40.0



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BG
Ion 63.00 (62.70 to 63.70): BG

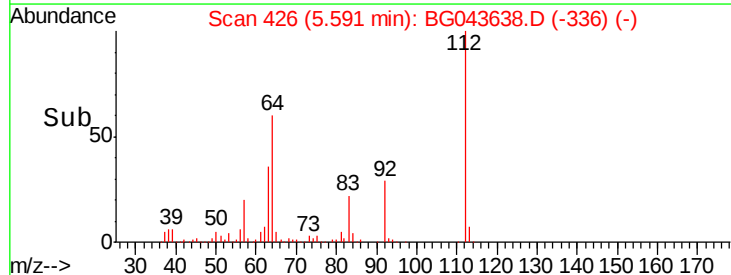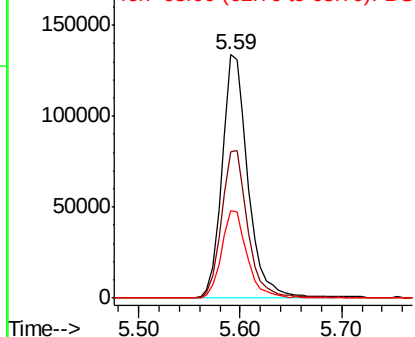

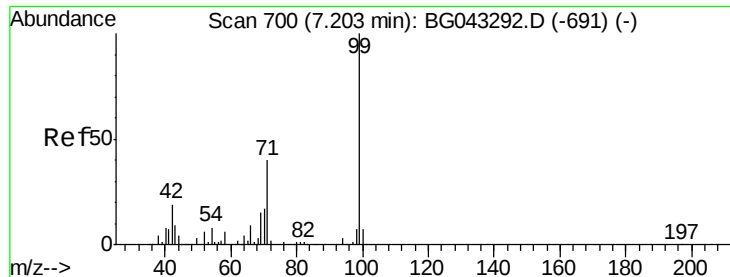

#7

Phenol-d6

Concen: 147.968 ng

RT: 7.20 min Scan# 700

Delta R.T. 0.00 min

Lab File: BG043638.D

Acq: 14 Nov 2019 17:52

Instrument :

BNA_G

ClientSampleId :

8-(8-10)


Tot Ion: 99 Resp: 336859

Ion Ratio Lower Upper




99 100

42 18.4 14.6 21.8

71 39.9 32.5 48.7

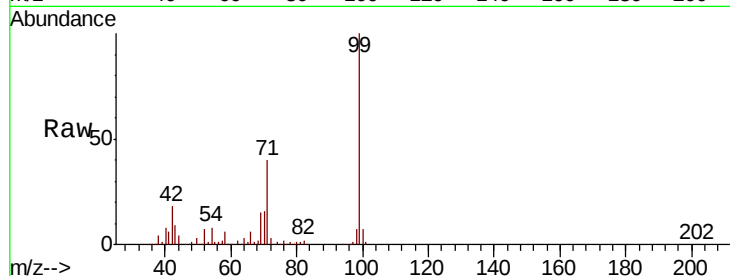

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

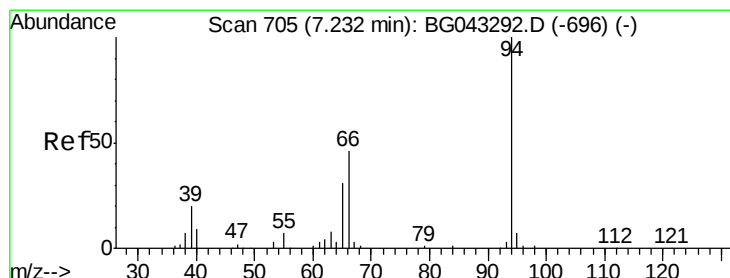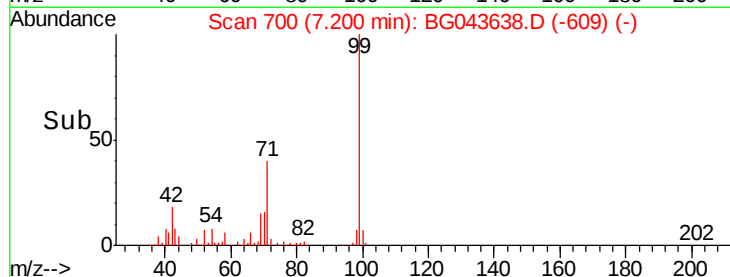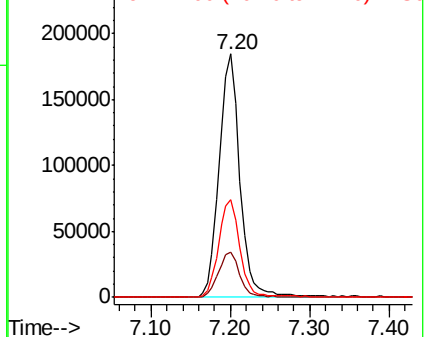

#10

Phenol

Concen: 4.889 ng

RT: 7.22 min Scan# 704

Delta R.T. 0.00 min

Lab File: BG043638.D

Acq: 14 Nov 2019 17:52


Tgt Ion: 94 Resp: 10170

Ion Ratio Lower Upper



94 100

65 39.7 12.6 52.6

66 76.8 30.7 70.7#

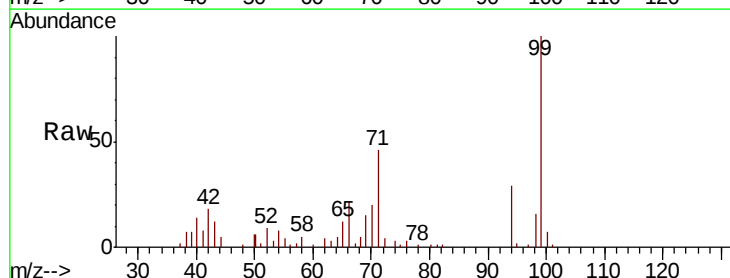

Abundance Ion 94.00 (93.70 to 94.70): BGC
Ion 65.00 (64.70 to 65.70): BGC
Ion 66.00 (65.70 to 66.70): BGC

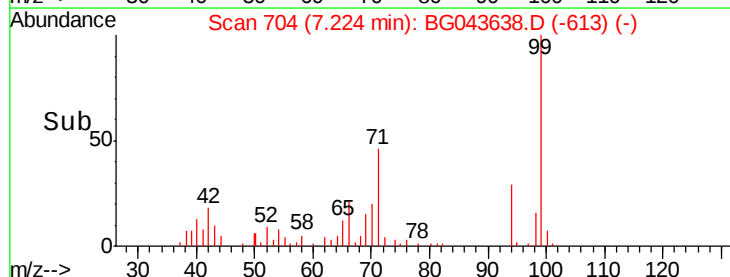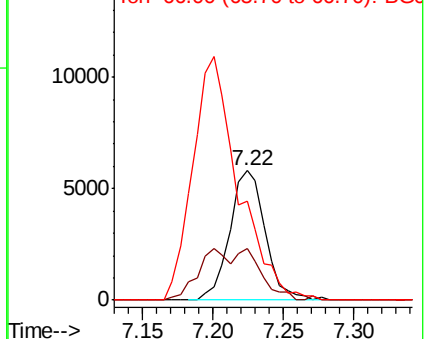







#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.80 min Scan# 1313
Delta R.T. -0.01 min
Lab File: BG043638.D
Acq: 14 Nov 2019 17:52

Instrument :
BNA_G
ClientSampleId :
8-(8-10)

Tot Ion:136	Resp:	111970
Ion	Ratio	Lower Upper
136	100	
137	9.5	8.7 13.1
54	7.1	5.4 8.2
68	2.9	3.0 4.4#

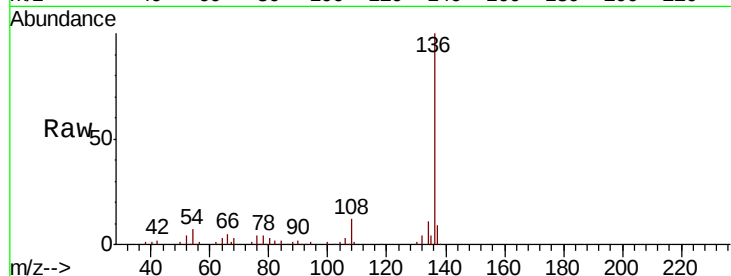


Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC

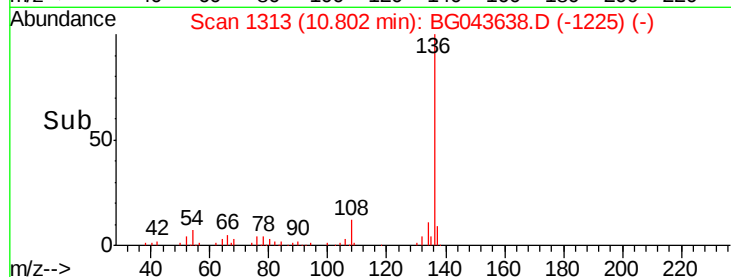
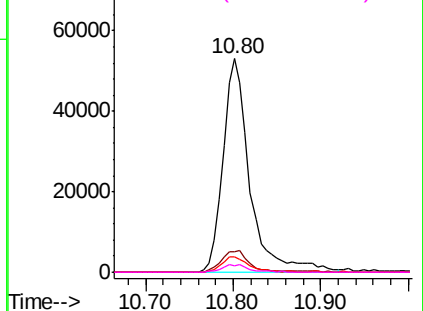



#23
Nitrobenzene-d5
Concen: 93.021 ng
RT: 9.16 min Scan# 1034
Delta R.T. -0.01 min
Lab File: BG043638.D
Acq: 14 Nov 2019 17:52

Tgt Ion: 82	Resp:	202030
Ion	Ratio	Lower Upper
82	100	
128	44.0	35.0 52.6
54	52.4	40.2 60.2



Abundance Ion 82.00 (81.70 to 82.70): BGC
Ion 128.00 (127.70 to 128.70): BGC
Ion 54.00 (53.70 to 54.70): BGC



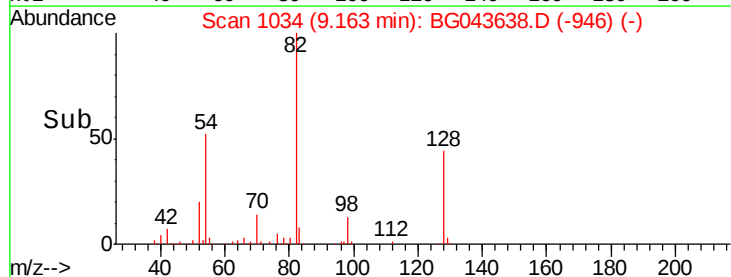
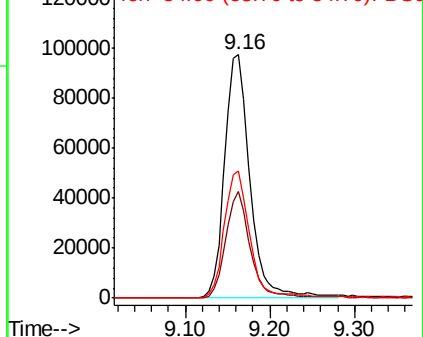


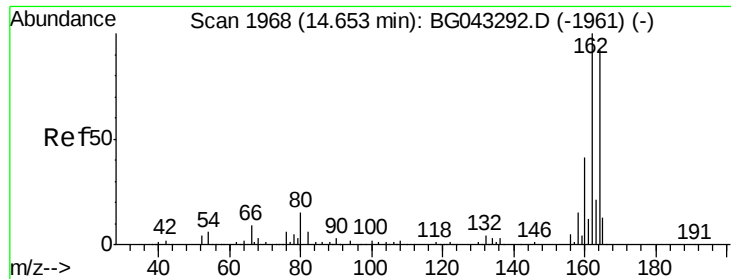

#39
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 14.63 min Scan# 1964
 Delta R.T. -0.01 min
 Lab File: BG043638.D
 Acq: 14 Nov 2019 17:52




Instrument :
 BNA_G
 ClientSampleId :
 8-(8-10)


Tot Ion:164 Resp: 84688
 Ion Ratio Lower Upper
 164 100
 162 102.5 83.5 125.3
 160 46.6 36.5 54.7

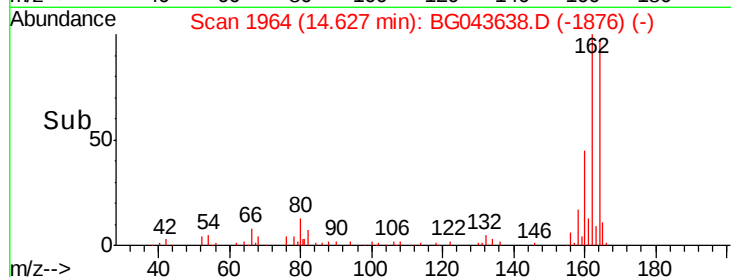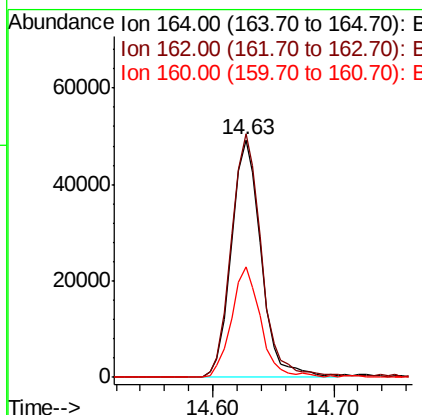

#42
 2,4,6-Tribromophenol
 Concen: 119.680 ng
 RT: 16.12 min Scan# 2218
 Delta R.T. -0.01 min
 Lab File: BG043638.D
 Acq: 14 Nov 2019 17:52

Tgt Ion:330 Resp: 192878
 Ion Ratio Lower Upper
 330 100
 332 98.0 77.4 116.0
 141 29.2 22.8 34.2

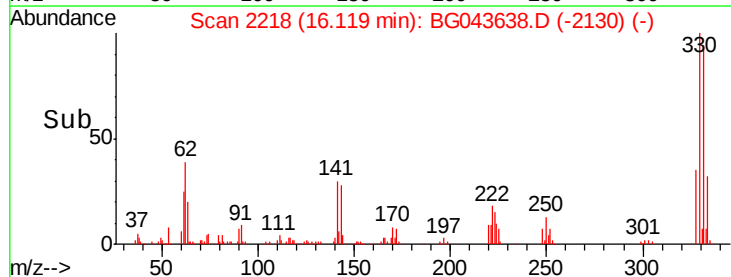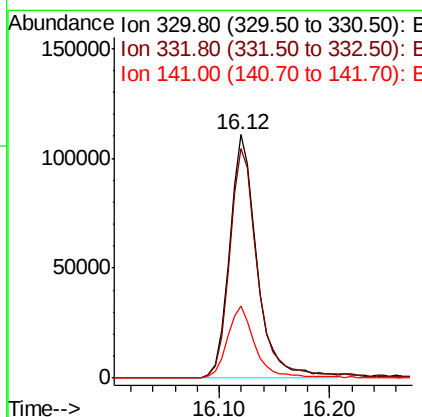

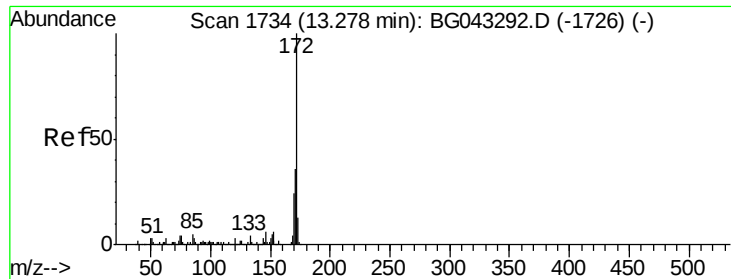

#45

2-Fluorobiphenyl

Concen: 85.152 ng

RT: 13.25 min Scan# 1730

Delta R.T. -0.01 min

Lab File: BG043638.D

Acq: 14 Nov 2019 17:52

Instrument :

BNA_G

ClientSampleId :

8-(8-10)


Tot Ion:172 Resp: 521879

Ion Ratio Lower Upper

172 100

171 34.5 28.9 43.3




170 22.8 18.5 27.7



Abundance Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

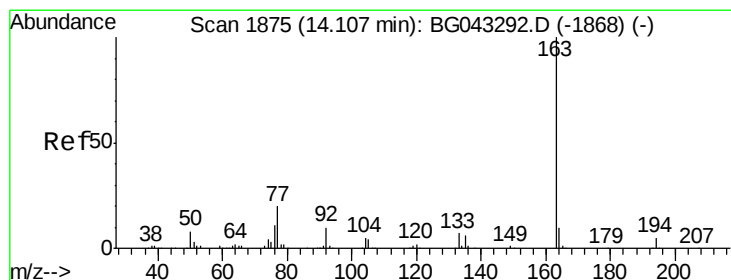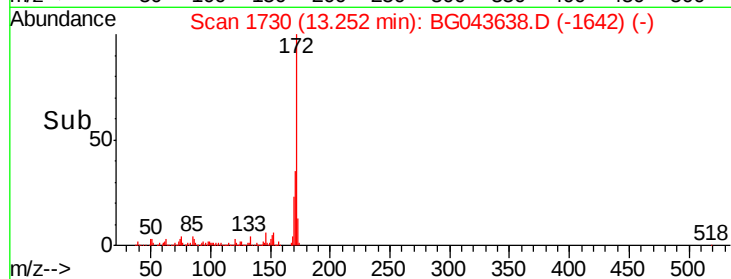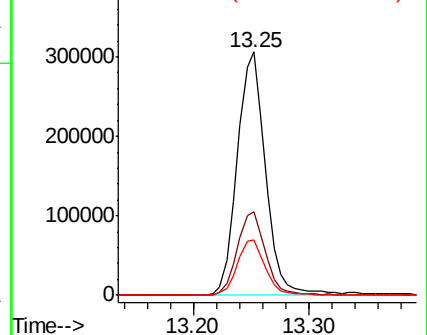

#50

Dimethylphthalate

Concen: 13.010 ng

RT: 14.08 min Scan# 1871

Delta R.T. -0.01 min

Lab File: BG043638.D

Acq: 14 Nov 2019 17:52


Tgt Ion:163 Resp: 85342

Ion Ratio Lower Upper

163 100

194 4.5 3.8 5.6



164 12.0 8.9 13.3

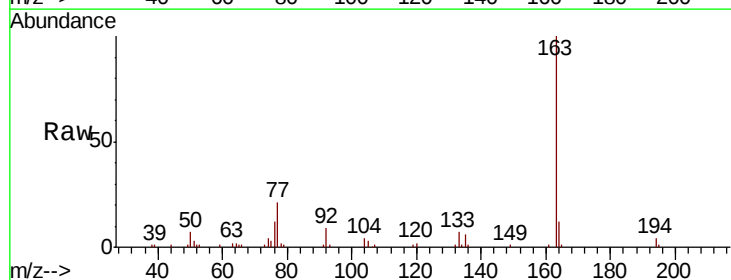

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

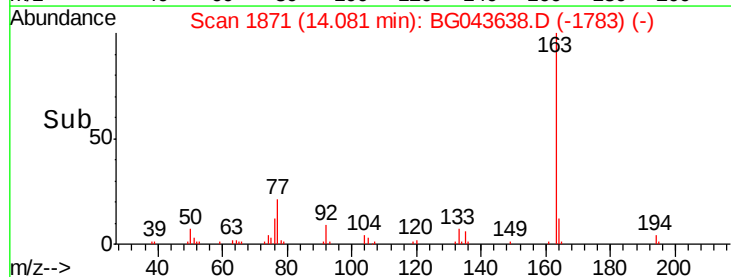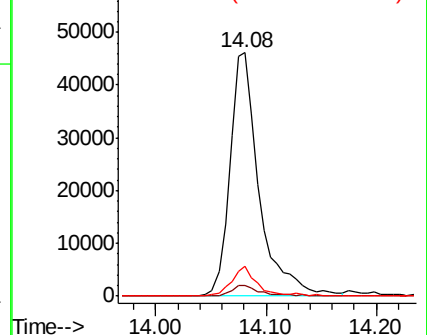







#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.37 min Scan# 2431
Delta R.T. -0.02 min
Lab File: BG043638.D
Acq: 14 Nov 2019 17:52

Instrument :
BNA_G
ClientSampleId :
8-(8-10)

Tot Ion	Ratio	Lower	Upper
188	100		
94	6.1	4.2	6.4
80	6.5	4.5	6.7




Abundance Ion 188.00 (187.70 to 188.70): E
150000
Ion 94.00 (93.70 to 94.70): BG
Ion 80.00 (79.70 to 80.70): BG

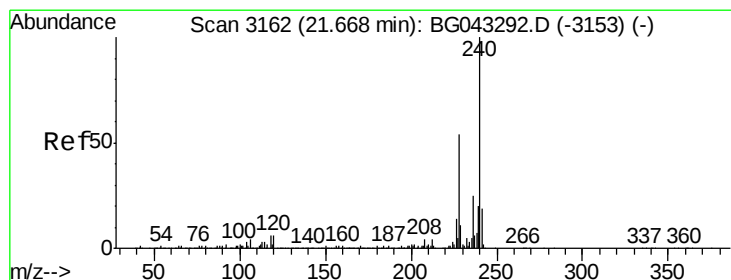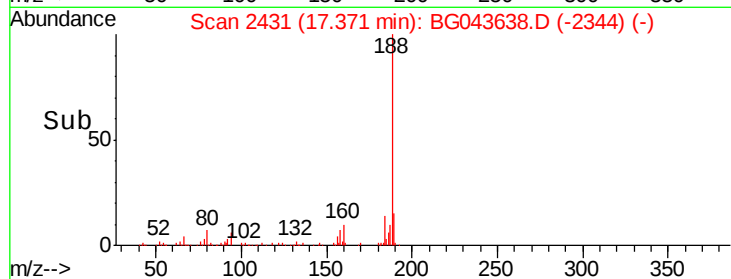
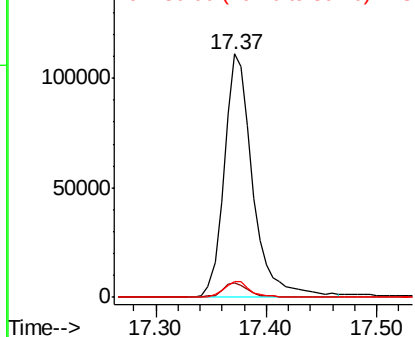



#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.64 min Scan# 3157
Delta R.T. -0.02 min
Lab File: BG043638.D
Acq: 14 Nov 2019 17:52

Tgt Ion	Ratio	Lower	Upper
240	100		
120	6.6	4.6	6.8
236	23.6	19.8	29.8

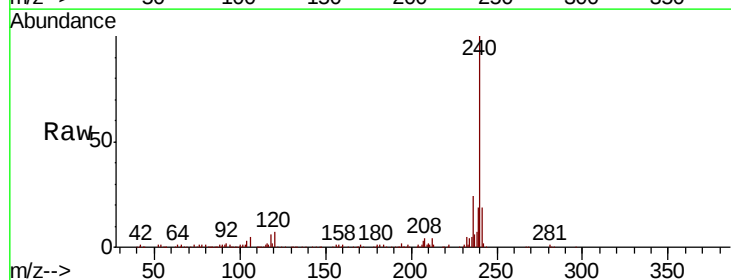

Abundance Ion 240.00 (239.70 to 240.70): E
150000
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

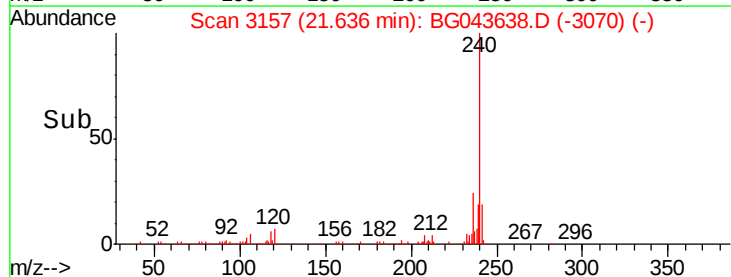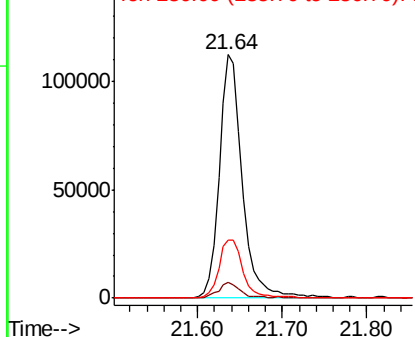

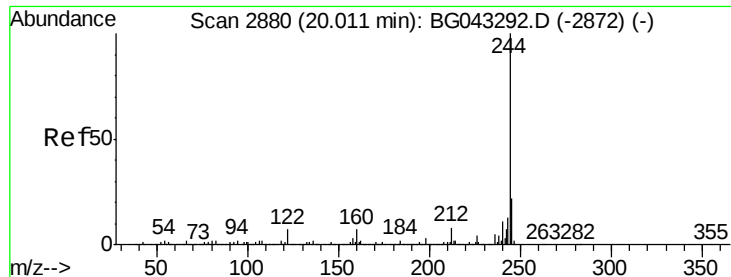

#79

Terphenyl-d14

Concen: 86.538 ng

RT: 19.99 min Scan# 2876

Delta R.T. -0.01 min

Lab File: BG043638.D

Acq: 14 Nov 2019 17:52

Instrument :


BNA_G

ClientSampleId :

8-(8-10)

Tot Ion:244 Resp: 977640

Ion	Ratio	Lower	Upper
244	100		
212	7.2	5.8	8.6
122	6.6	5.4	8.2






Abundance

Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

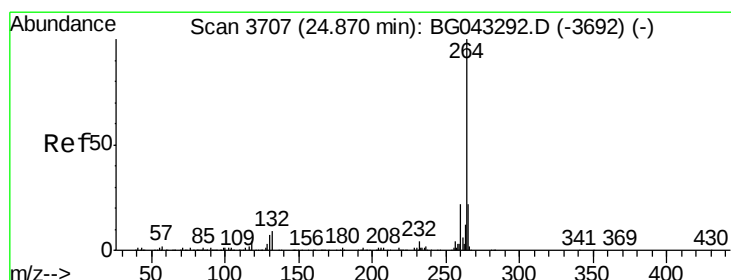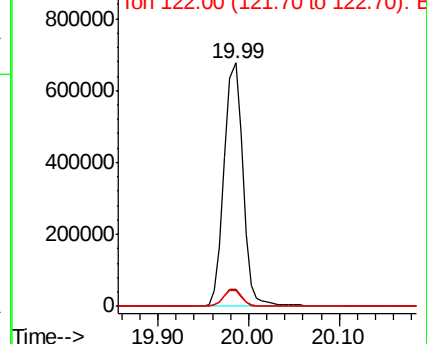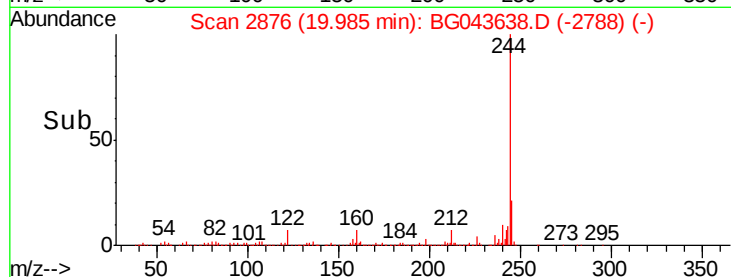

#87

Perylene-d12

Concen: 20.000 ng

RT: 24.82 min Scan# 3699


Delta R.T. -0.03 min

Lab File: BG043638.D

Acq: 14 Nov 2019 17:52

Tgt Ion:264 Resp: 250533

Ion	Ratio	Lower	Upper
264	100		
260	23.9	17.5	26.3
265	21.9	17.4	26.0



Abundance

Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

