
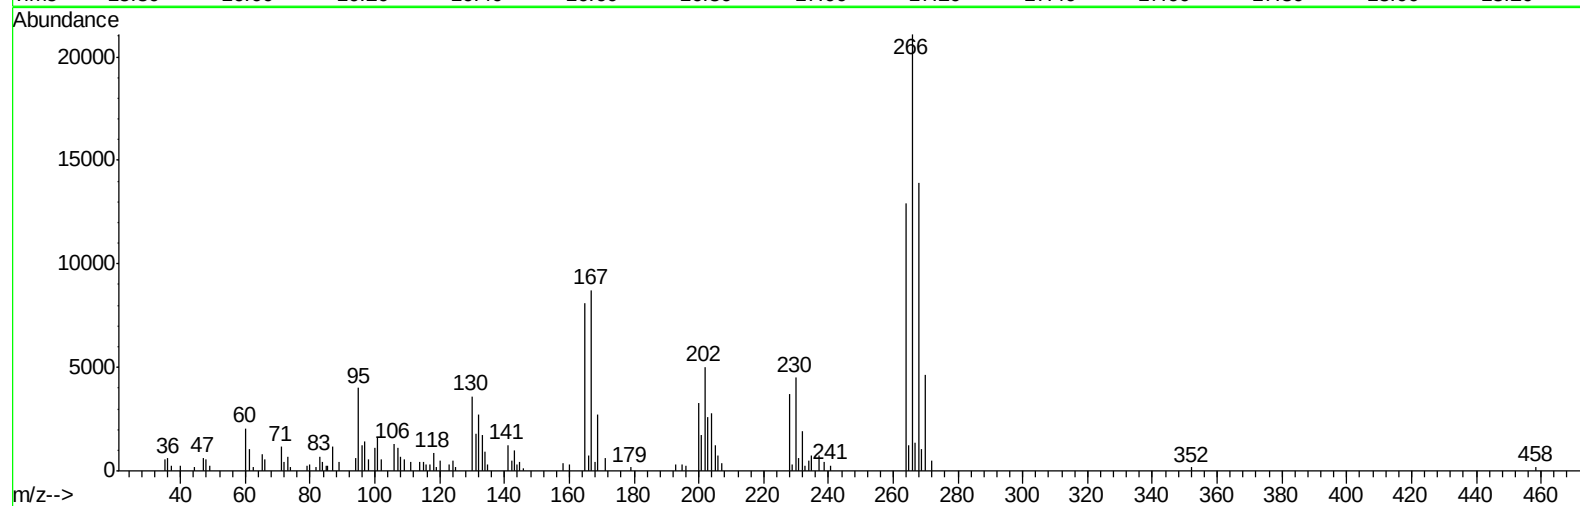


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG111419\
Data File : BG043647.D
Acq On : 15 Nov 2019 4:41
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 15 08:07:32 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG102119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 04 15:22:15 2019
Response via : Initial Calibration

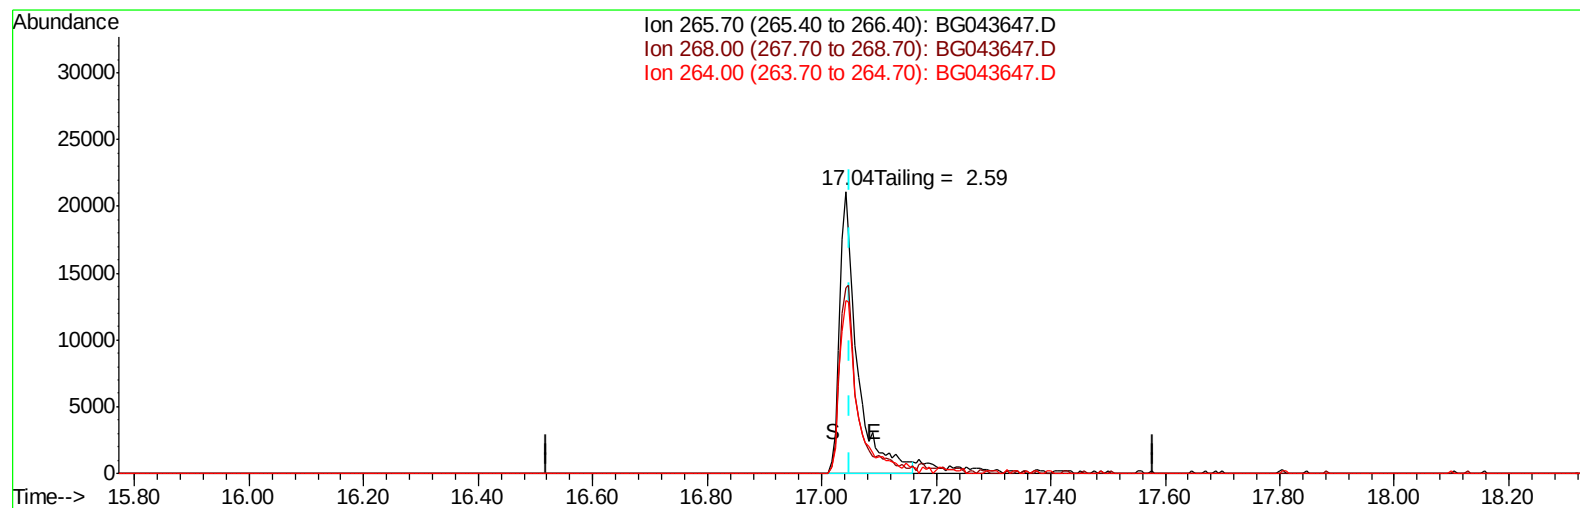

TIC: BG043647.D

(70) Pentachlorophenol (C)



17.041min (-0.009) 18613.51ng

response 45071

Ion	Exp%	Act%
265.70	100	100
268.00	63.00	66.02
264.00	61.10	61.25
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG111419\
 Data File : BG043647.D
 Acq On : 15 Nov 2019 4:41
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 15 08:07:32 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG102119.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 04 15:22:15 2019
 Response via : Initial Calibration

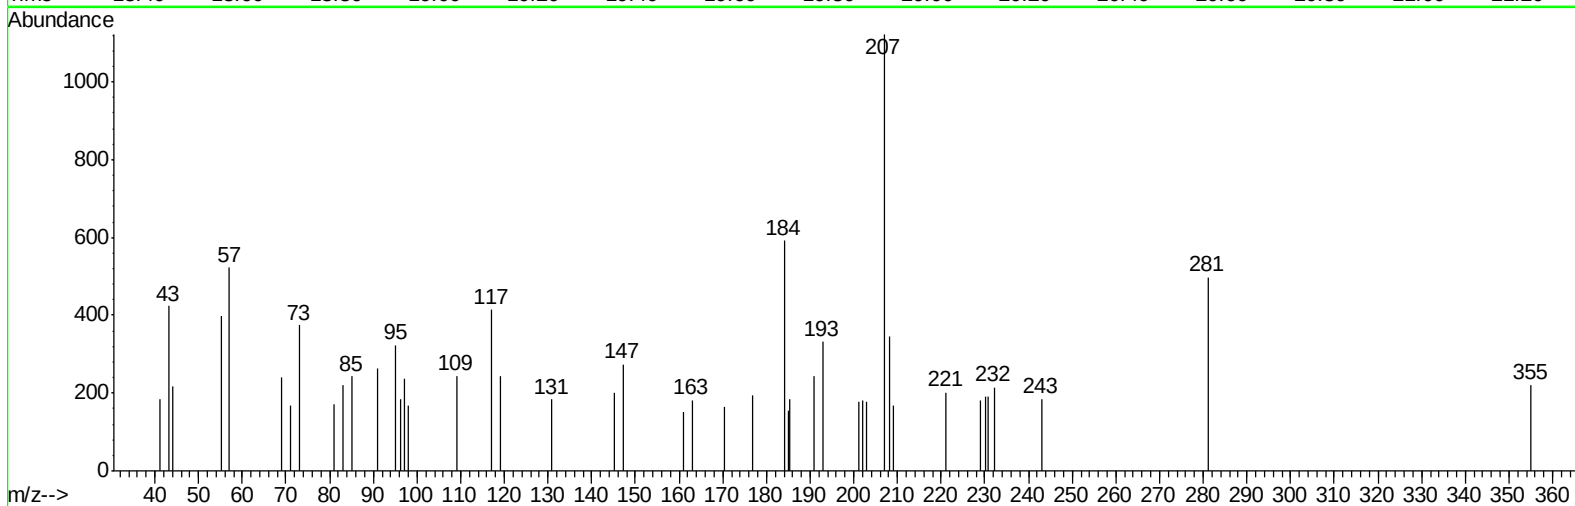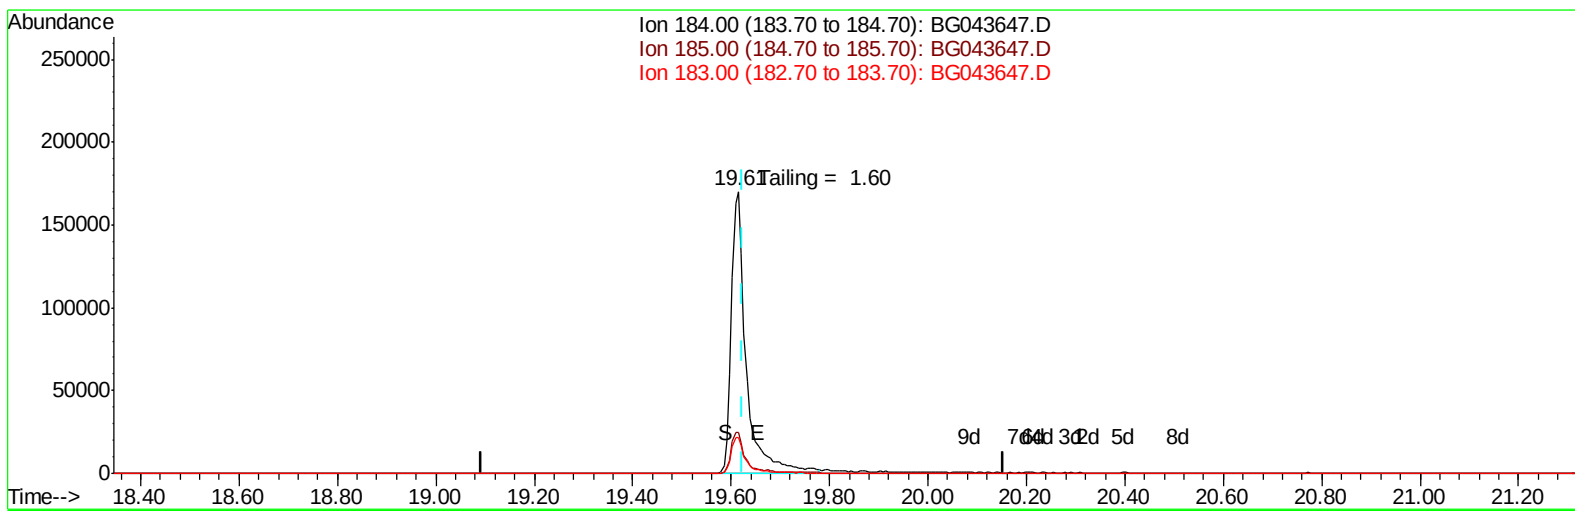

TIC: BG043647.D

(77) Benzidine

20.308min (+0.685) 168.00ng

response 213

Ion	Exp%	Act%
184.00	100	100
185.00	13.70	57.26#
183.00	12.50	0.00#
0.00	0.00	0.00