


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG111419\
 Data File : BG043628.D
 Acq On : 14 Nov 2019 11:19
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG102119.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Nov 04 15:22:15 2019

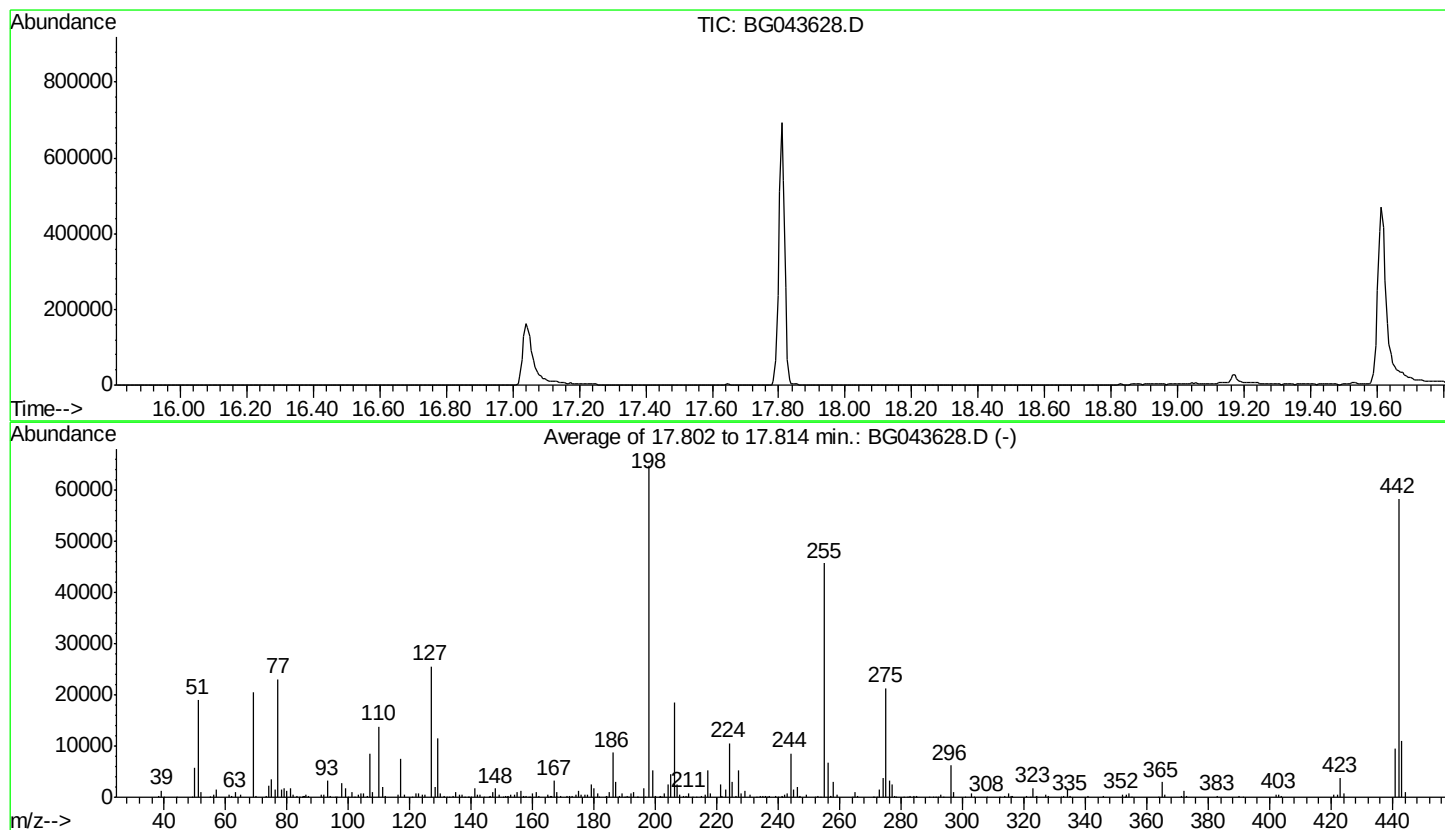

AutoFind: Scans 2504, 2505, 2506; Background Corrected with Scan 2498

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.5	19067	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	31.7	20485	PASS
70	69	0.00	2	0.7	147	PASS
127	198	10	80	39.4	25512	PASS
197	198	0.00	2	0.2	101	PASS
198	198	100	100	100.0	64696	PASS
199	198	5	9	8.1	5228	PASS
275	198	10	60	33.0	21320	PASS
365	198	1	100	4.6	2970	PASS
441	198	0.01	100	14.5	9403	PASS
442	198	50	100	89.9	58194	PASS
443	442	15	24	18.7	10907	PASS