
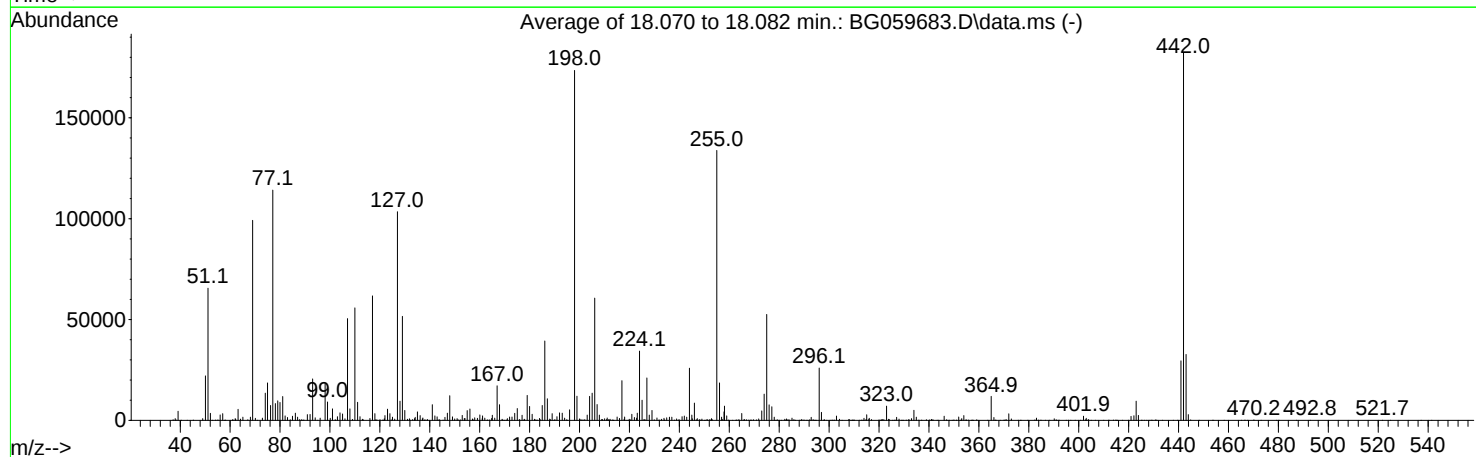


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111423\
 Data File : BG059683.D
 Acq On : 14 Nov 2023 16:01
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111423.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Nov 15 08:14:53 2023

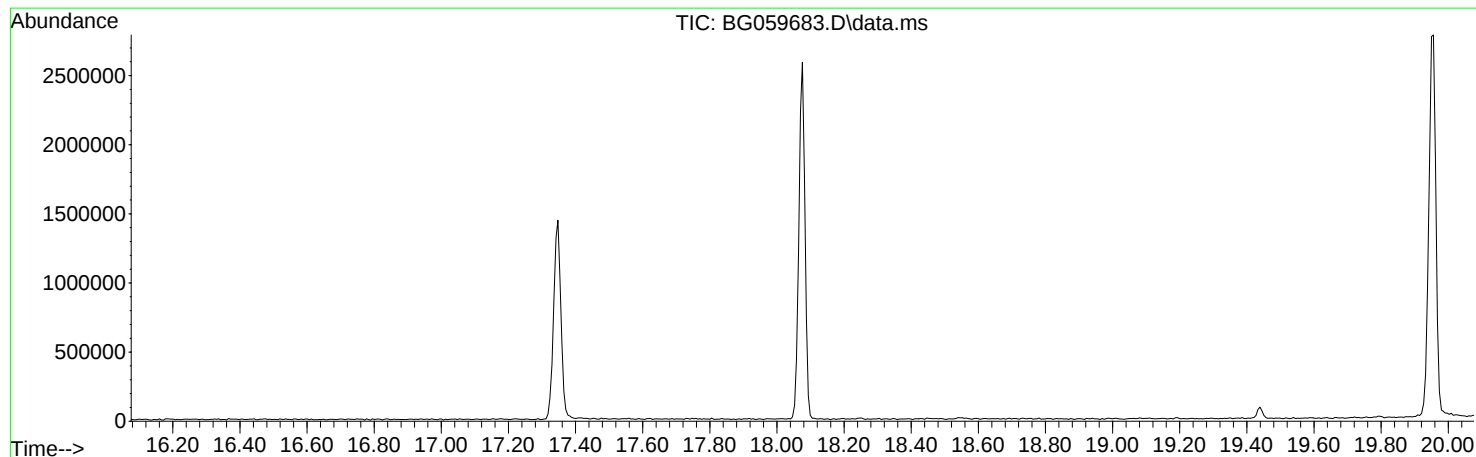




AutoFind: Scans 2499, 2500, 2501; Background Corrected with Scan 2492

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.7	65507	PASS
68	69	0.00	2	1.6	1610	PASS
69	198	0.00	100	57.2	99211	PASS
70	69	0.00	2	1.0	1008	PASS
127	198	10	80	59.6	103459	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	173547	PASS
199	198	5	9	6.9	12021	PASS
275	198	10	60	30.3	52565	PASS
365	198	1	100	6.9	11895	PASS
441	198	0.01	100	17.0	29512	PASS
442	442	50	100	100.0	182400	PASS
443	442	15	24	17.9	32688	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111423\
Data File : BG059683.D
Acq On : 14 Nov 2023 16:01
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Nov 15 07:27:32 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111423.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 15 07:19:07 2023
Response via : Initial Calibration

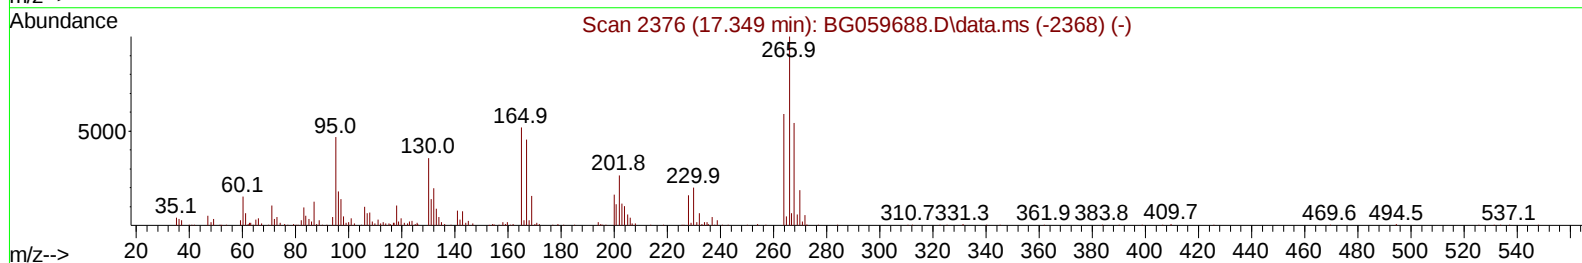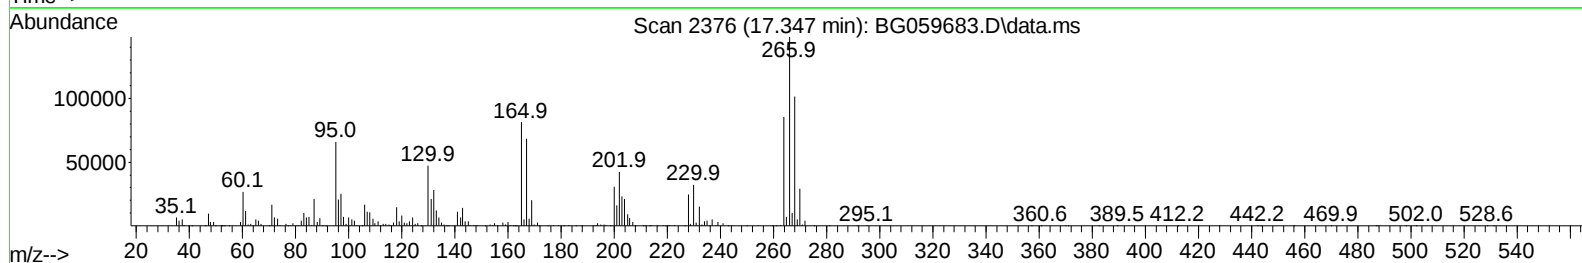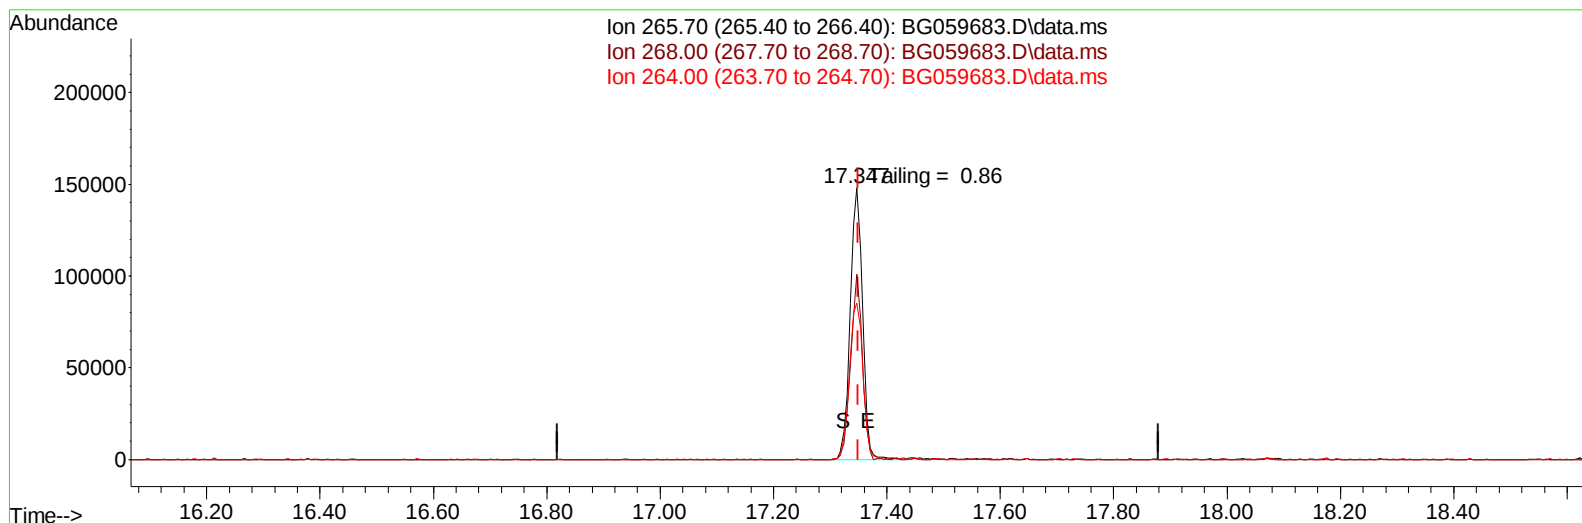

TIC: BG059683.D\data.ms

(70) Pentachlorophenol (C)

17.347min (-0.002) 175282.37 ng




response 223027

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	54.30	68.38#
264.00	59.10	57.65
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111423\
Data File : BG059683.D
Acq On : 14 Nov 2023 16:01
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Nov 15 07:27:32 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111423.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 15 07:19:07 2023
Response via : Initial Calibration

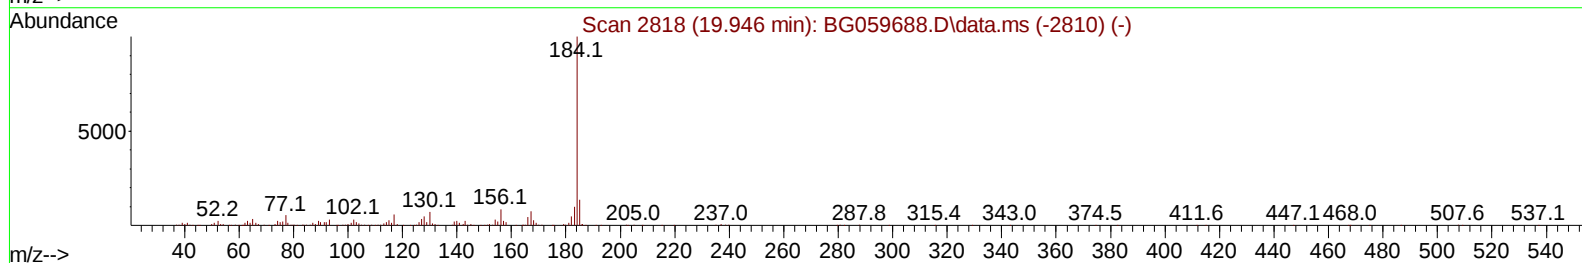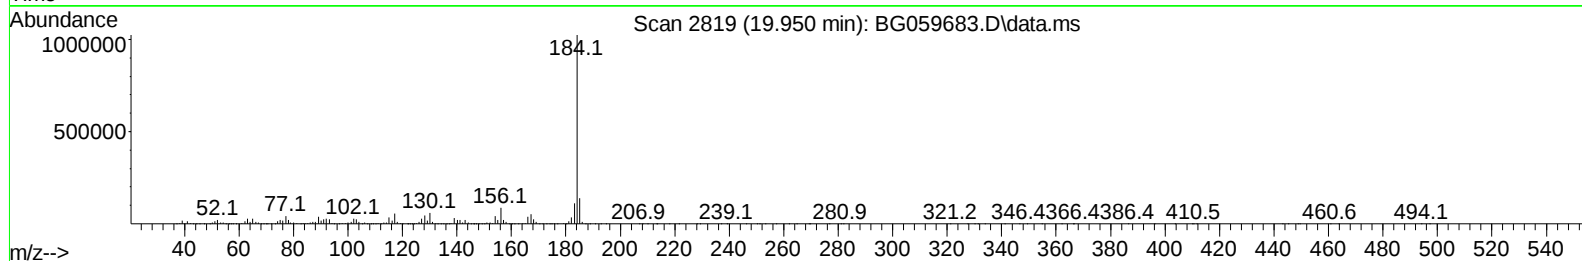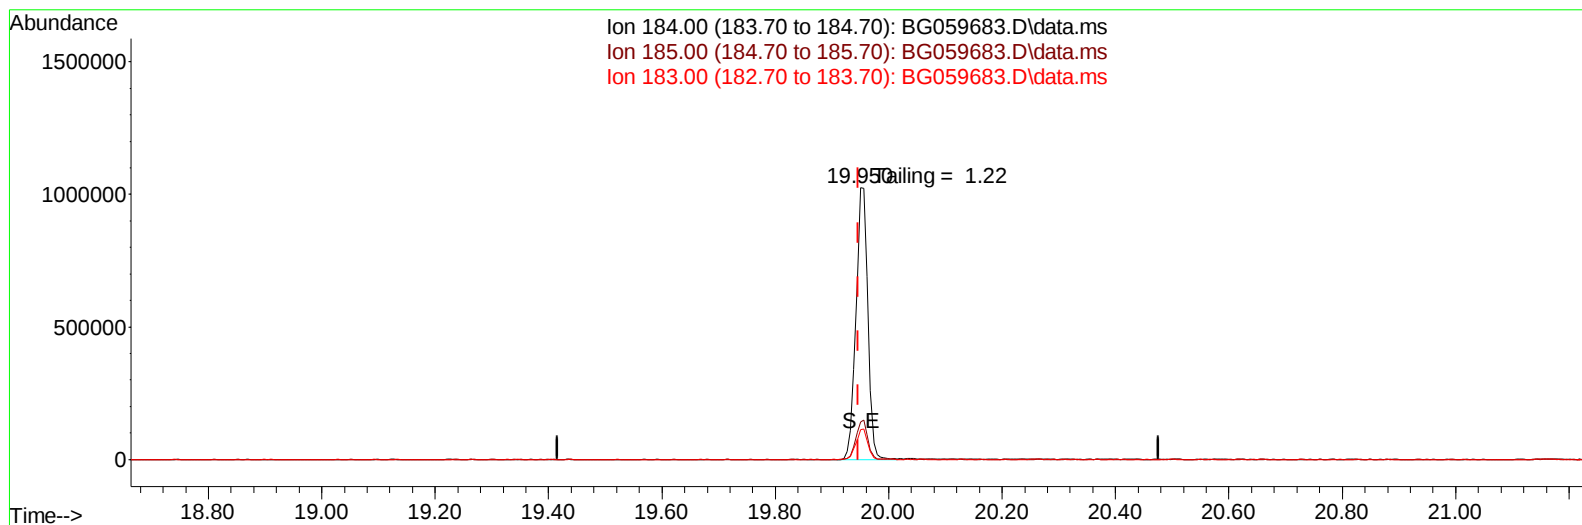

TIC: BG059683.D\data.ms

(77) Benzidine

19.950min (+ 0.004) 309124.51 ng

response 1504306

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	13.74
183.00	9.70	10.93
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/14/2023	BNA_G	<u>BG059683.D</u>
Compound Name	Response	Retention Time
DDT	542812	21.166
DDD	8469	20.761
DDE	0	20.146
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8469	551281	1.54

Instrument :
BNA_G
ClientSampleId :
DFTPP