


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111425\
Data File : BG064773.D
Acq On : 14 Nov 2025 9:37
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111225.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Nov 12 17:10:56 2025

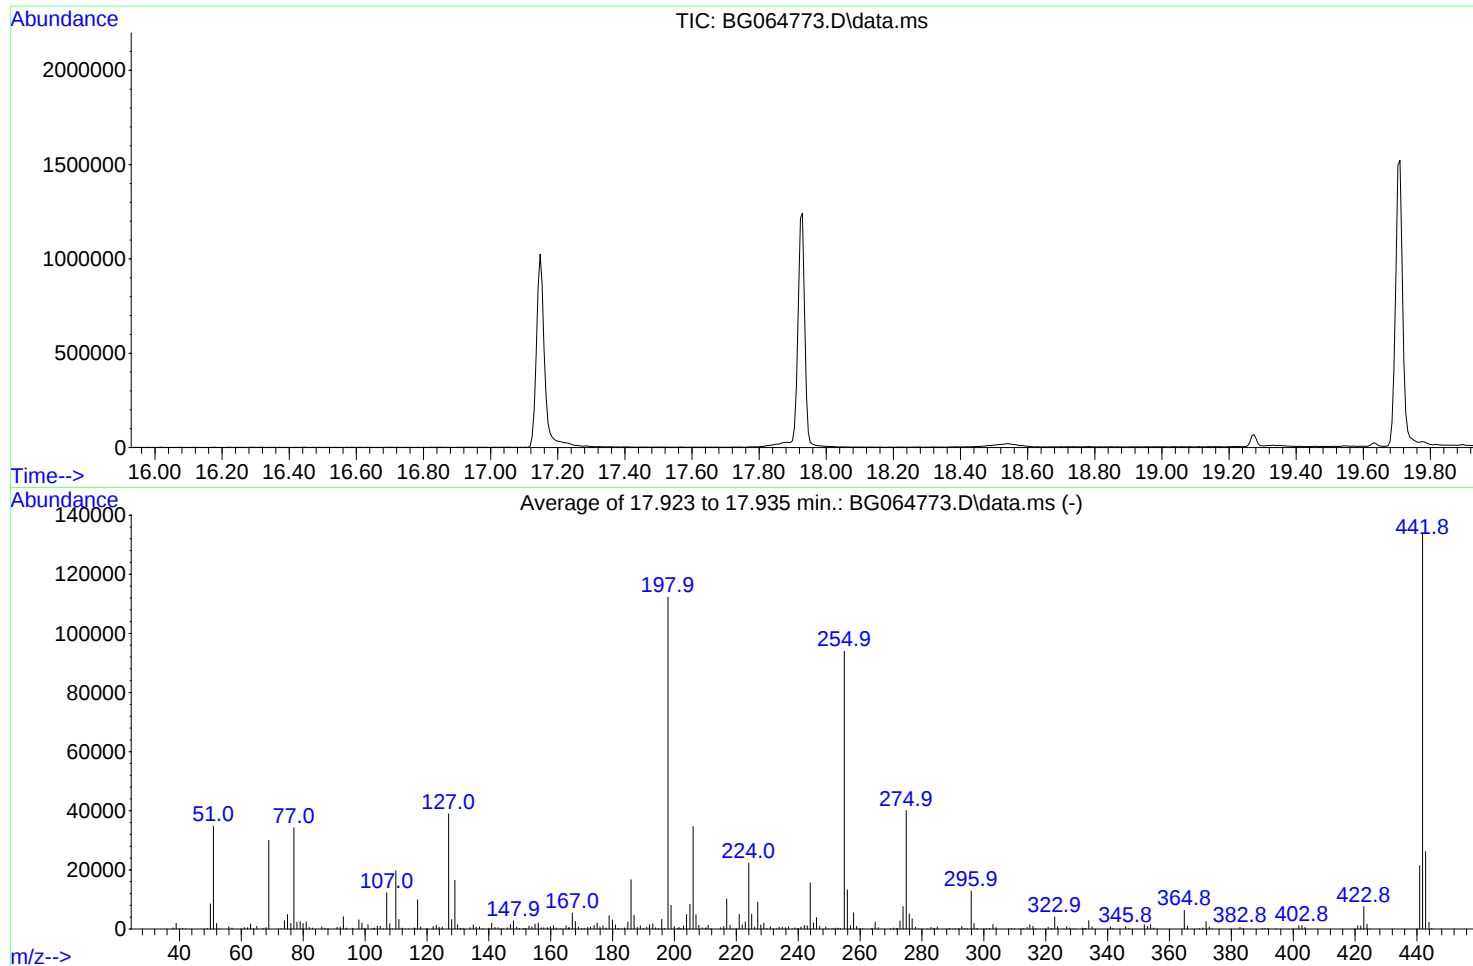

AutoFind: Scans 2525, 2526, 2527; Background Corrected with Scan 2518

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	1.7	501	PASS
69	69	100	100	100.0	29973	PASS
70	69	0.00	2	0.0	0	PASS
197	198	0.00	2	0.2	216	PASS
198	198	100	100	100.0	112261	PASS
199	198	5	9	7.1	7992	PASS
365	198	1	100	5.6	6305	PASS
441	443	0.01	150	82.0	21445	PASS
442	442	100	100	100.0	133571	PASS
443	442	15	24	19.6	26168	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
11/14/2025	BNA_G	<u>BG064773.D</u>
Compound Name	Response	Retention Time
DDT	614510	20.937
DDD	13122	20.496
DDE	69	19.274
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
13191	627701	2.10

Instrument :
BNA_G
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111425\
Data File : BG064773.D
Acq On : 14 Nov 2025 9:37
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Nov 14 10:26:10 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 12 17:10:56 2025
Response via : Initial Calibration

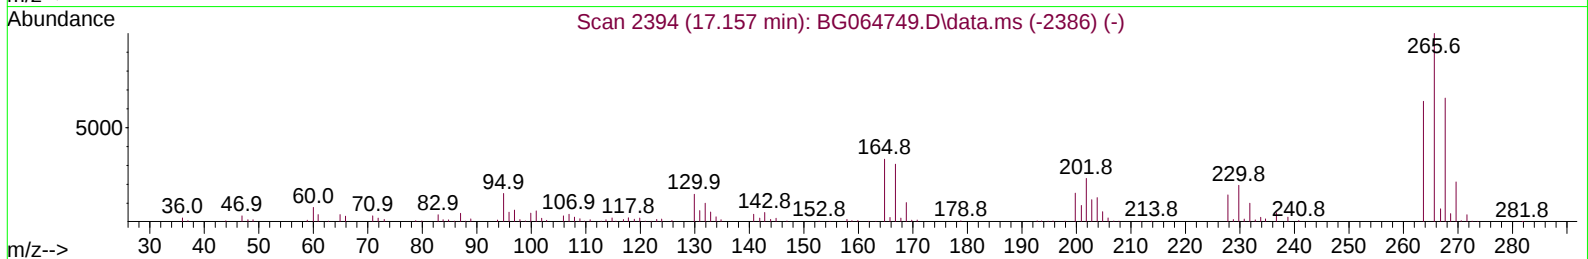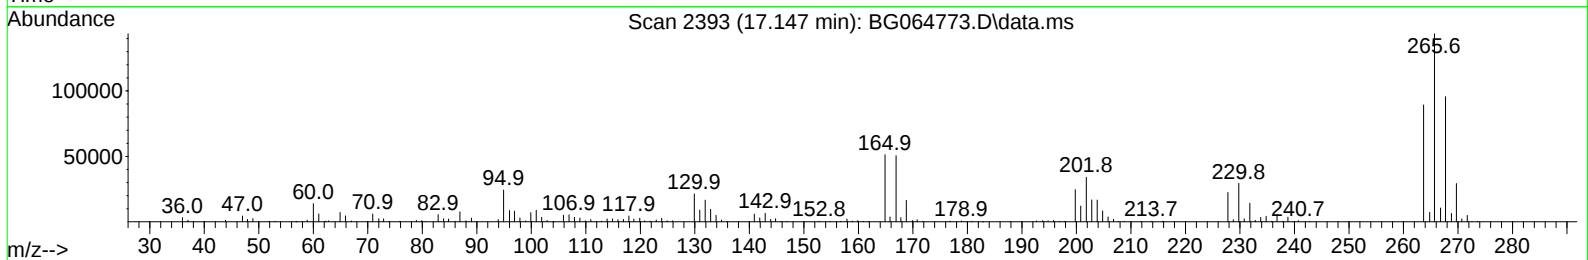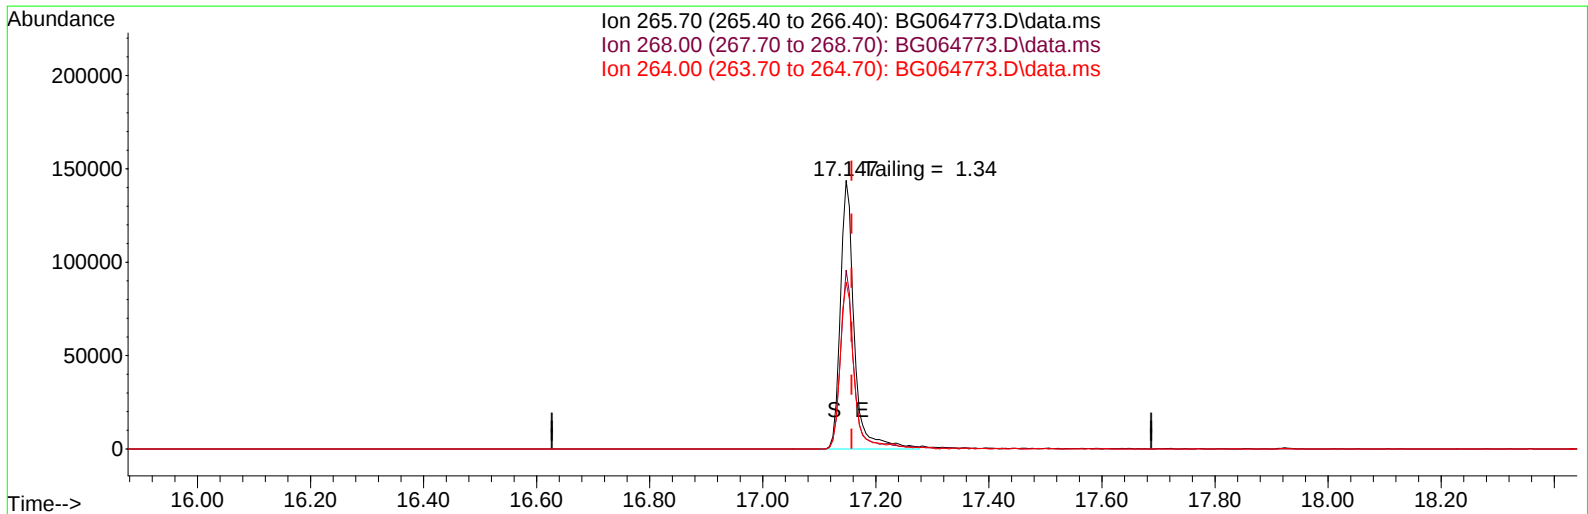

TIC: BG064773.D\data.ms

(70) Pentachlorophenol (C)

17.147min (-0.010) 408516.59 ng




response 245802

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	70.10	66.57
264.00	64.00	62.10
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111425\
Data File : BG064773.D
Acq On : 14 Nov 2025 9:37
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Nov 14 10:26:10 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 12 17:10:56 2025
Response via : Initial Calibration

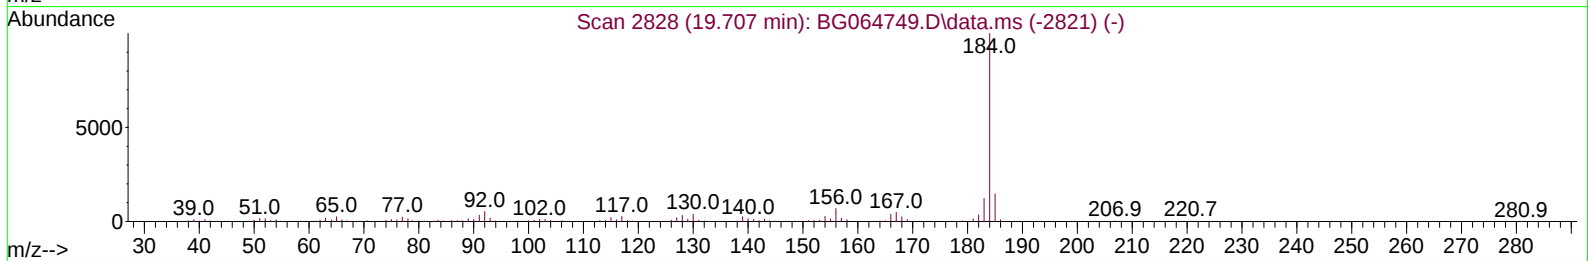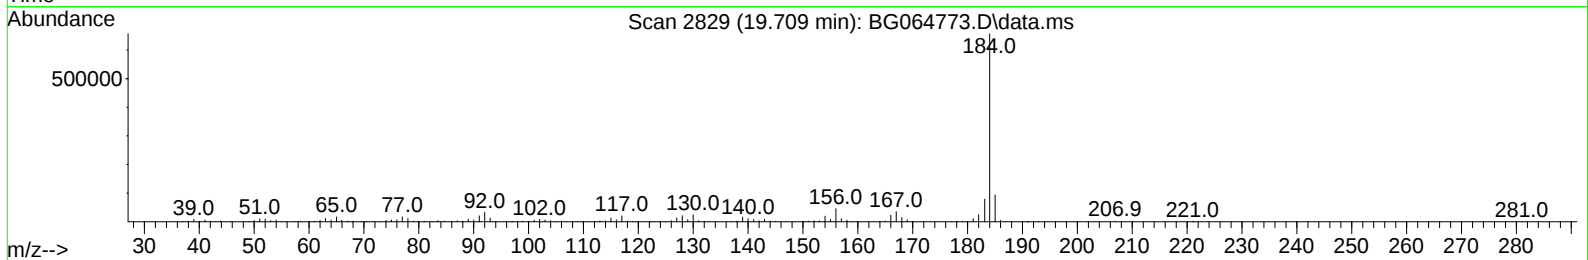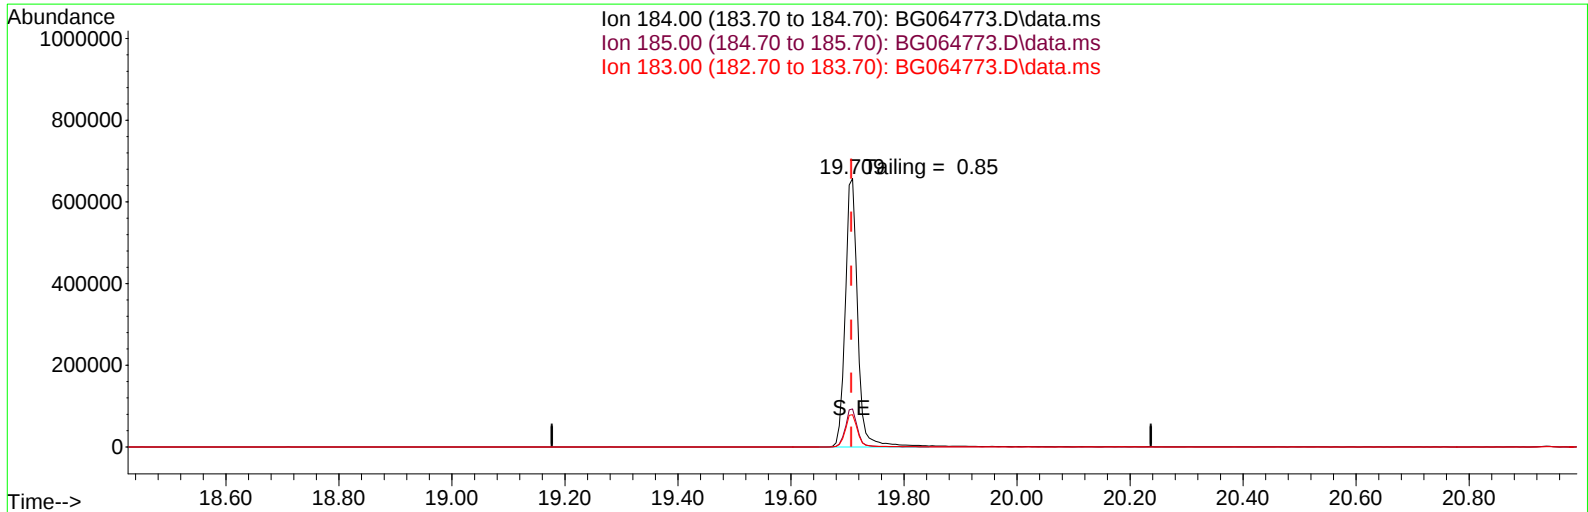

TIC: BG064773.D\data.ms

(77) Benzidine

19.709min (+ 0.002) 3494.74 ng m

response 1016582

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.19
183.00	12.20	12.01
0.00	0.00	0.00