
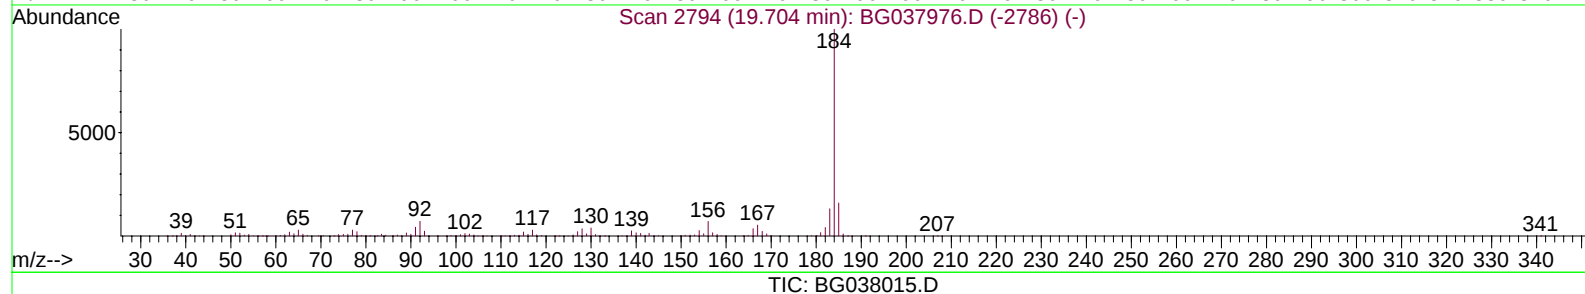
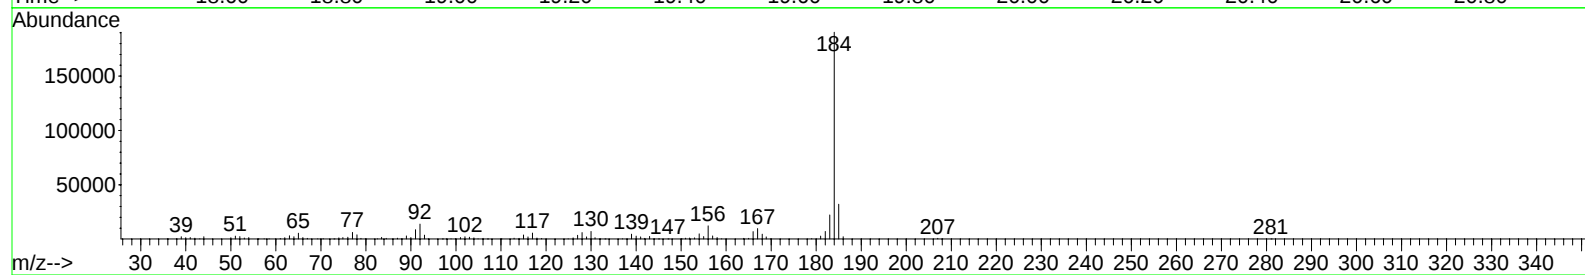


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG111518\
Data File : BG038015.D
Acq On : 15 Nov 2018 11:41
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 15 17:04:50 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG111318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 13 16:39:28 2018
Response via : Initial Calibration

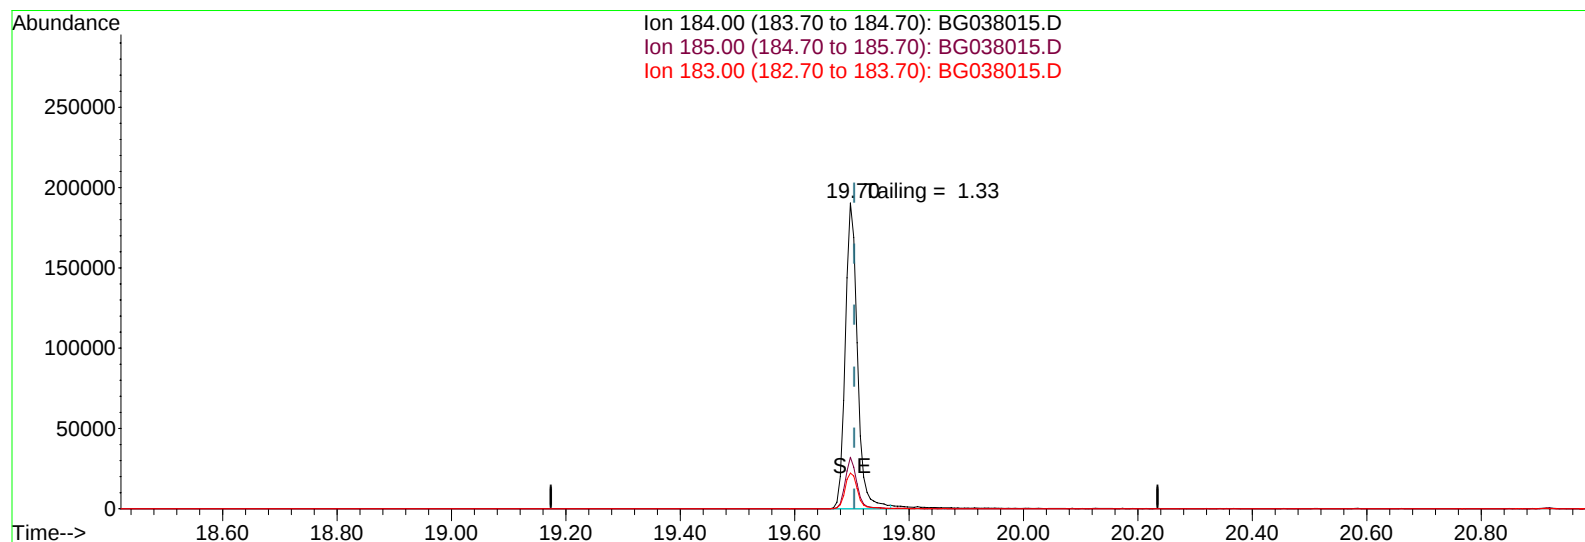

(77) Benzidine




19.697min (-0.007) 0.00ng

response 285053

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	16.84
183.00	12.70	11.66
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG111518\
Data File : BG038015.D
Acq On : 15 Nov 2018 11:41
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 15 17:04:50 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG111318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 13 16:39:28 2018
Response via : Initial Calibration

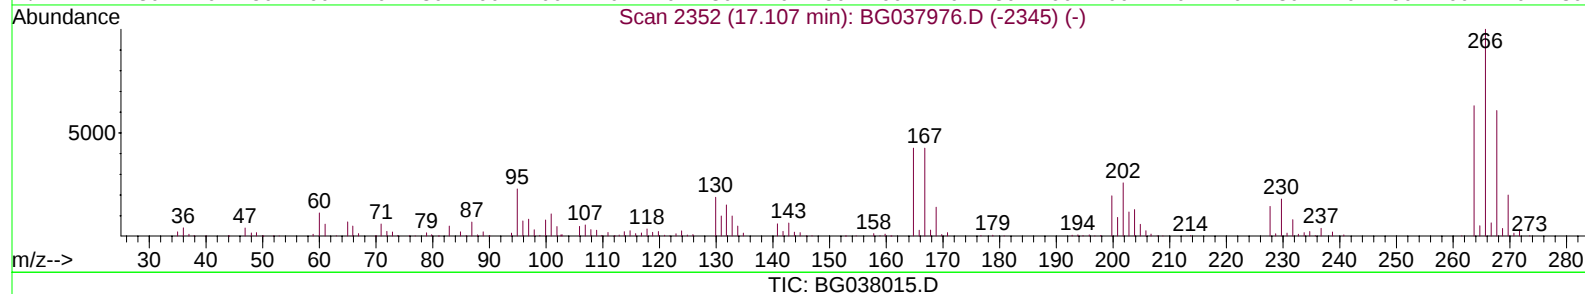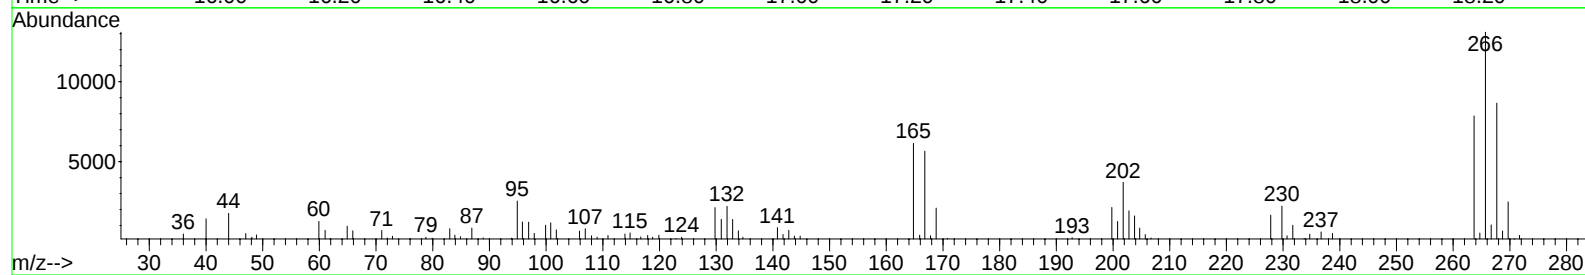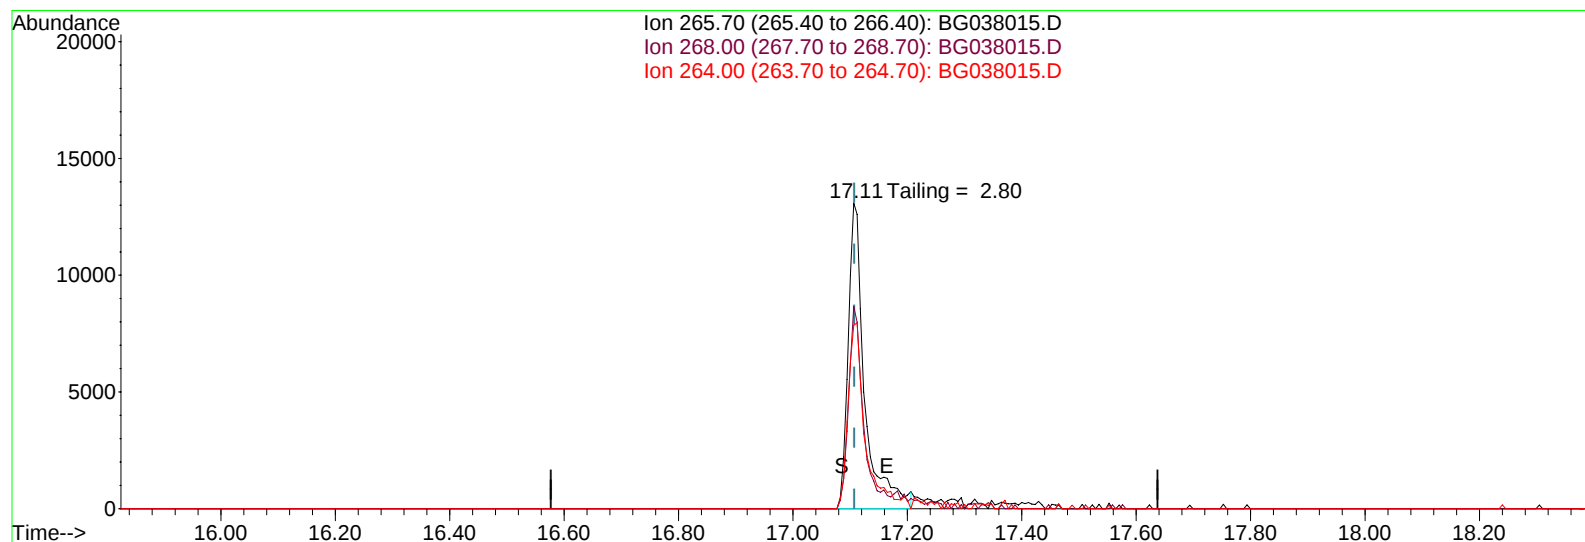

(70) Pentachlorophenol (C)

17.106min (-0.001) 39419.85ng

response 26085

Ion	Exp%	Act%
265.70	100	100
268.00	68.80	71.24
264.00	73.60	64.05
0.00	0.00	0.00