


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG111518\
Data File : BG038015.D
Acq On : 15 Nov 2018 11:41
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG111318.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Nov 13 16:39:28 2018

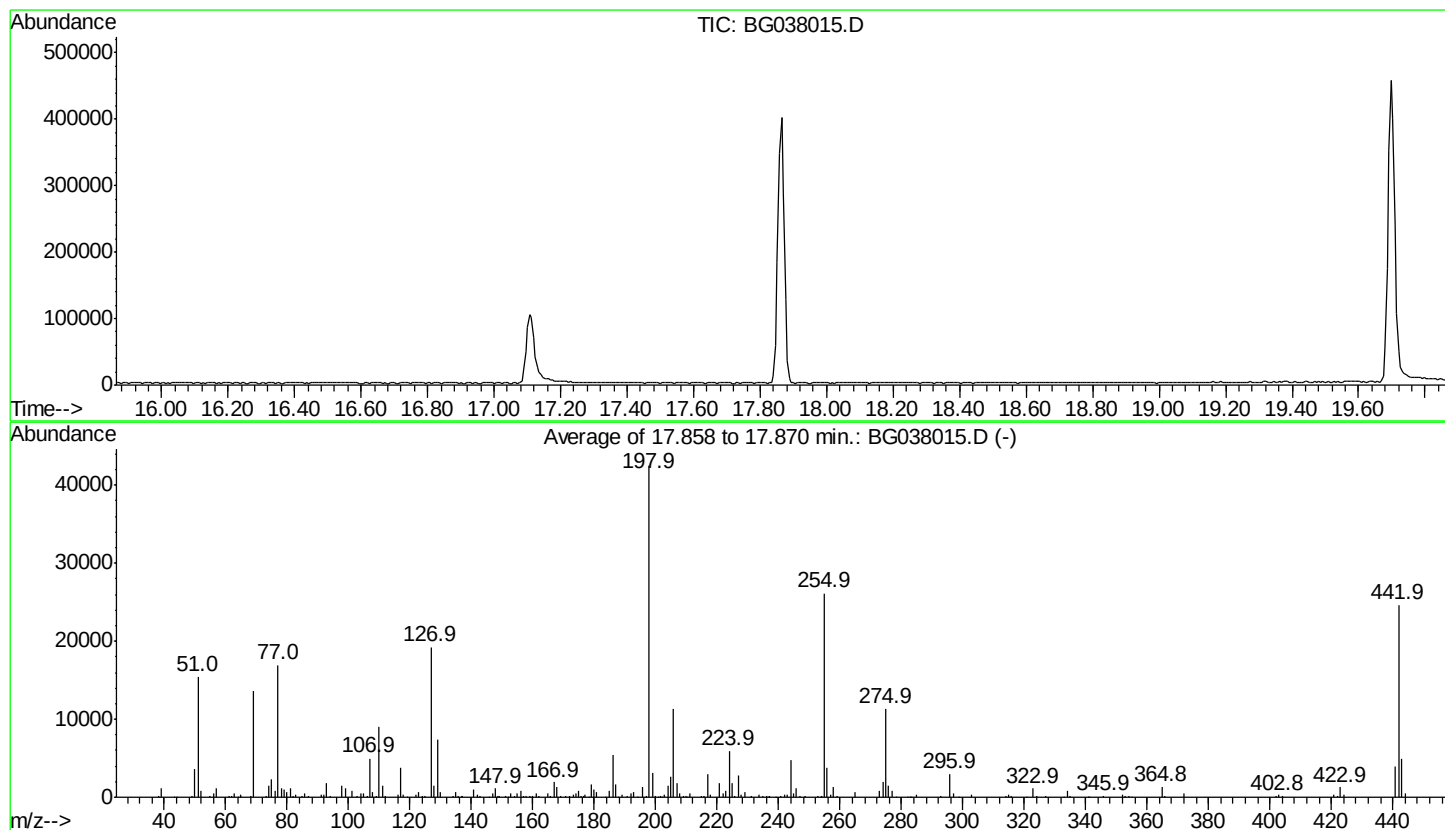

AutoFind: Scans 2480, 2481, 2482; Background Corrected with Scan 2473

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.3	15427	PASS
68	69	0.00	2	1.1	147	PASS
69	198	0.00	100	32.0	13602	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	45.2	19219	PASS
197	198	0.00	2	0.3	138	PASS
198	198	100	100	100.0	42509	PASS
199	198	5	9	7.2	3077	PASS
275	198	10	60	26.7	11334	PASS
365	198	1	100	3.2	1342	PASS
441	198	0.01	100	9.2	3932	PASS
442	198	50	100	57.9	24621	PASS
443	442	15	24	19.8	4873	PASS