
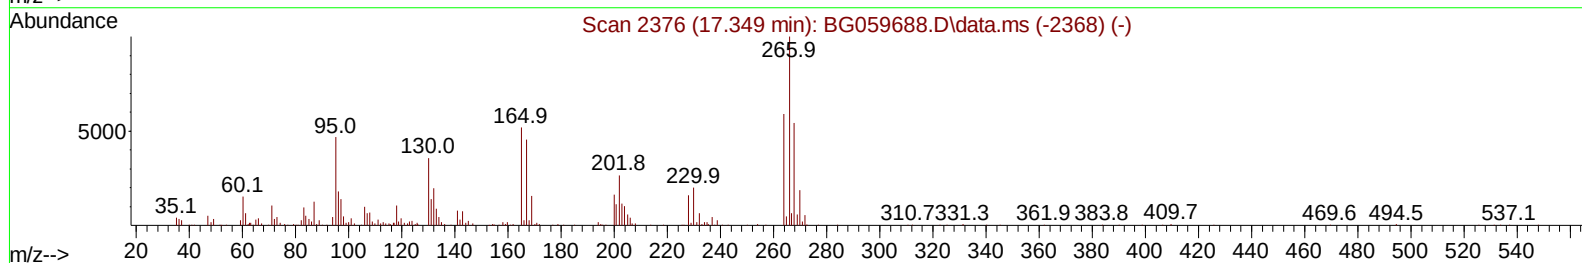
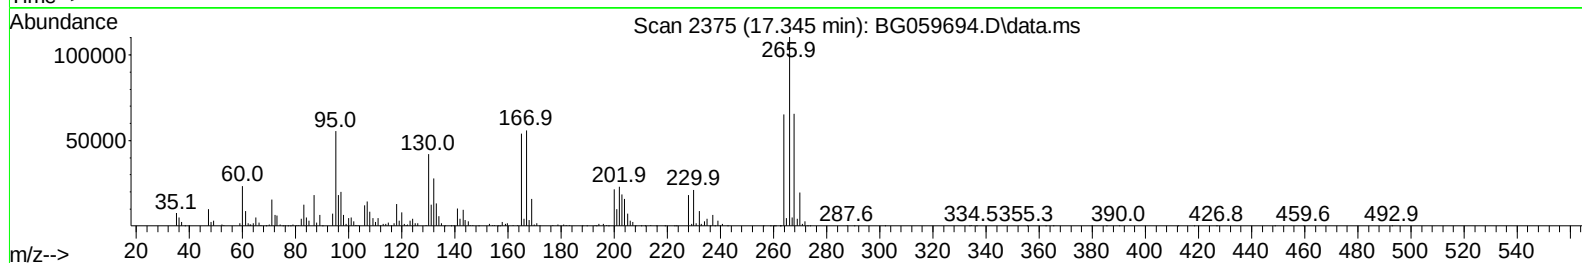


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111523\
Data File : BG059694.D
Acq On : 15 Nov 2023 10:26
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 15 18:47:57 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111423.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 15 08:14:53 2023
Response via : Initial Calibration

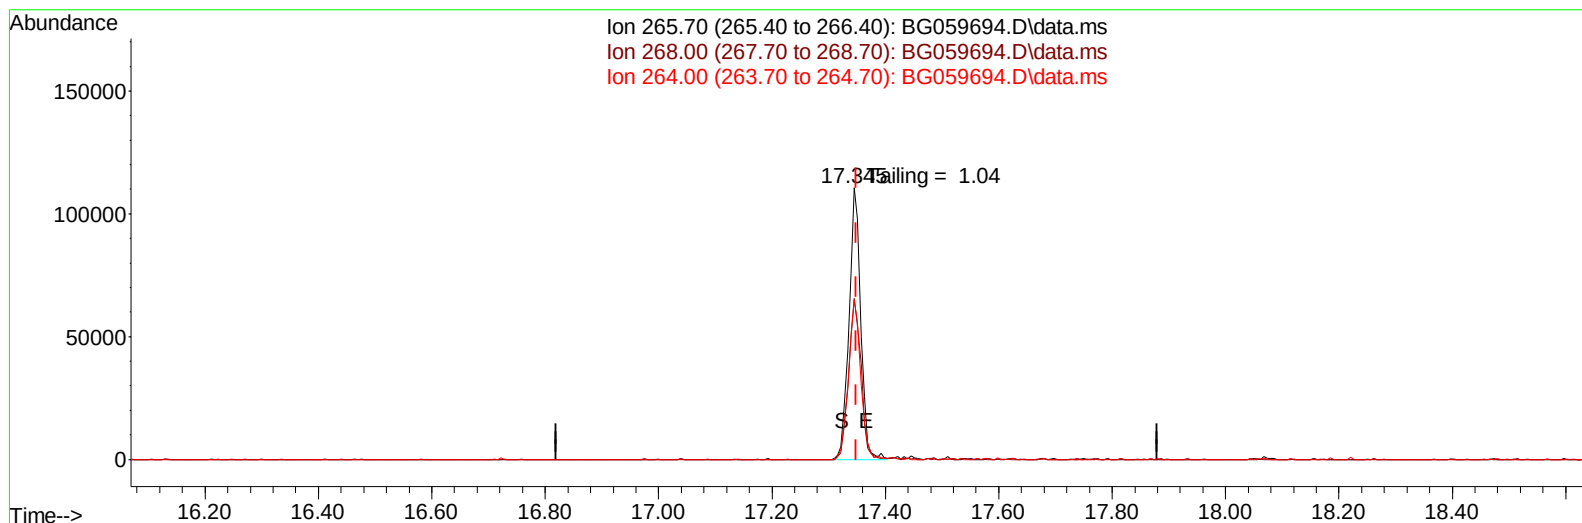

TIC: BG059694.D\data.ms

(70) Pentachlorophenol (C)




17.345min (-0.004) 316893.95 ng

response 157577

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	54.30	59.39
264.00	59.10	58.89
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111523\
 Data File : BG059694.D
 Acq On : 15 Nov 2023 10:26
 Operator : MA/JU
 Sample : DFTTP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 15 18:47:57 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111423.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 15 08:14:53 2023
 Response via : Initial Calibration

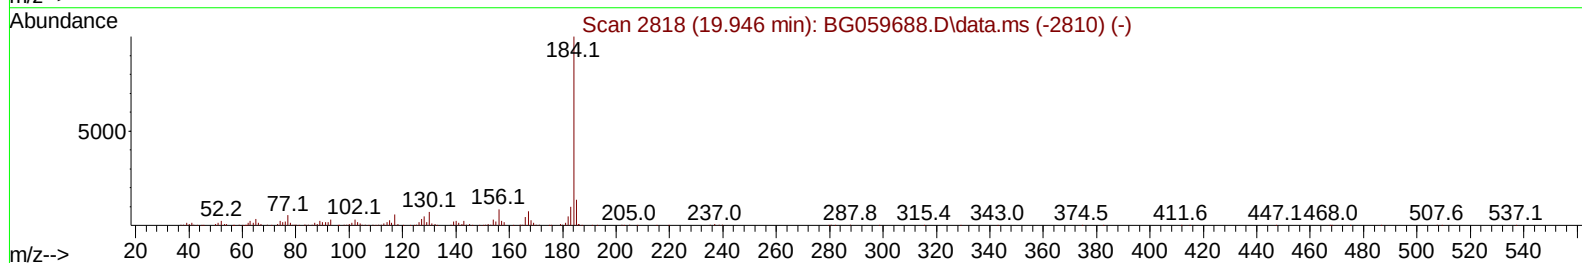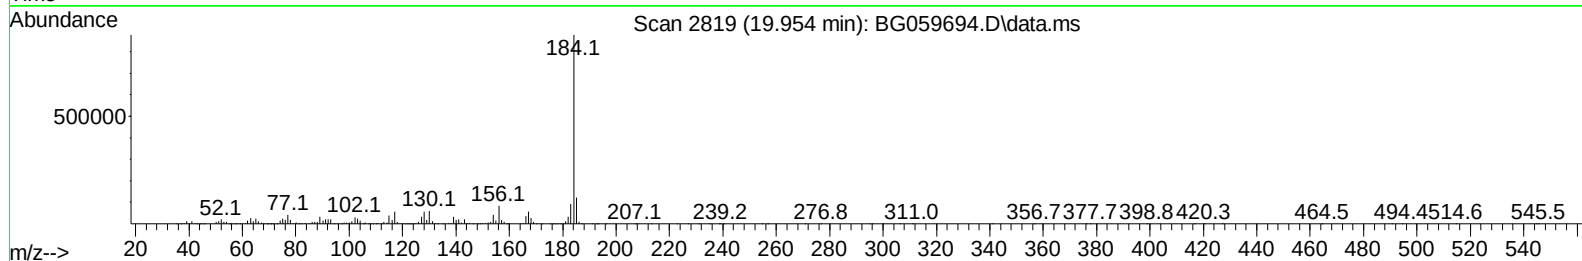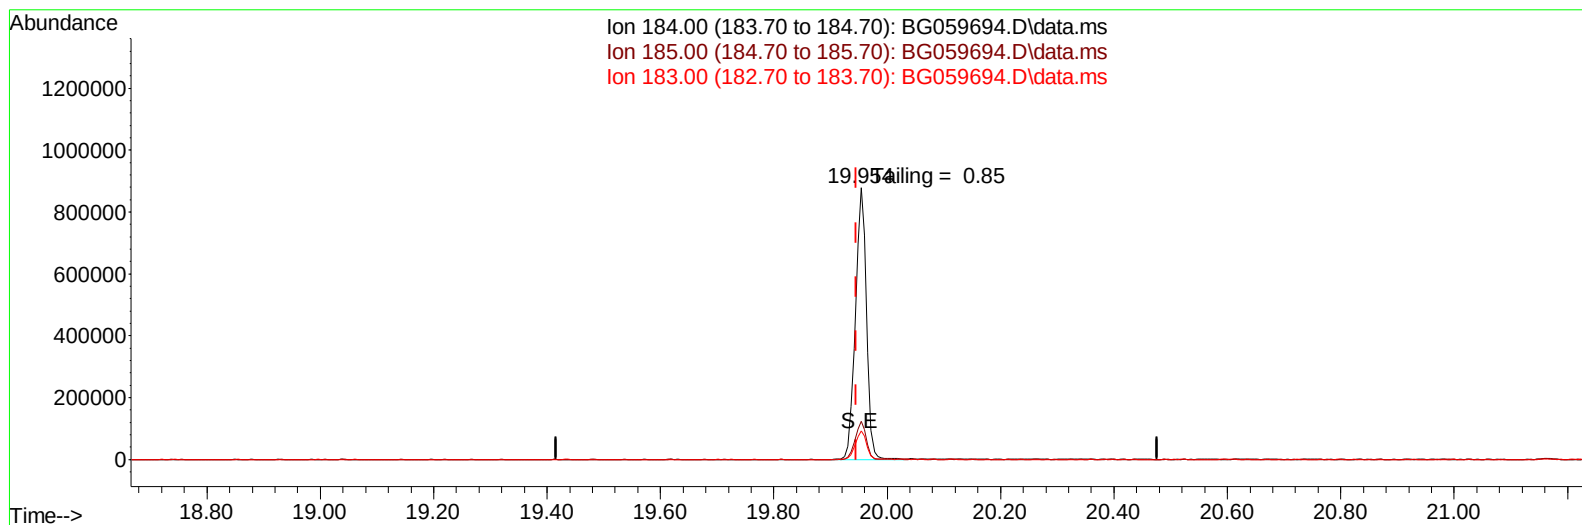

TIC: BG059694.D\data.ms

(77) Benzidine**19.954min (+ 0.008) 1103413.50 ng****response 1193242**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	14.07
183.00	9.70	10.49
0.00	0.00	0.00