


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111523\
Data File : BG059694.D
Acq On : 15 Nov 2023 10:26
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111423.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Nov 15 08:14:53 2023

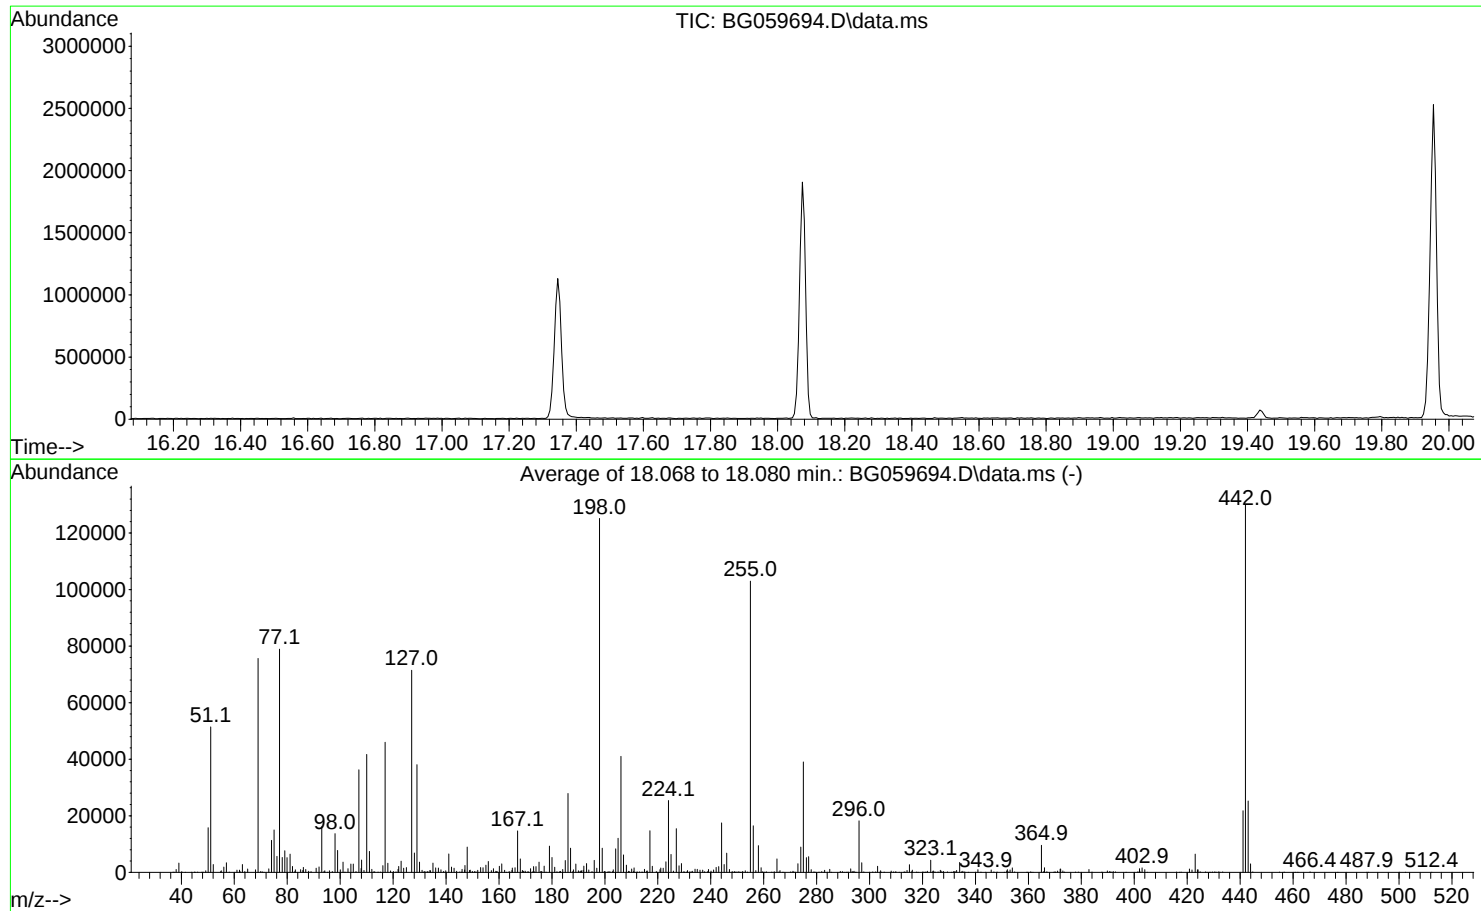




AutoFind: Scans 2498, 2499, 2500; Background Corrected with Scan 2491

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.1	51461	PASS
68	69	0.00	2	1.2	927	PASS
69	198	0.00	100	60.5	75648	PASS
70	69	0.00	2	0.5	348	PASS
127	198	10	80	57.1	71456	PASS
197	198	0.00	2	1.2	1471	PASS
198	198	100	100	100.0	125128	PASS
199	198	5	9	6.9	8573	PASS
275	198	10	60	31.2	39064	PASS
365	198	1	100	7.7	9574	PASS
441	198	0.01	100	17.4	21789	PASS
442	442	50	100	100.0	130072	PASS
443	442	15	24	19.4	25240	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111523\
Data File : BG059694.D
Acq On : 15 Nov 2023 10:26
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Nov 15 18:47:57 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111423.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 15 08:14:53 2023
Response via : Initial Calibration

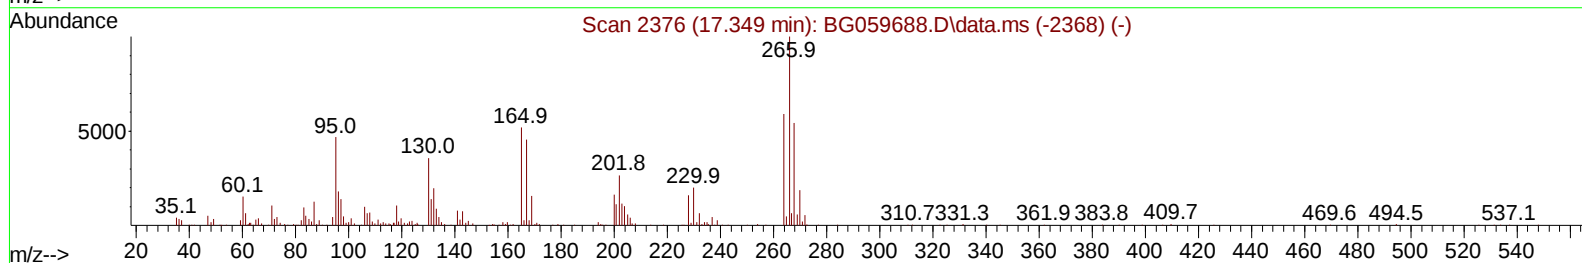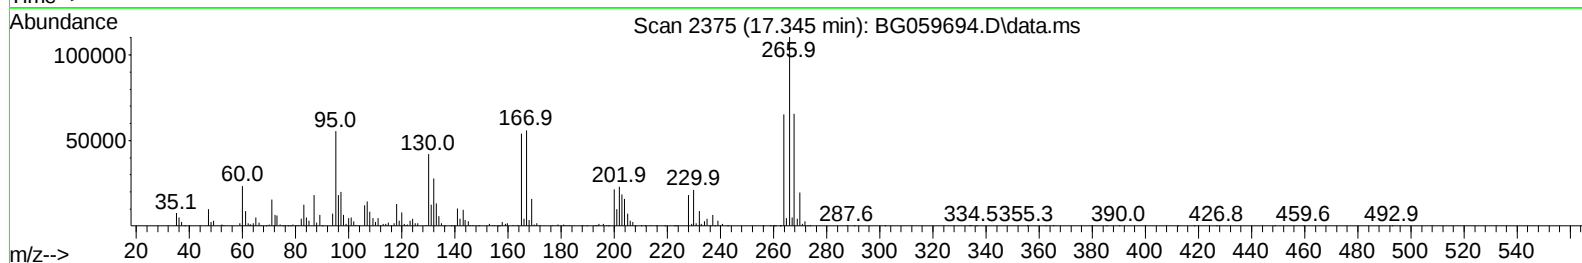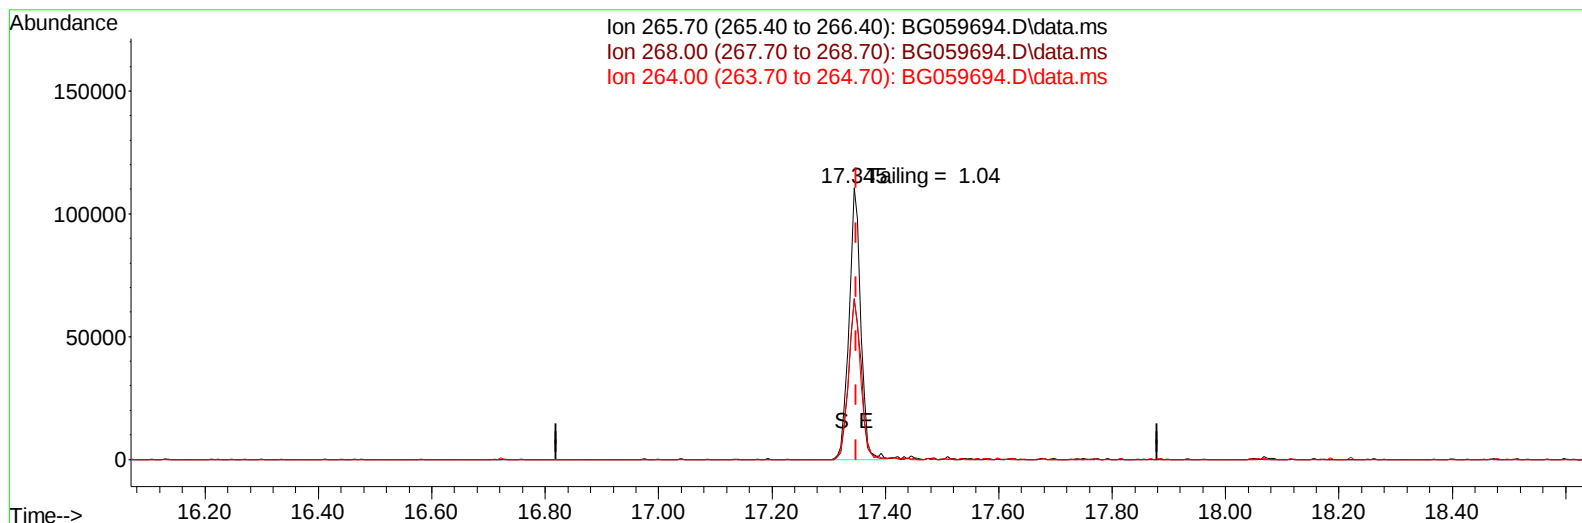

TIC: BG059694.D\data.ms

(70) Pentachlorophenol (C)

17.345min (-0.004) 316893.95 ng




response 157577

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	54.30	59.39
264.00	59.10	58.89
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111523\
Data File : BG059694.D
Acq On : 15 Nov 2023 10:26
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Nov 15 18:47:57 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111423.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 15 08:14:53 2023
Response via : Initial Calibration

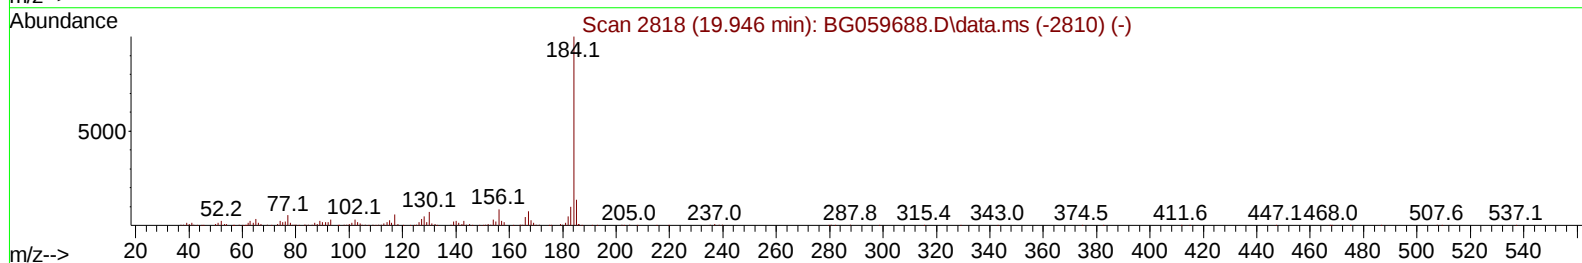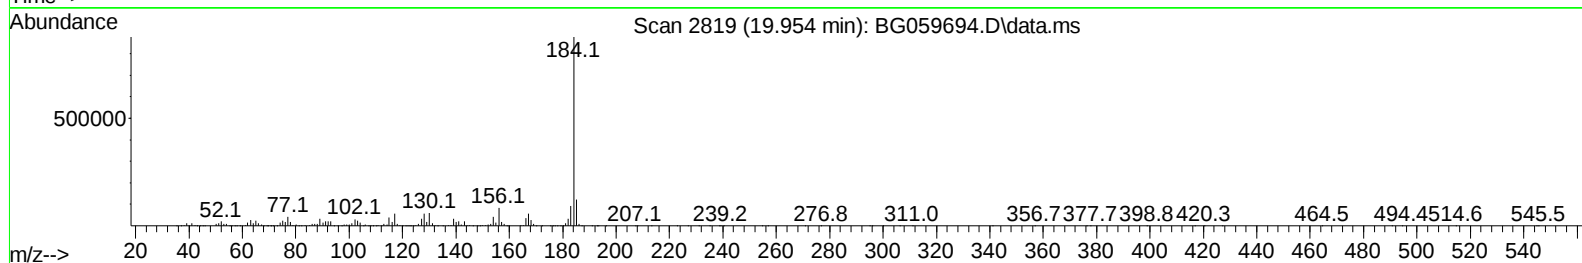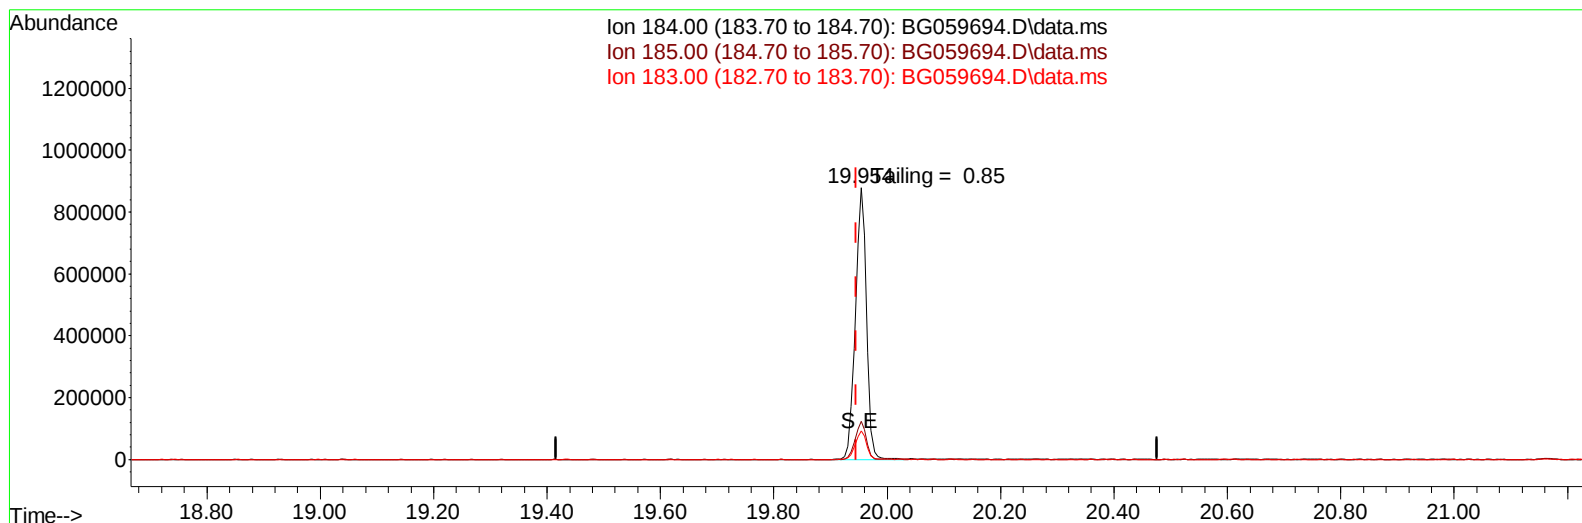

TIC: BG059694.D\data.ms

(77) Benzidine

19.954min (+ 0.008) 1103413.50 ng

response 1193242

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	14.07
183.00	9.70	10.49
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/15/2023	BNA_G	<u>BG059694.D</u>
Compound Name	Response	Retention Time
DDT	568648	21.164
DDD	15027	20.7
DDE	0	20.146
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
15027	583675	2.57

Instrument :
BNA_G
ClientSampleId :
DFTPP