

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111524\
 Data File : BG063420.D
 Acq On : 15 Nov 2024 11:18
 Operator : RC/JU
 Sample : PB164957BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK957

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG063420.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.301	32	36	42	rBV4	33106	50208	1.26%	0.137%
2	3.706	101	105	114	rBV	353584	566660	14.19%	1.548%
3	4.047	160	163	167	rVB4	8362	12135	0.30%	0.033%
4	4.799	288	291	295	rBV4	4290	6575	0.16%	0.018%
5	5.745	448	452	455	rBV4	4335	5950	0.15%	0.016%
6	6.232	533	535	537	rBV3	5647	6058	0.15%	0.017%
7	7.008	659	667	678	rBV	423318	737038	18.46%	2.013%
8	7.161	685	693	703	rBV	299527	511444	12.81%	1.397%
9	7.366	722	728	743	rVB	430620	703831	17.63%	1.922%
10	7.772	796	797	800	rBV2	6374	5904	0.15%	0.016%
11	7.831	800	807	816	rVV	359947	617857	15.48%	1.687%
12	8.541	922	928	937	rBV	558678	955845	23.94%	2.611%
13	8.988	996	1004	1014	rBV	415016	729536	18.27%	1.992%
14	9.164	1029	1034	1042	rBV5	19325	49080	1.23%	0.134%
15	9.705	1119	1126	1136	rBV	384715	695430	17.42%	1.899%
16	10.251	1212	1219	1227	rBV	583869	1049761	26.30%	2.867%
17	10.469	1254	1256	1259	rBV4	4545	6407	0.16%	0.017%
18	10.621	1274	1282	1289	rBV	521312	895334	22.43%	2.445%
19	10.757	1298	1305	1314	rBV	517125	956174	23.95%	2.611%
20	11.767	1474	1477	1480	rBV3	5381	5746	0.14%	0.016%
21	12.225	1548	1555	1560	rBV3	10755	24995	0.63%	0.068%
22	12.513	1602	1604	1608	rBV	4707	6190	0.16%	0.017%
23	12.742	1640	1643	1645	rBV2	4889	6412	0.16%	0.018%
24	13.876	1829	1836	1845	rBV	1241582	1729518	43.32%	4.724%
25	14.164	1878	1885	1894	rBV	1282095	1994844	49.97%	5.448%
26	14.352	1915	1917	1922	rVB3	4400	6613	0.17%	0.018%
27	14.470	1930	1937	1947	rBV	1011106	1521568	38.11%	4.156%
28	14.546	1947	1950	1954	rBV4	5869	8937	0.22%	0.024%
29	14.687	1965	1974	1985	rBV	410116	784265	19.64%	2.142%
30	14.881	2005	2007	2012	rBV5	5743	6858	0.17%	0.019%
31	15.040	2032	2034	2037	rVB3	5848	6889	0.17%	0.019%
32	15.469	2100	2107	2114	rBV	1801429	2635490	66.02%	7.198%
33	15.592	2121	2128	2139	rBV	552274	852402	21.35%	2.328%
34	15.704	2144	2147	2148	rBV3	11782	9383	0.24%	0.026%
35	15.786	2160	2161	2165	rVB4	6436	5954	0.15%	0.016%
36	16.238	2236	2238	2243	rBV5	9545	16212	0.41%	0.044%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111524\
 Data File : BG063420.D
 Acq On : 15 Nov 2024 11:18
 Operator : RC/JU
 Sample : PB164957BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK957

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
 Title : SVOA CALIBRATION

37	16.438	2271	2272	2277	rVB4	7610	6311	0.16%	0.017%
38	16.755	2324	2326	2329	rVB5	6713	7696	0.19%	0.021%
39	16.902	2349	2351	2355	rVB4	7634	8760	0.22%	0.024%
40	17.014	2367	2370	2373	rVB5	4943	6735	0.17%	0.018%
41	17.225	2399	2406	2412	rBV	1419727	2102479	52.66%	5.742%
42	17.319	2416	2422	2431	rVV2	2069878	3177809	79.60%	8.679%
43	17.596	2466	2469	2471	rBV3	7005	7604	0.19%	0.021%
44	18.113	2555	2557	2558	rBV2	6870	5814	0.15%	0.016%
45	18.318	2590	2592	2596	rVB5	7595	7402	0.19%	0.020%
46	18.547	2627	2631	2632	rBV4	7146	7166	0.18%	0.020%
47	18.741	2662	2664	2667	rBV3	8329	10073	0.25%	0.028%
48	19.182	2736	2739	2745	rVB3	38073	54834	1.37%	0.150%
49	19.258	2748	2752	2755	rBV2	28736	39317	0.98%	0.107%
50	19.623	2808	2814	2821	rBV	2859929	3992188	100.00%	10.903%
51	19.816	2845	2847	2848	rBV2	10764	7844	0.20%	0.021%
52	21.479	3124	3130	3138	rBV	1597401	2458112	61.57%	6.714%
53	24.311	3602	3612	3625	rVB	1504637	3873254	97.02%	10.579%
54	24.517	3638	3647	3662	rVB	1015633	2657440	66.57%	7.258%




Sum of corrected areas: 36614341

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111524\
Data File : BG063420.D
Acq On : 15 Nov 2024 11:18
Operator : RC/JU
Sample : PB164957BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK957

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

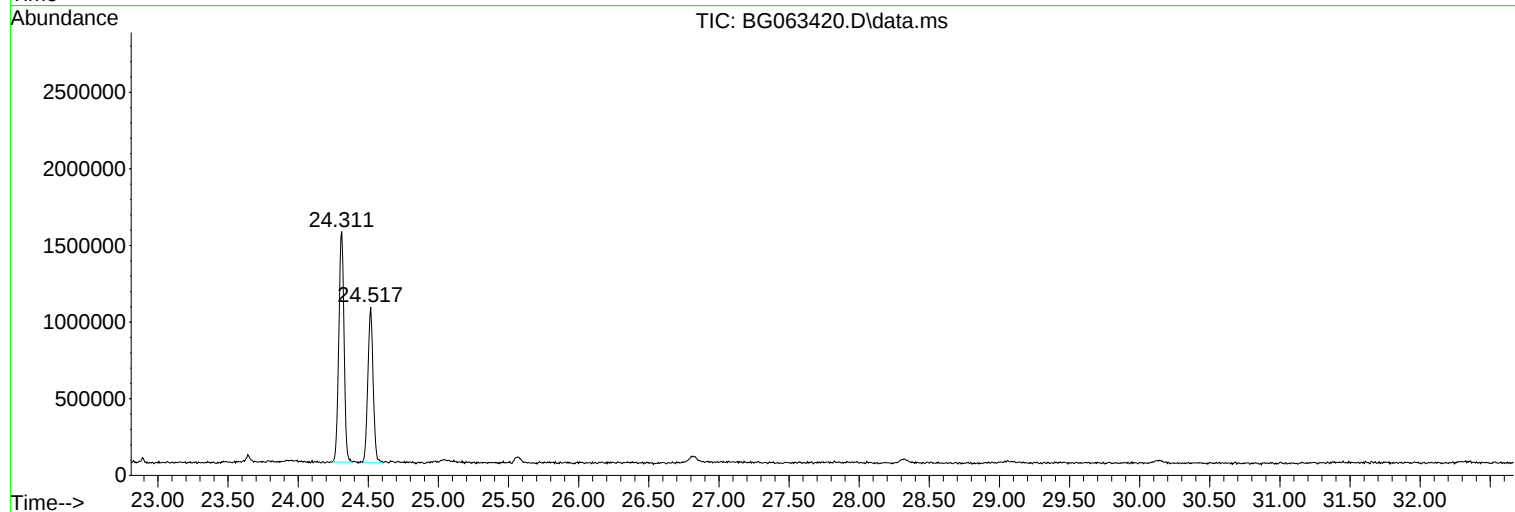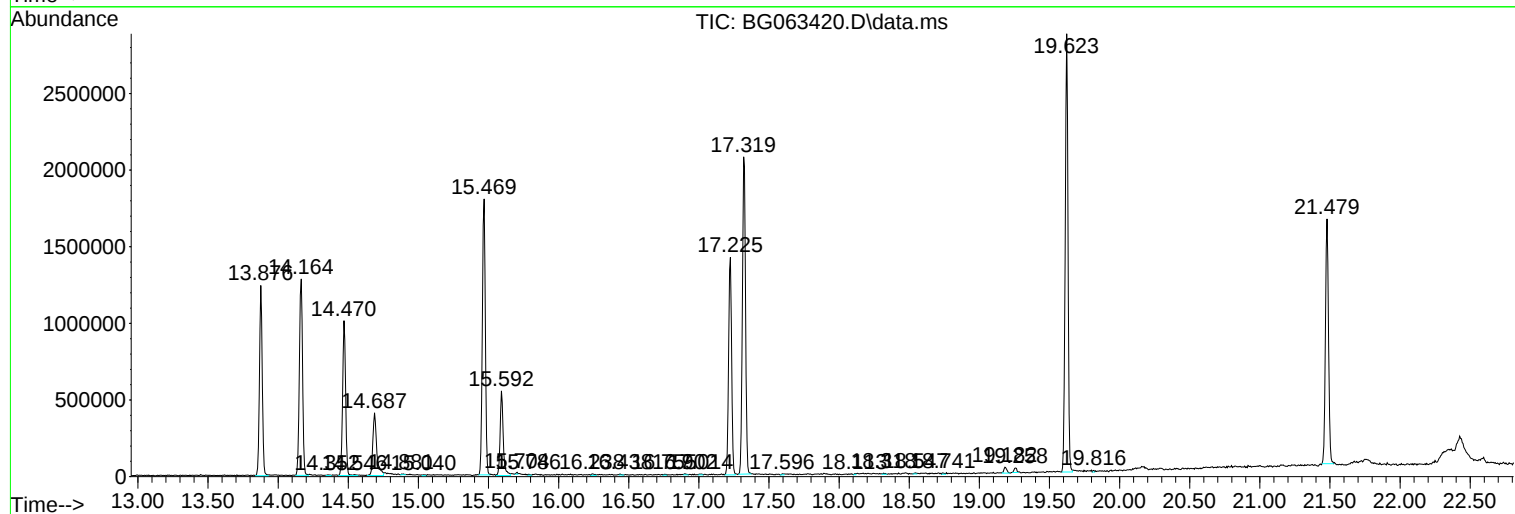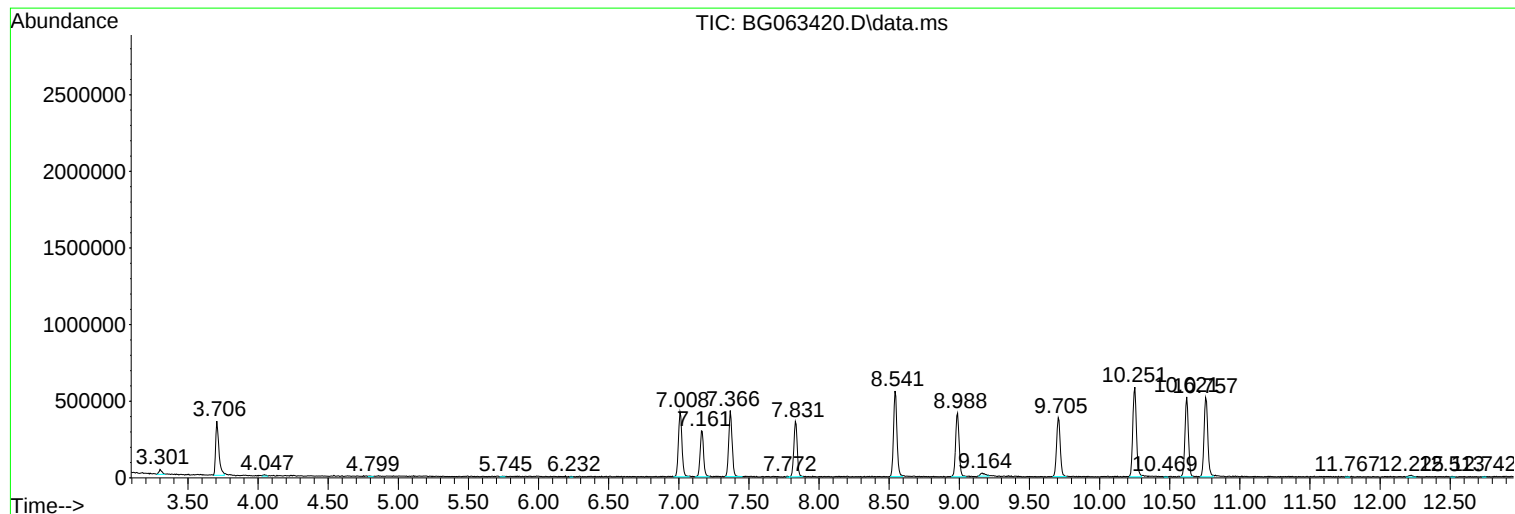

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111524\
Data File : BG063420.D
Acq On : 15 Nov 2024 11:18
Operator : RC/JU
Sample : PB164957BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK957

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111524\
Data File : BG063420.D
Acq On : 15 Nov 2024 11:18
Operator : RC/JU
Sample : PB164957BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK957

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc