

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111524\
 Data File : BG063425.D
 Acq On : 15 Nov 2024 14:28
 Operator : RC/JU
 Sample : P4784-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 E27L5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG063425.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.305	33	37	44	rVB4	26982	39488	0.95%	0.113%
2	3.710	102	106	119	rVB	107491	186813	4.50%	0.533%
3	4.045	160	163	167	rVB4	10271	10724	0.26%	0.031%
4	4.909	305	310	311	rBV4	4977	6885	0.17%	0.020%
5	5.649	432	436	441	rBV4	5688	12620	0.30%	0.036%
6	5.784	455	459	462	rBV4	4537	6801	0.16%	0.019%
7	6.842	634	639	640	rBV3	5521	6992	0.17%	0.020%
8	7.012	661	668	678	rVB	143098	253593	6.11%	0.724%
9	7.165	688	694	703	rBV	309066	514029	12.38%	1.467%
10	7.371	723	729	737	rVB	368809	645049	15.54%	1.841%
11	7.829	800	807	817	rBV	334581	600977	14.47%	1.716%
12	8.164	861	864	869	rBV4	4862	9169	0.22%	0.026%
13	8.546	922	929	937	rBV	394752	702157	16.91%	2.004%
14	8.916	989	992	996	rBV4	4939	6964	0.17%	0.020%
15	8.986	996	1004	1014	rVV	430767	735751	17.72%	2.100%
16	9.221	1041	1044	1047	rBV3	5576	6394	0.15%	0.018%
17	9.709	1117	1127	1141	rBV	391786	718450	17.30%	2.051%
18	10.250	1212	1219	1229	rBV	587598	1061370	25.56%	3.030%
19	10.397	1242	1244	1245	rBV2	7244	7068	0.17%	0.020%
20	10.620	1272	1282	1291	rBV	490155	897509	21.62%	2.562%
21	10.761	1298	1306	1317	rBV	423199	808825	19.48%	2.309%
22	10.978	1340	1343	1350	rBV3	3697	6312	0.15%	0.018%
23	11.301	1396	1398	1403	rVB3	4321	7314	0.18%	0.021%
24	12.218	1550	1554	1557	rBV2	9281	12565	0.30%	0.036%
25	12.670	1629	1631	1635	rBV3	5530	7121	0.17%	0.020%
26	12.982	1679	1684	1690	rVB3	5081	13429	0.32%	0.038%
27	13.746	1809	1814	1816	rBV5	5267	6980	0.17%	0.020%
28	13.875	1830	1836	1849	rVB	1172491	1749890	42.15%	4.995%
29	14.163	1876	1885	1897	rVB	1266939	1959978	47.21%	5.595%
30	14.468	1930	1937	1945	rVB	934711	1474259	35.51%	4.208%
31	14.691	1969	1975	1983	rBV2	101163	215782	5.20%	0.616%
32	15.214	2061	2064	2068	rBV4	9651	12558	0.30%	0.036%
33	15.273	2071	2074	2075	rBV2	6950	6471	0.16%	0.018%
34	15.467	2100	2107	2117	rBV	1811526	2654674	63.94%	7.578%
35	15.538	2117	2119	2122	rVB3	6410	6704	0.16%	0.019%
36	15.590	2122	2128	2138	rBV	620499	952931	22.95%	2.720%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111524\
 Data File : BG063425.D
 Acq On : 15 Nov 2024 14:28
 Operator : RC/JU
 Sample : P4784-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 E27L5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
 Title : SVOA CALIBRATION

37	15.708	2141	2148	2151	rBV9	11446	22997	0.55%	0.066%
38	15.825	2163	2168	2169	rBV5	4870	6320	0.15%	0.018%
39	16.895	2349	2350	2352	rBV2	8164	6825	0.16%	0.019%
40	17.142	2388	2392	2397	rBV3	47834	61948	1.49%	0.177%
41	17.224	2399	2406	2413	rVV	1364052	2016573	48.57%	5.756%
42	17.324	2416	2423	2431	rVV	2135316	3251641	78.32%	9.282%
43	17.447	2442	2444	2447	rVB4	5393	5792	0.14%	0.017%
44	17.600	2464	2470	2471	rBV4	7526	13145	0.32%	0.038%
45	17.894	2516	2520	2521	rBV3	10302	12658	0.30%	0.036%
46	17.964	2530	2532	2533	rBV2	6791	6040	0.15%	0.017%
47	18.129	2558	2560	2564	rVB4	6675	8489	0.20%	0.024%
48	18.334	2593	2595	2598	rBV3	5028	5762	0.14%	0.016%
49	18.440	2607	2613	2614	rBV6	7378	11265	0.27%	0.032%
50	18.552	2626	2632	2637	rBV8	19820	31866	0.77%	0.091%
51	18.616	2640	2643	2647	rVB6	9741	11461	0.28%	0.033%
52	19.186	2735	2740	2743	rBV	35837	50538	1.22%	0.144%
53	19.257	2748	2752	2757	rBV3	36740	55117	1.33%	0.157%
54	19.310	2760	2761	2764	rBV3	8623	6439	0.16%	0.018%
55	19.621	2808	2814	2822	rBV	2981059	4151945	100.00%	11.852%
56	21.478	3123	3130	3139	rBV	1568027	2458367	59.21%	7.018%
57	24.310	3602	3612	3622	rVB	1584372	3973904	95.71%	11.344%
58	24.515	3638	3647	3659	rVB	945155	2537939	61.13%	7.245%




Sum of corrected areas: 35031627

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111524\
Data File : BG063425.D
Acq On : 15 Nov 2024 14:28
Operator : RC/JU
Sample : P4784-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
E27L5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

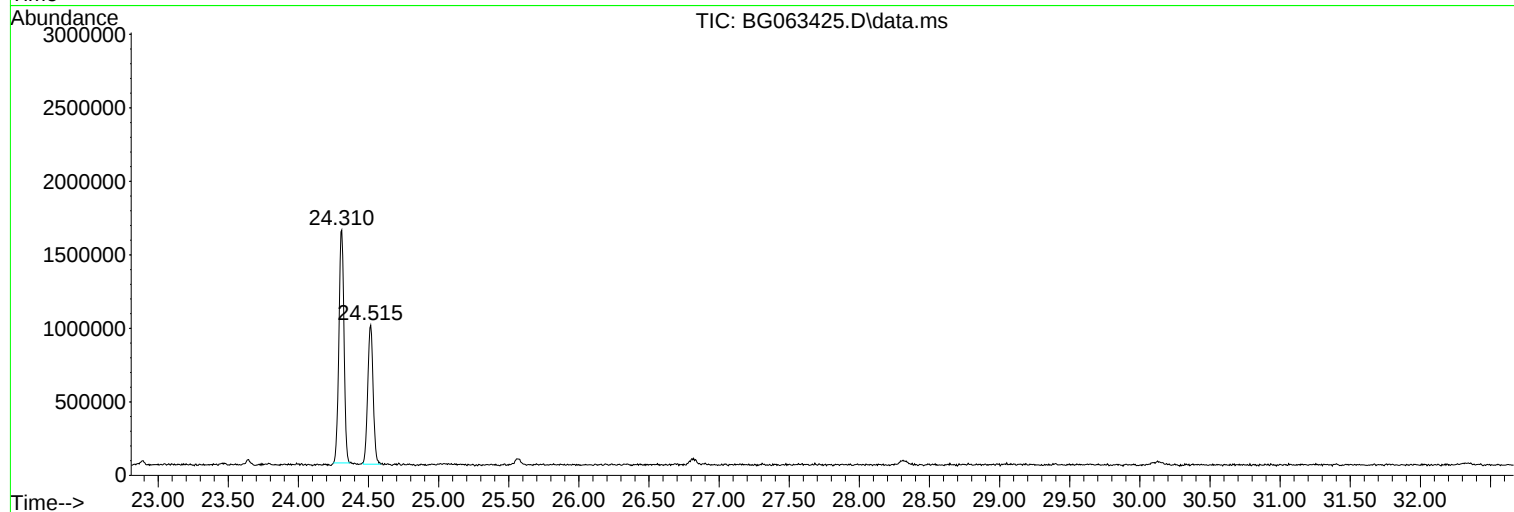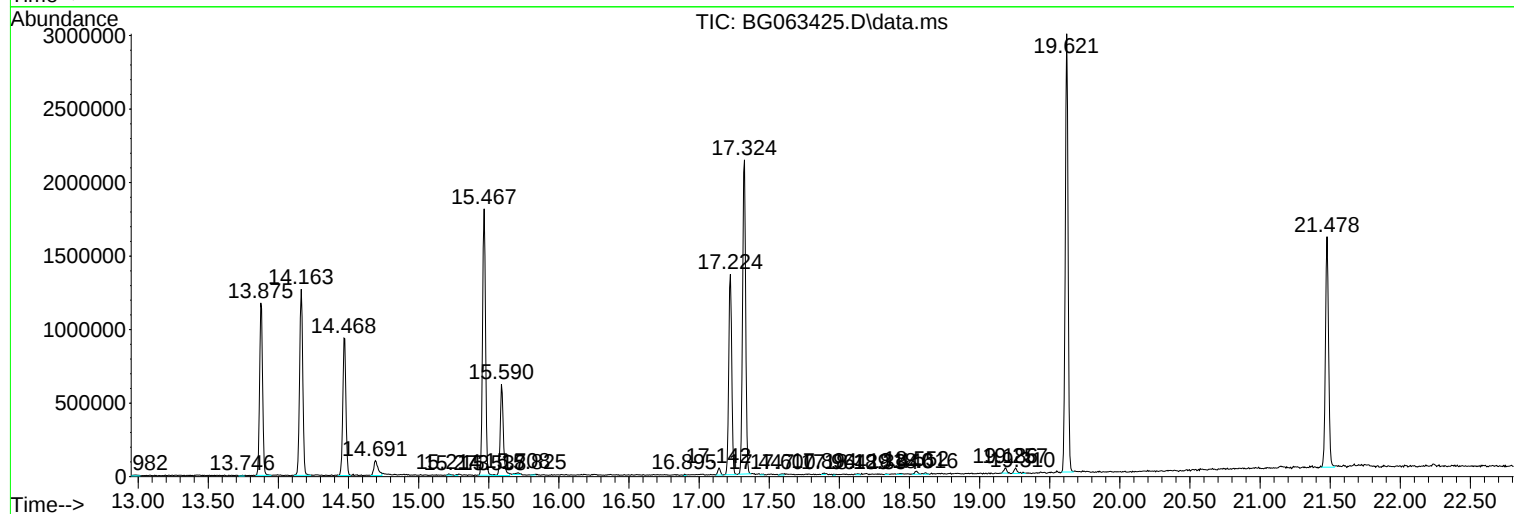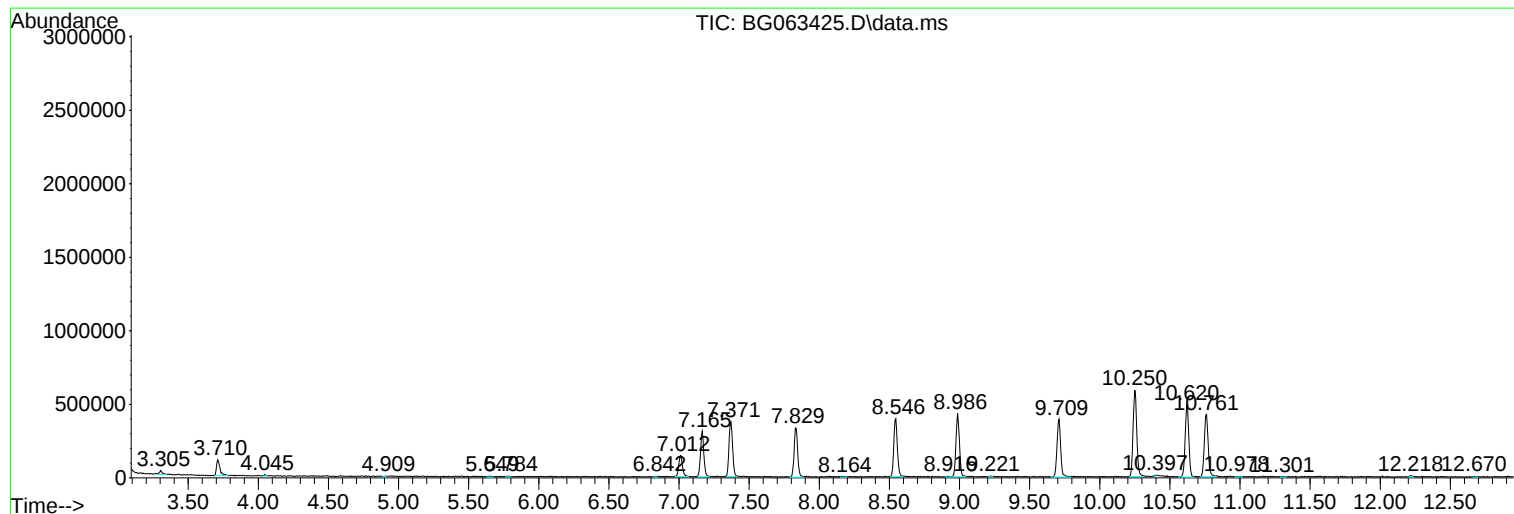

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111524\
Data File : BG063425.D
Acq On : 15 Nov 2024 14:28
Operator : RC/JU
Sample : P4784-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
E27L5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111524\
Data File : BG063425.D
Acq On : 15 Nov 2024 14:28
Operator : RC/JU
Sample : P4784-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
E27L5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc