

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111524\
 Data File : BG063452.D
 Acq On : 16 Nov 2024 10:14
 Operator : RC/JU
 Sample : PB164999BL
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK999

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG063452.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.302	33	36	40	rVB2	23396	30005	0.79%	0.089%
2	3.701	100	104	121	rBV	305359	527804	13.85%	1.562%
3	4.036	159	161	162	rBV2	8221	5968	0.16%	0.018%
4	6.263	538	540	543	rBV2	4608	5348	0.14%	0.016%
5	7.003	659	666	675	rBV	457111	770718	20.22%	2.280%
6	7.162	685	693	702	rBV	316048	544840	14.29%	1.612%
7	7.362	721	727	737	rBV	439612	733747	19.25%	2.171%
8	7.826	799	806	814	rBV	308663	516535	13.55%	1.528%
9	8.537	921	927	937	rBV2	538868	957324	25.11%	2.833%
10	8.736	960	961	965	rVB3	5526	5344	0.14%	0.016%
11	8.983	996	1003	1014	rBV	426268	748855	19.64%	2.216%
12	9.177	1030	1036	1046	rBV9	15185	48839	1.28%	0.145%
13	9.706	1118	1126	1134	rBV	396208	692188	18.16%	2.048%
14	9.964	1167	1170	1171	rBV2	7533	6804	0.18%	0.020%
15	10.246	1211	1218	1230	rBV	577656	1064032	27.91%	3.148%
16	10.617	1274	1281	1292	rVB	458085	804534	21.11%	2.381%
17	10.758	1298	1305	1315	rBV	524401	978546	25.67%	2.895%
18	11.028	1347	1351	1353	rBV2	4858	5977	0.16%	0.018%
19	11.369	1407	1409	1413	rVB	4867	6529	0.17%	0.019%
20	11.480	1425	1428	1431	rBV2	5169	5732	0.15%	0.017%
21	12.215	1547	1553	1559	rBV3	8554	16914	0.44%	0.050%
22	12.362	1575	1578	1581	rBV	4598	7070	0.19%	0.021%
23	13.789	1819	1821	1825	rBV	3778	5542	0.15%	0.016%
24	13.877	1829	1836	1848	rVV	1133301	1628635	42.72%	4.819%
25	14.165	1875	1885	1895	rBV	1223000	1911078	50.13%	5.655%
26	14.471	1931	1937	1944	rBV	808817	1236527	32.44%	3.659%
27	14.688	1967	1974	1987	rBV	347433	670741	17.60%	1.985%
28	15.017	2025	2030	2033	rBV2	4026	5948	0.16%	0.018%
29	15.470	2100	2107	2115	rBV	1651725	2516859	66.02%	7.447%
30	15.593	2122	2128	2142	rBV	454714	732788	19.22%	2.168%
31	15.711	2144	2148	2152	rVB5	12581	18198	0.48%	0.054%
32	16.704	2316	2317	2323	rVB2	5389	5935	0.16%	0.018%
33	16.839	2338	2340	2345	rVB4	5710	8249	0.22%	0.024%
34	16.892	2345	2349	2350	rBV2	5160	6832	0.18%	0.020%
35	16.903	2350	2351	2355	rVB4	7130	5985	0.16%	0.018%
36	17.226	2399	2406	2415	rBV	1139061	1707156	44.78%	5.051%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111524\
Data File : BG063452.D
Acq On : 16 Nov 2024 10:14
Operator : RC/JU
Sample : PB164999BL
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK999

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Title : SVOA CALIBRATION

37	17.326	2416	2423	2435	rVB2	1990965	3033590	79.58%	8.976%
38	17.620	2469	2473	2475	rVB4	4308	5412	0.14%	0.016%
39	17.896	2518	2520	2522	rBV3	9340	9627	0.25%	0.028%
40	19.124	2727	2729	2732	rVB3	7546	6948	0.18%	0.021%
41	19.189	2735	2740	2744	rBV5	31916	53572	1.41%	0.159%
42	19.259	2748	2752	2759	rVB2	28260	46548	1.22%	0.138%
43	19.624	2808	2814	2821	rBV	2690050	3811995	100.00%	11.279%
44	20.158	2903	2905	2909	rBV4	9030	10263	0.27%	0.030%
45	21.480	3124	3130	3137	rBV	1318707	2060393	54.05%	6.096%
46	24.312	3602	3612	3625	rBV2	1408798	3720178	97.59%	11.008%
47	24.524	3638	3648	3659	rBV	791846	2094038	54.93%	6.196%




Sum of corrected areas: 33796690

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111524\
Data File : BG063452.D
Acq On : 16 Nov 2024 10:14
Operator : RC/JU
Sample : PB164999BL
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK999

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

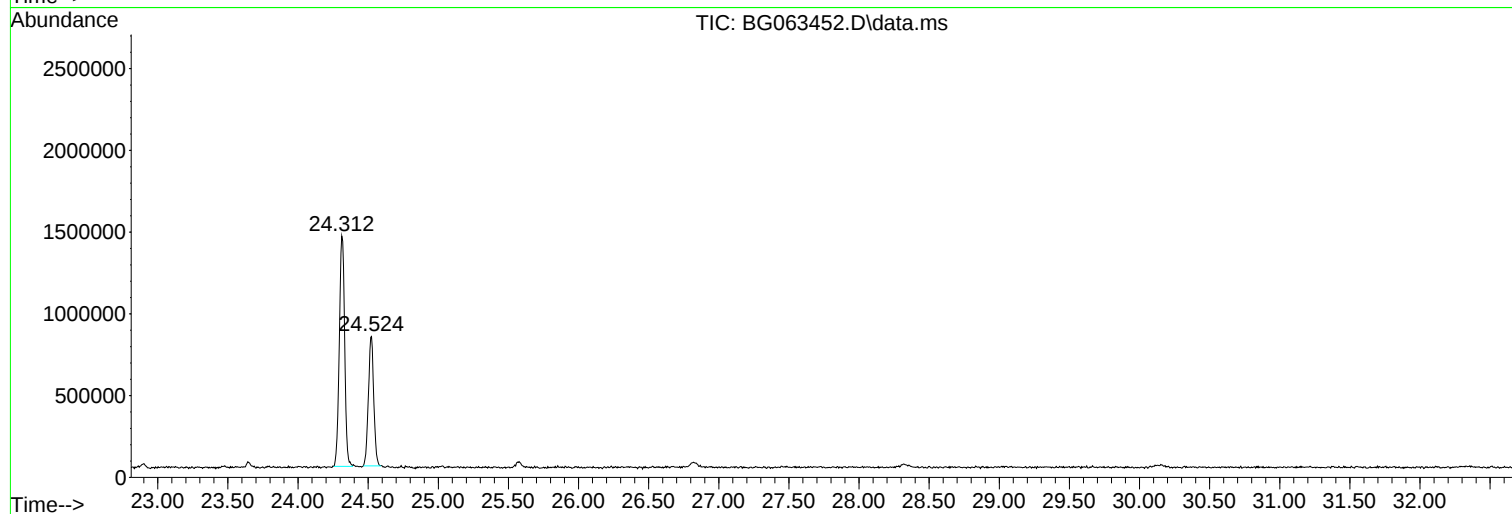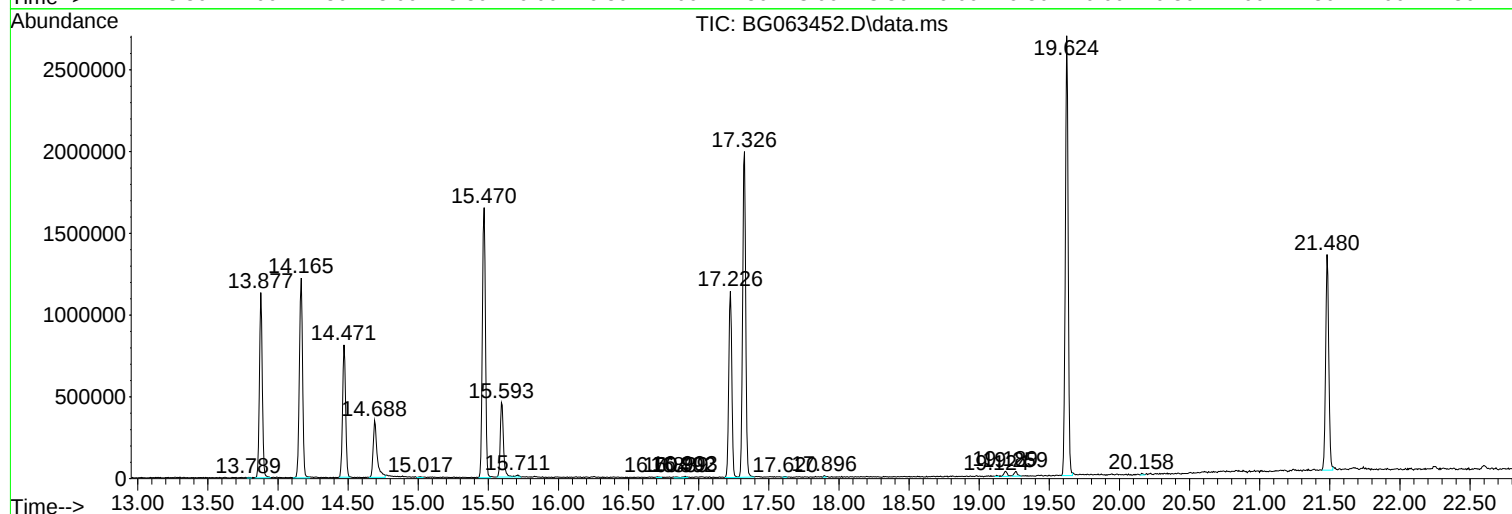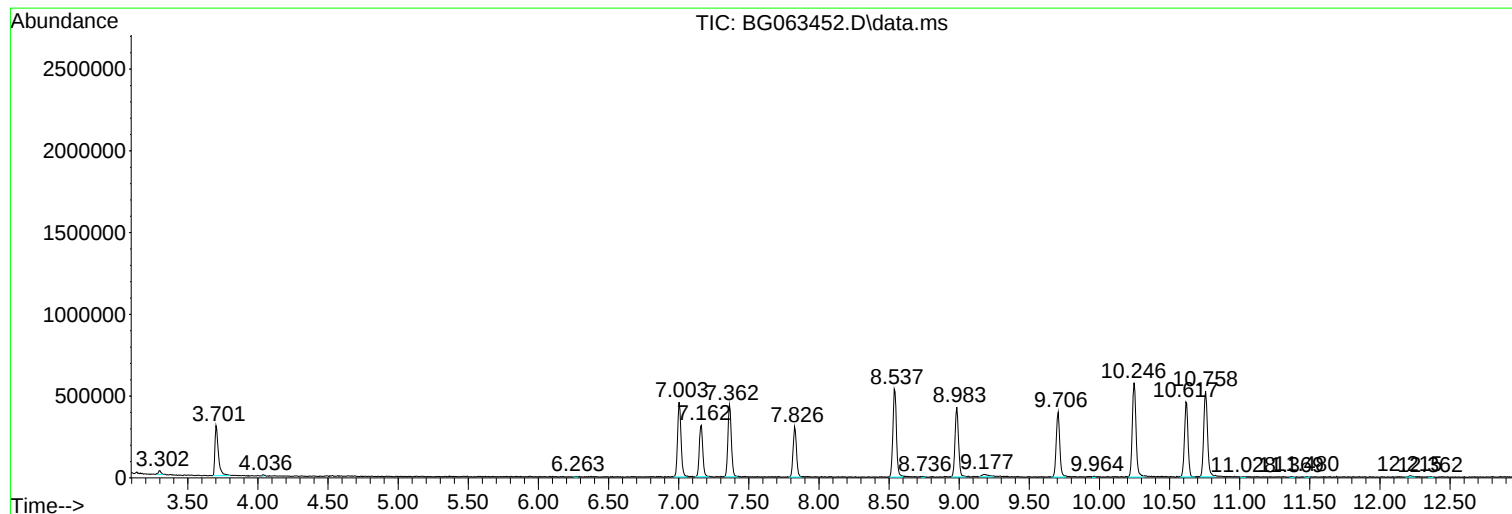

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111524\
Data File : BG063452.D
Acq On : 16 Nov 2024 10:14
Operator : RC/JU
Sample : PB164999BL
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK999

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111524\
Data File : BG063452.D
Acq On : 16 Nov 2024 10:14
Operator : RC/JU
Sample : PB164999BL
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK999

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc