

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111524\
 Data File : BG063473.D
 Acq On : 16 Nov 2024 23:32
 Operator : RC/JU
 Sample : PB165035BL
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK035

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG063473.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.300	33	36	44	rVB3	35145	53731	1.23%	0.136%
2	3.652	94	96	101	rBV6	5347	7144	0.16%	0.018%
3	3.705	101	105	121	rBV	411234	694659	15.89%	1.761%
4	4.034	159	161	163	rBV2	6122	5974	0.14%	0.015%
5	4.710	273	276	280	rBV3	4802	6771	0.15%	0.017%
6	6.860	638	642	644	rBV4	4372	5983	0.14%	0.015%
7	7.007	659	667	679	rBV	504505	884402	20.23%	2.242%
8	7.160	687	693	704	rBV	358313	598003	13.68%	1.516%
9	7.366	721	728	738	rVB	491049	828568	18.95%	2.100%
10	7.830	800	807	816	rVB	344294	583930	13.36%	1.480%
11	8.541	921	928	939	rBV	650546	1137654	26.02%	2.883%
12	8.987	993	1004	1015	rBV	466073	860801	19.69%	2.182%
13	9.199	1034	1040	1044	rBV7	14058	34294	0.78%	0.087%
14	9.704	1119	1126	1136	rBV	455547	818655	18.72%	2.075%
15	10.174	1203	1206	1209	rVB3	5564	6921	0.16%	0.018%
16	10.251	1212	1219	1230	rBV	657393	1231347	28.16%	3.121%
17	10.621	1272	1282	1291	rVB	522071	917136	20.98%	2.325%
18	10.756	1298	1305	1315	rBV2	593387	1118486	25.58%	2.835%
19	12.219	1551	1554	1558	rBV3	7747	10399	0.24%	0.026%
20	12.436	1584	1591	1592	rBV3	3363	6432	0.15%	0.016%
21	12.789	1648	1651	1655	rBV3	3758	6325	0.14%	0.016%
22	13.347	1743	1746	1748	rBV2	4742	6020	0.14%	0.015%
23	13.529	1774	1777	1781	rVB2	4788	6324	0.14%	0.016%
24	13.876	1829	1836	1847	rBV	1307376	1897716	43.40%	4.810%
25	14.164	1878	1885	1899	rVB	1418514	2249152	51.44%	5.701%
26	14.469	1930	1937	1944	rBV	920158	1466467	33.54%	3.717%
27	14.687	1968	1974	1984	rBV2	396836	762429	17.44%	1.932%
28	14.845	1999	2001	2003	rBV2	6546	6521	0.15%	0.017%
29	15.468	2098	2107	2114	rBV	1952011	2944841	67.35%	7.464%
30	15.591	2122	2128	2142	rBV	554817	870319	19.91%	2.206%
31	15.709	2144	2148	2154	rVB7	13291	28083	0.64%	0.071%
32	15.832	2167	2169	2174	rVB3	6967	7605	0.17%	0.019%
33	17.219	2398	2405	2413	rBV	1353357	2017001	46.13%	5.112%
34	17.319	2416	2422	2429	rBV2	2363806	3499710	80.04%	8.870%
35	17.895	2515	2520	2524	rBV6	13201	20394	0.47%	0.052%
36	18.417	2605	2609	2612	rBV3	7005	6981	0.16%	0.018%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111524\
Data File : BG063473.D
Acq On : 16 Nov 2024 23:32
Operator : RC/JU
Sample : PB165035BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK035

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Title : SVOA CALIBRATION

37	18.664	2648	2651	2655	rVB4	4337	6152	0.14%	0.016%
38	18.917	2691	2694	2697	rBV3	3940	6252	0.14%	0.016%
39	19.181	2734	2739	2744	rBV4	41549	59944	1.37%	0.152%
40	19.252	2747	2751	2757	rBV2	34434	56979	1.30%	0.144%
41	19.622	2807	2814	2823	rBV	2971213	4372313	100.00%	11.082%
42	20.168	2905	2907	2910	rBV4	9793	8838	0.20%	0.022%
43	21.373	3108	3112	3119	rVB	142536	189391	4.33%	0.480%
44	21.473	3123	3129	3136	rBV	1468502	2353623	53.83%	5.965%
45	24.305	3601	3611	3624	rVB	1666138	4301127	98.37%	10.901%
46	24.510	3637	3646	3663	rVB	947376	2492989	57.02%	6.319%




Sum of corrected areas: 39454786

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111524\
Data File : BG063473.D
Acq On : 16 Nov 2024 23:32
Operator : RC/JU
Sample : PB165035BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK035

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

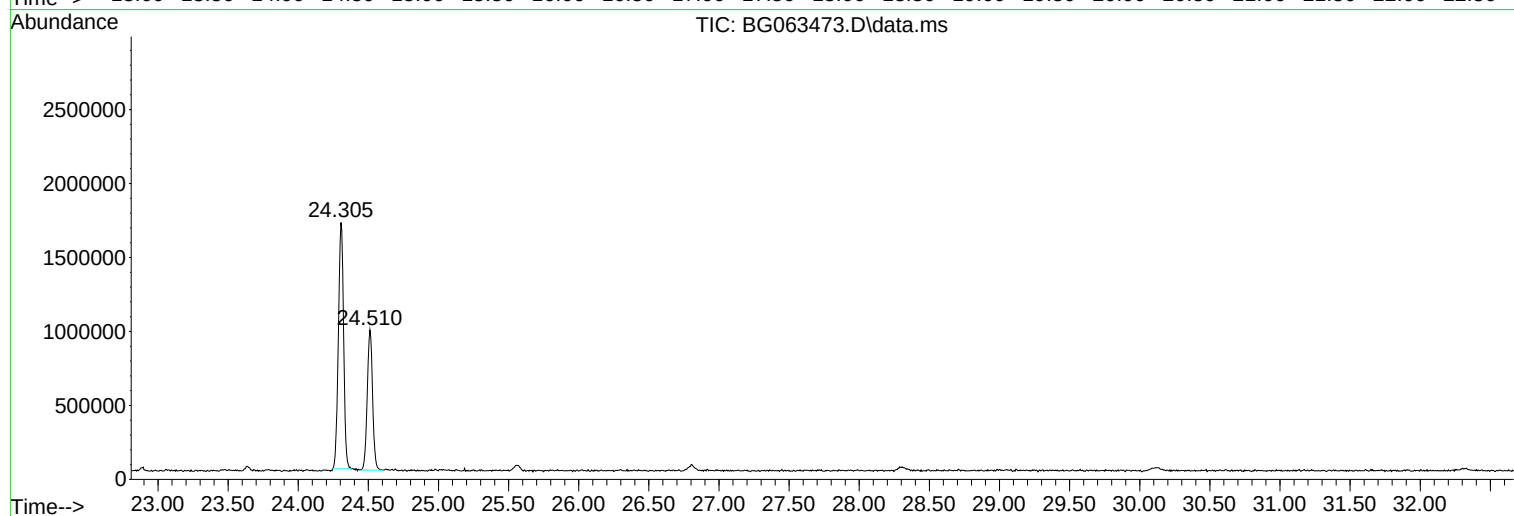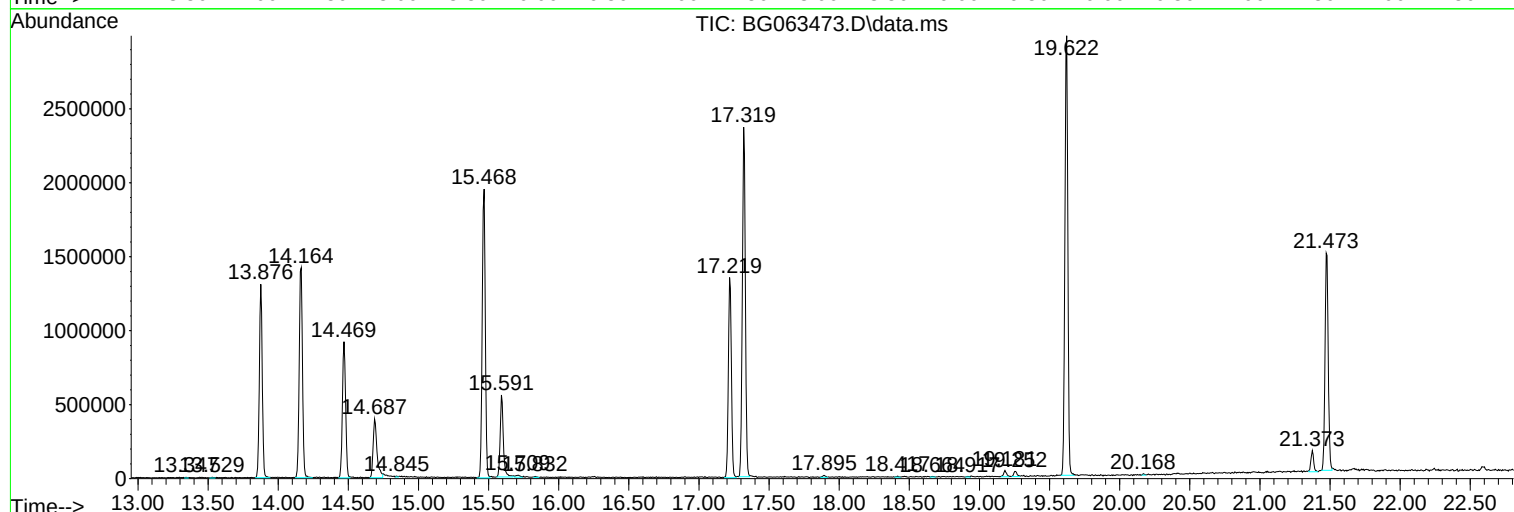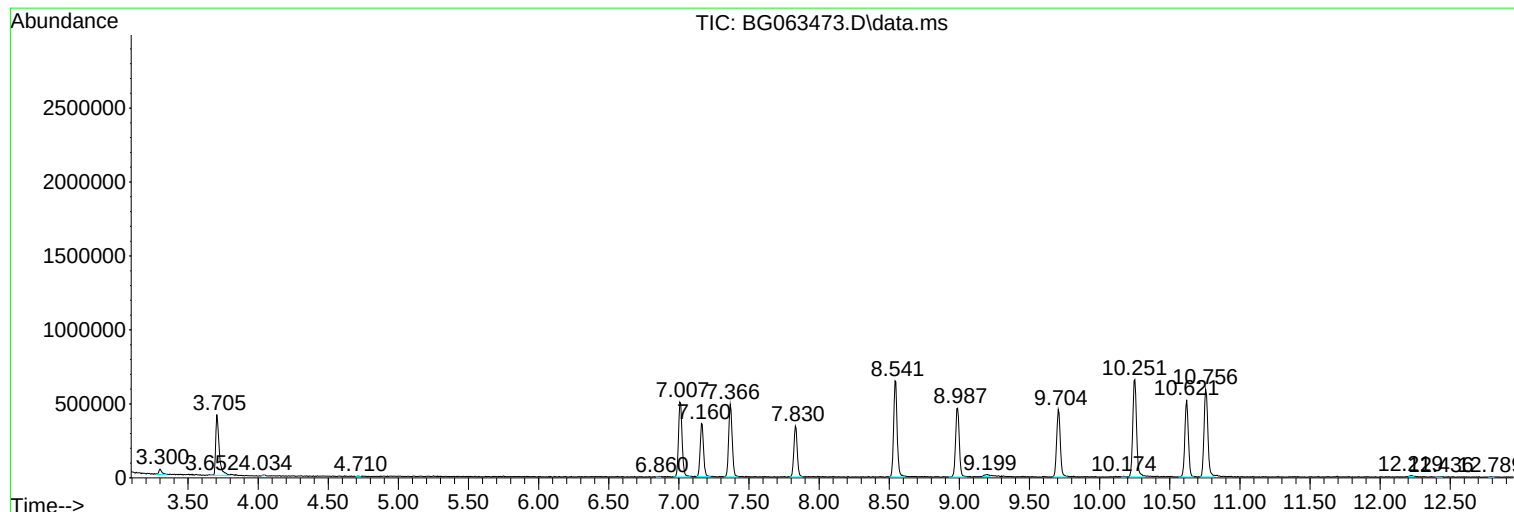

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111524\
Data File : BG063473.D
Acq On : 16 Nov 2024 23:32
Operator : RC/JU
Sample : PB165035BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK035

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111524\
Data File : BG063473.D
Acq On : 16 Nov 2024 23:32
Operator : RC/JU
Sample : PB165035BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK035

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc