
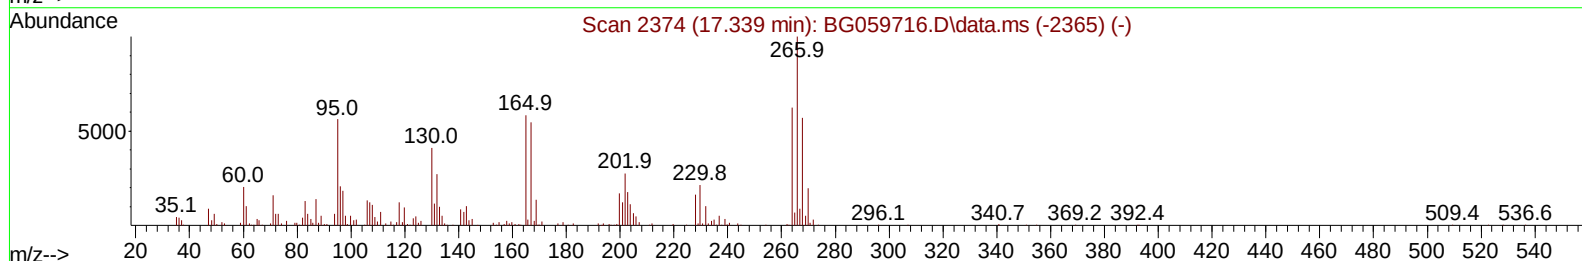
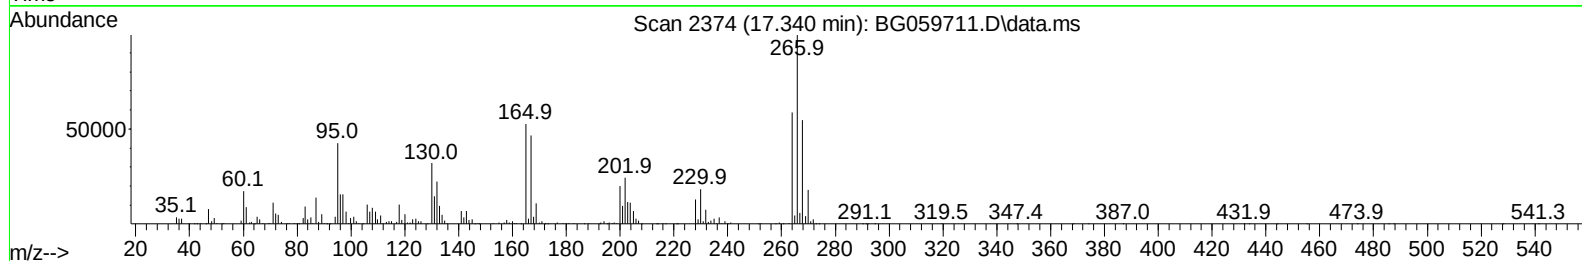


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111623\
Data File : BG059711.D
Acq On : 16 Nov 2023 10:07
Operator : MA/JU
Sample : DFTTP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 16 17:21:02 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 16 17:15:56 2023
Response via : Initial Calibration

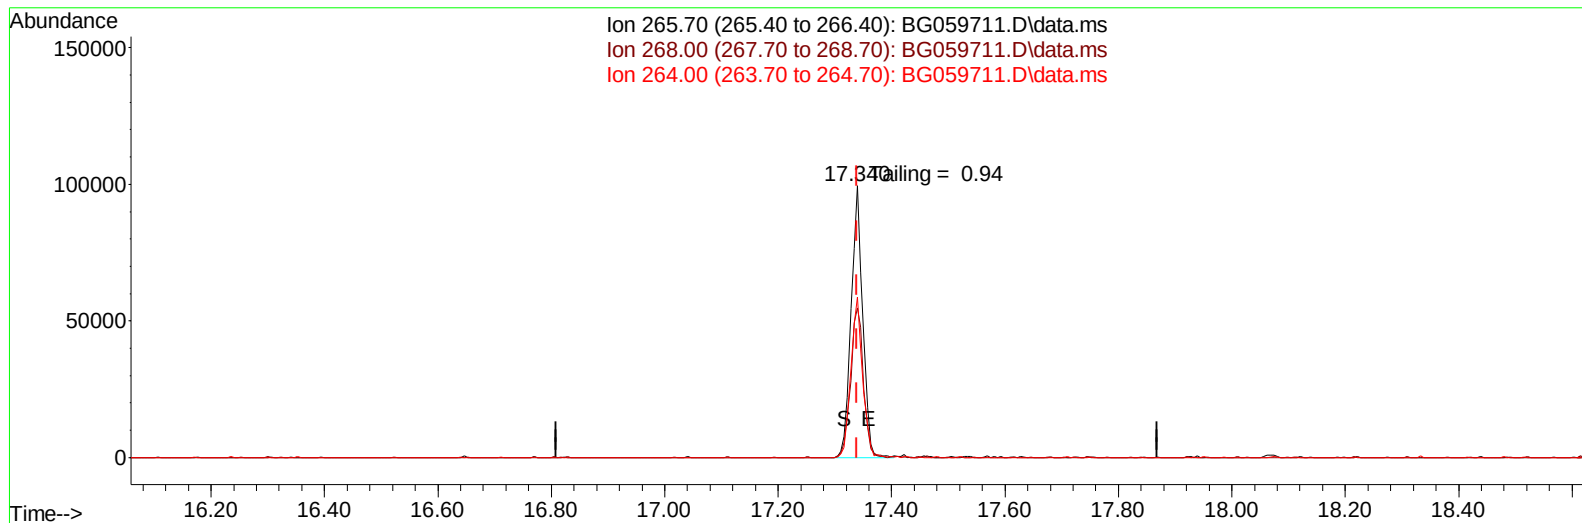

TIC: BG059711.D\data.ms

(70) Pentachlorophenol (C)




17.340min (+ 0.001) 233024.82 ng

response 140822

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	57.10	55.02
264.00	62.30	58.96
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111623\
Data File : BG059711.D
Acq On : 16 Nov 2023 10:07
Operator : MA/JU
Sample : DFTTP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 16 17:21:02 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 16 17:15:56 2023
Response via : Initial Calibration

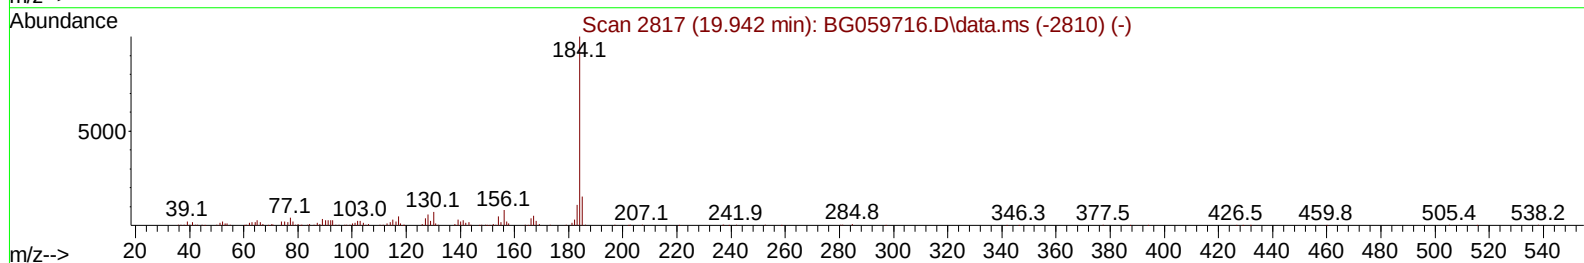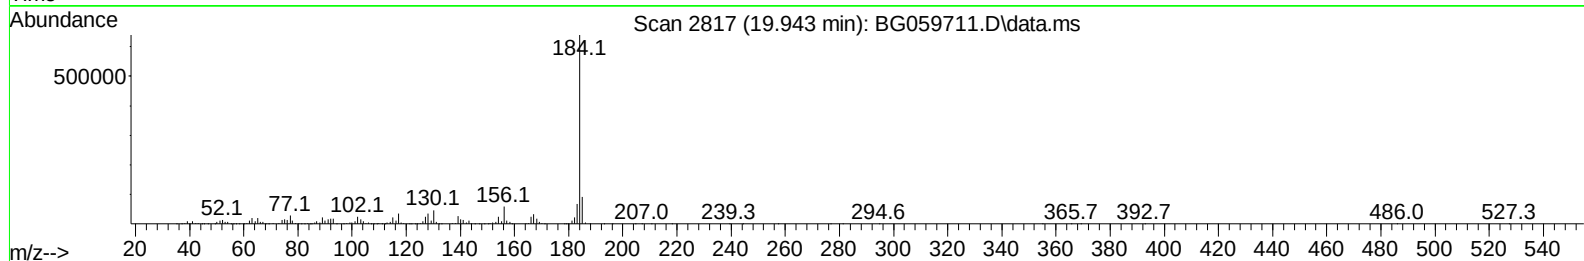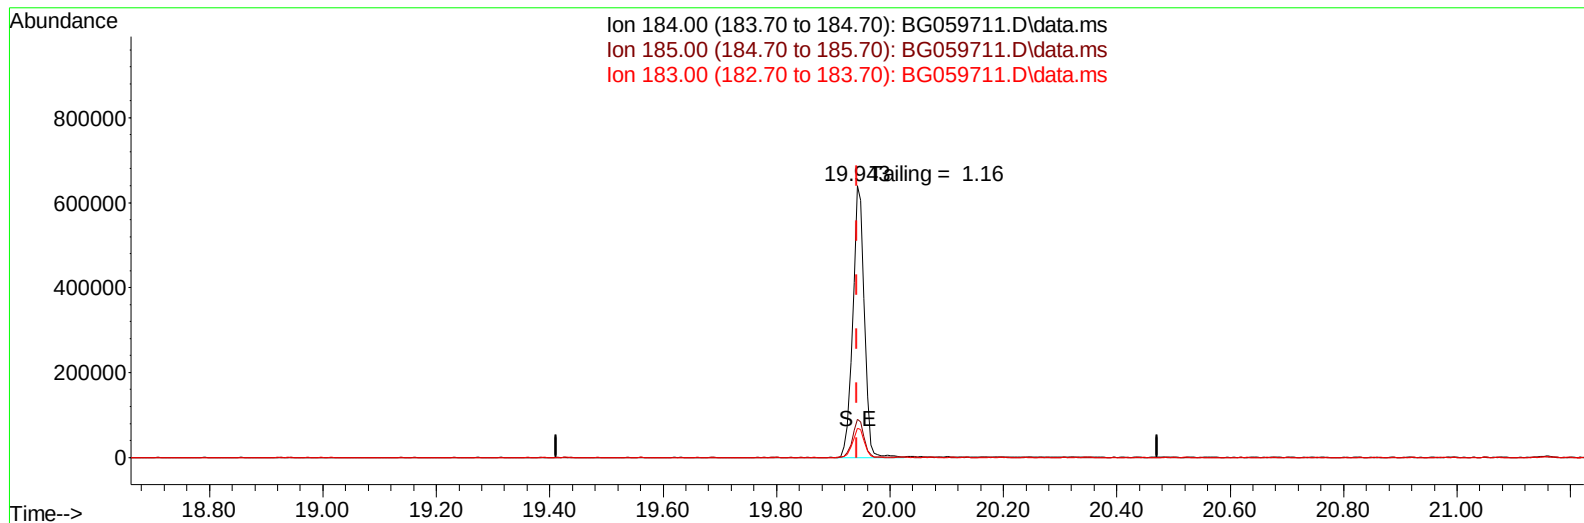

TIC: BG059711.D\data.ms

(77) Benzydine**19.943min (+ 0.001) 615326.11 ng****response 906944**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.11
183.00	11.00	10.67
0.00	0.00	0.00