


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111623\
 Data File : BG059711.D
 Acq On : 16 Nov 2023 10:07
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111623.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Nov 17 01:51:38 2023

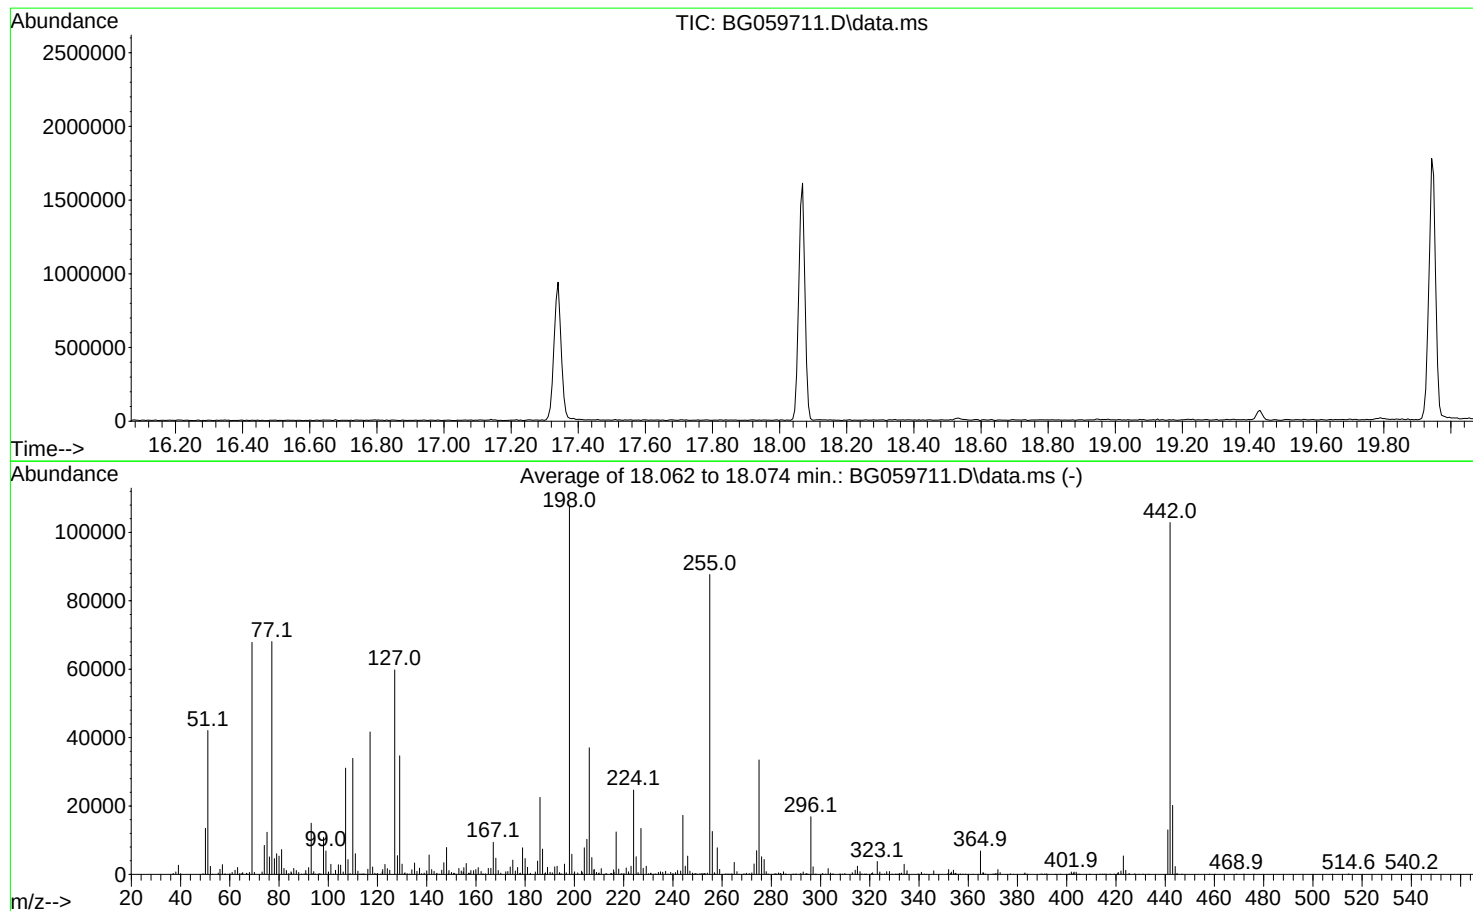




AutoFind: Scans 2497, 2498, 2499; Background Corrected with Scan 2490

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.1	42056	PASS
68	69	0.00	2	0.8	575	PASS
69	198	0.00	100	63.1	67832	PASS
70	69	0.00	2	0.9	617	PASS
127	198	10	80	55.6	59816	PASS
197	198	0.00	2	0.4	451	PASS
198	198	100	100	100.0	107576	PASS
199	198	5	9	5.5	5895	PASS
275	198	10	60	31.1	33451	PASS
365	198	1	100	6.4	6855	PASS
441	198	0.01	100	12.1	13029	PASS
442	442	50	100	100.0	102904	PASS
443	442	15	24	19.6	20168	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111623\
Data File : BG059711.D
Acq On : 16 Nov 2023 10:07
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Nov 16 17:21:02 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 16 17:15:56 2023
Response via : Initial Calibration

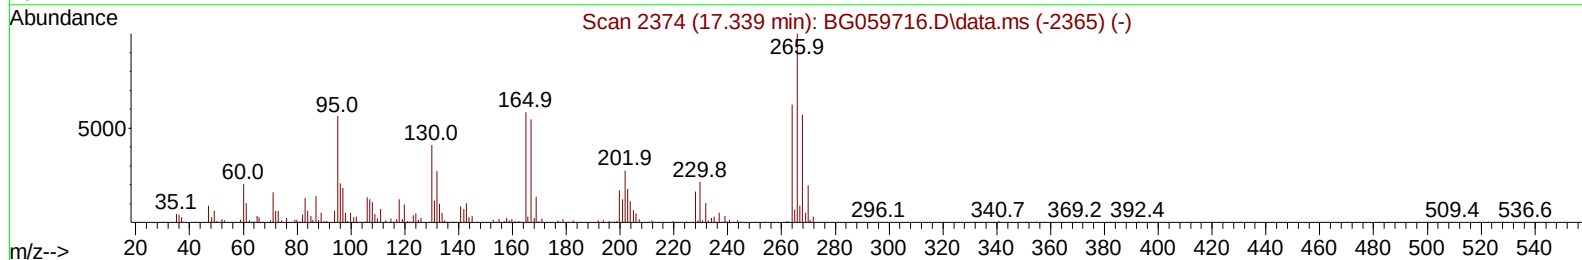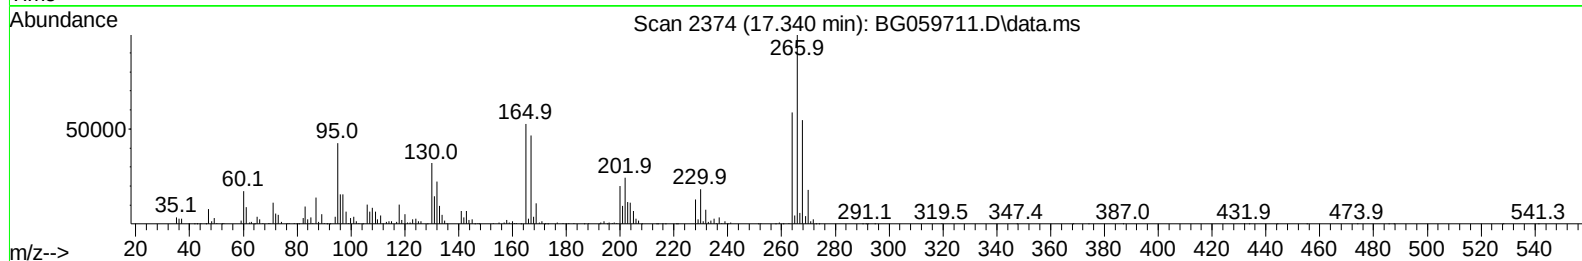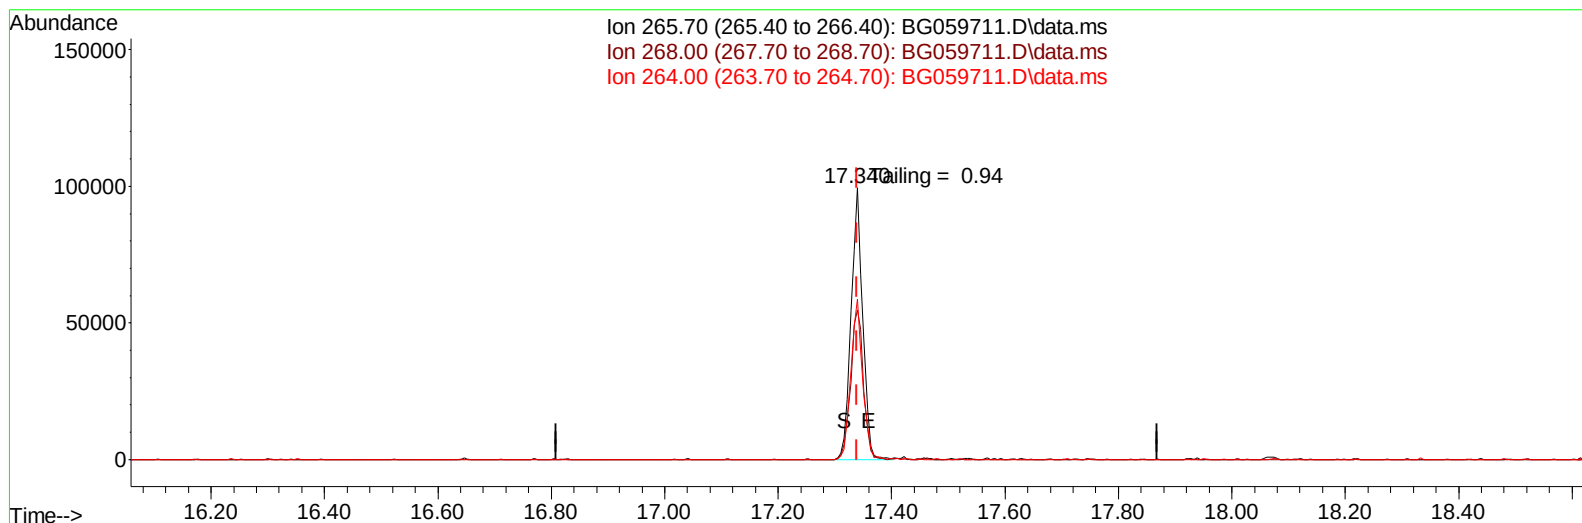

TIC: BG059711.D\data.ms

(70) Pentachlorophenol (C)

17.340min (+ 0.001) 233024.82 ng




response 140822

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	57.10	55.02
264.00	62.30	58.96
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111623\
Data File : BG059711.D
Acq On : 16 Nov 2023 10:07
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Nov 16 17:21:02 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 16 17:15:56 2023
Response via : Initial Calibration

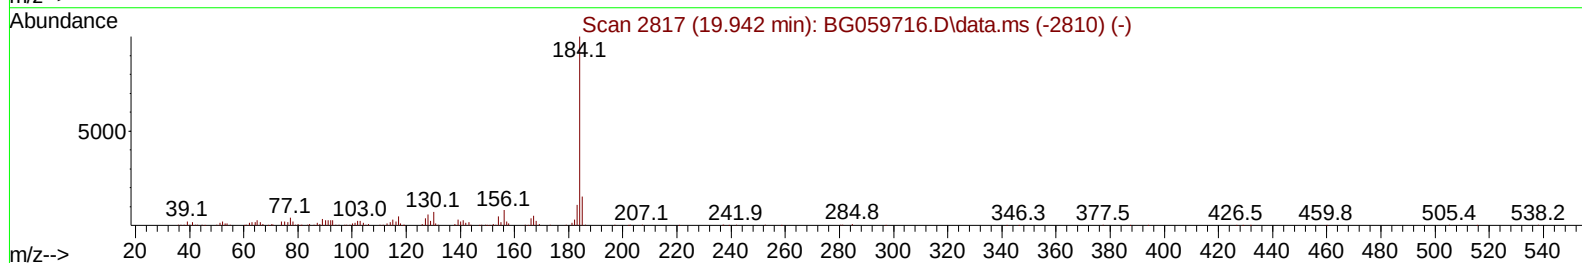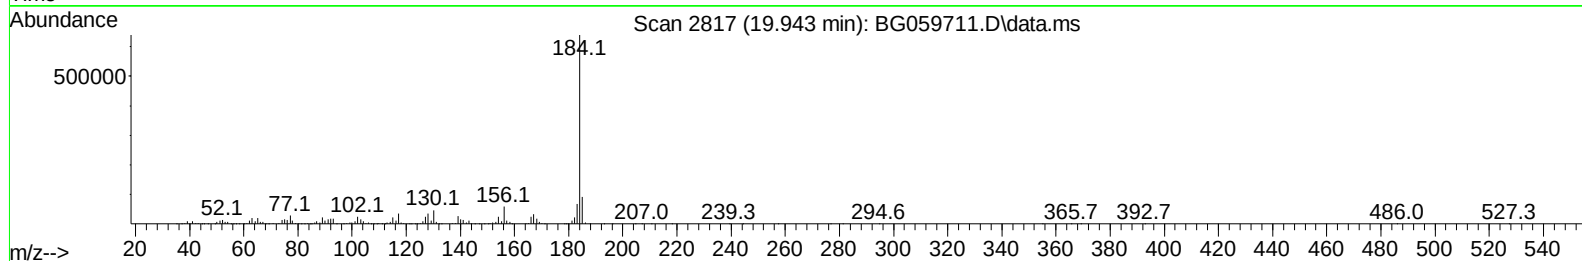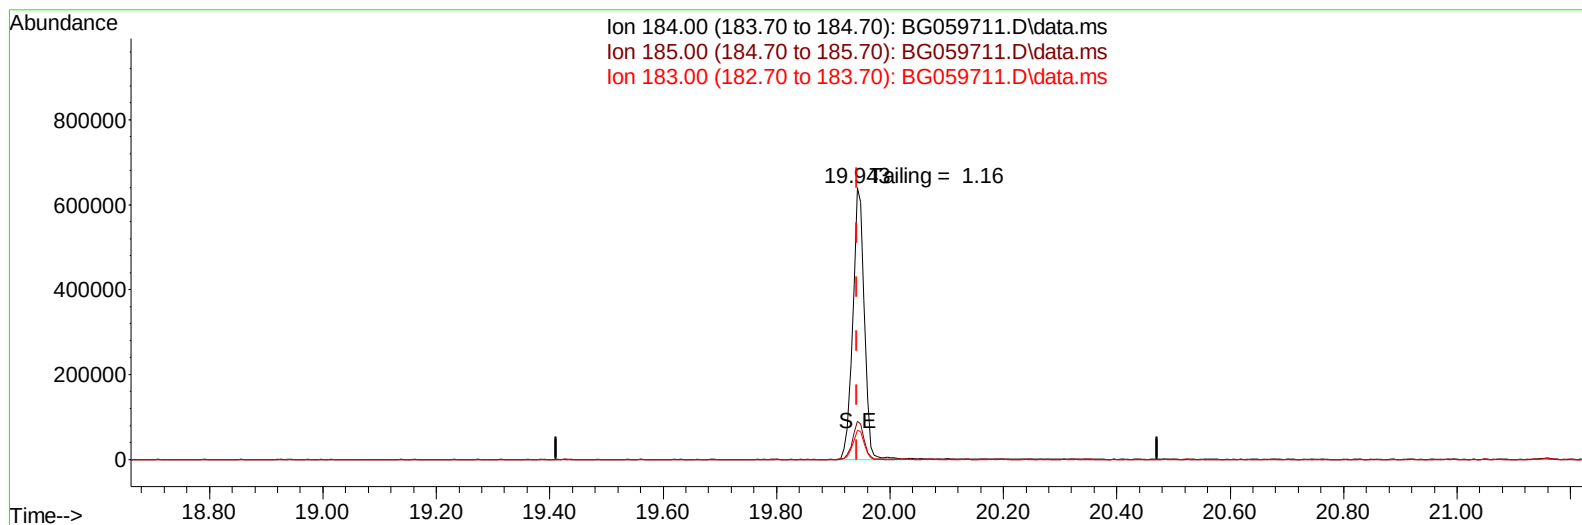

TIC: BG059711.D\data.ms

(77) Benzidine

19.943min (+ 0.001) 615326.11 ng

response 906944

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.11
183.00	11.00	10.67
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/16/2023	BNA_G	<u>BG059711.D</u>
Compound Name	Response	Retention Time
DDT	493181	21.153
DDD	4500	20.742
DDE	0	20.146
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4500	497681	0.90

Instrument :
BNA_G
ClientSampleId :
DFTPP