
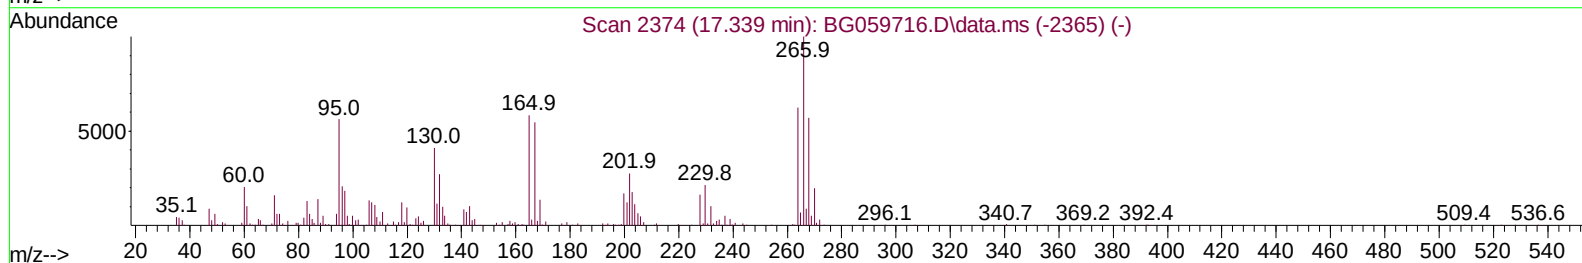
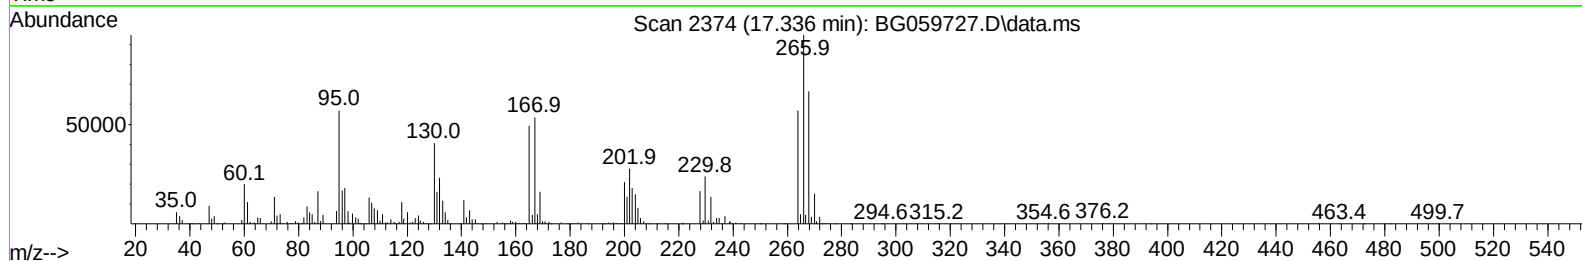


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111723\
Data File : BG059727.D
Acq On : 17 Nov 2023 10:03
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 17 13:45:22 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 17 01:51:38 2023
Response via : Initial Calibration

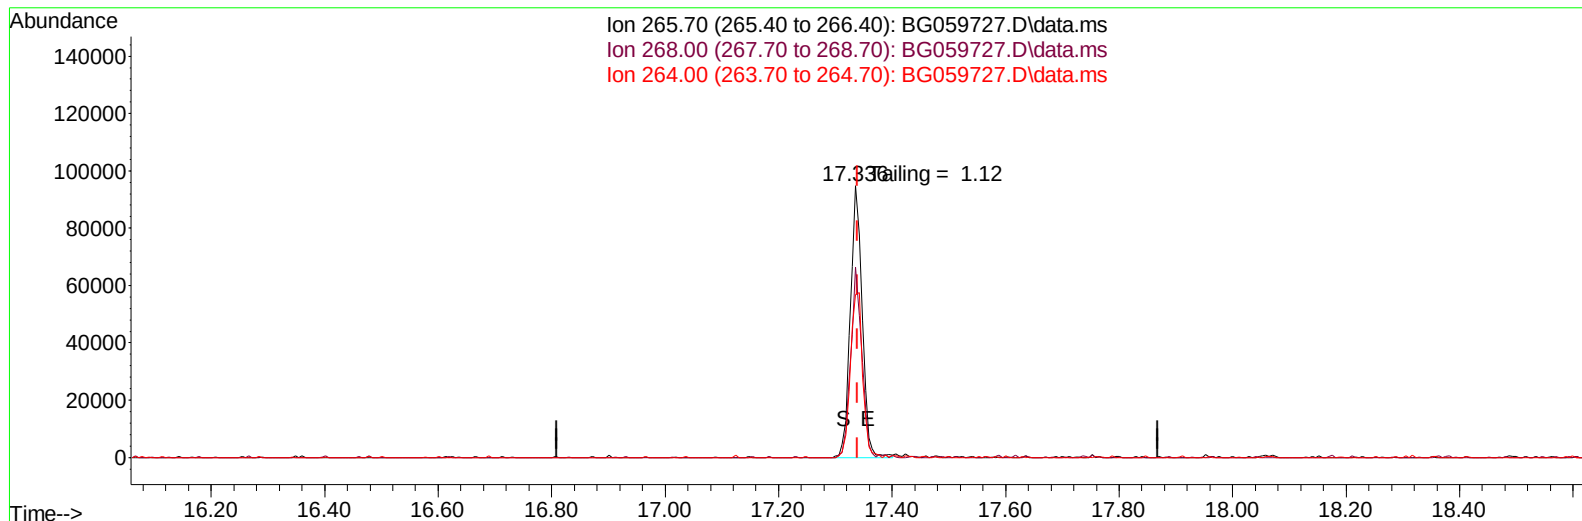

TIC: BG059727.D\data.ms

(70) Pentachlorophenol (C)




17.336min (-0.003) 140483.76 ng

response 135406

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	57.10	70.21#
264.00	62.30	60.05
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111723\
Data File : BG059727.D
Acq On : 17 Nov 2023 10:03
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 17 13:45:22 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 17 01:51:38 2023
Response via : Initial Calibration

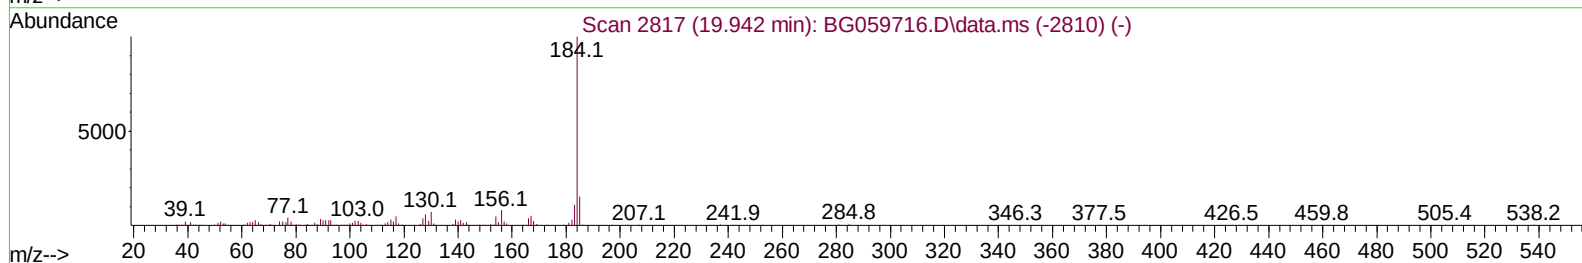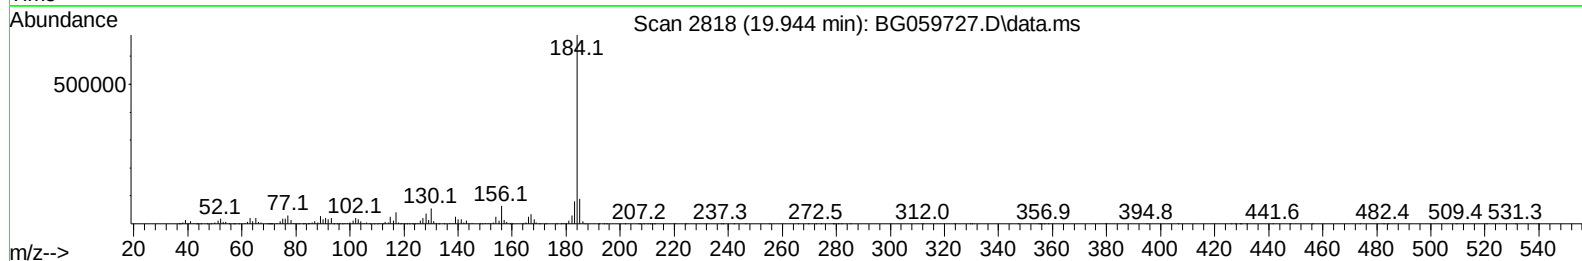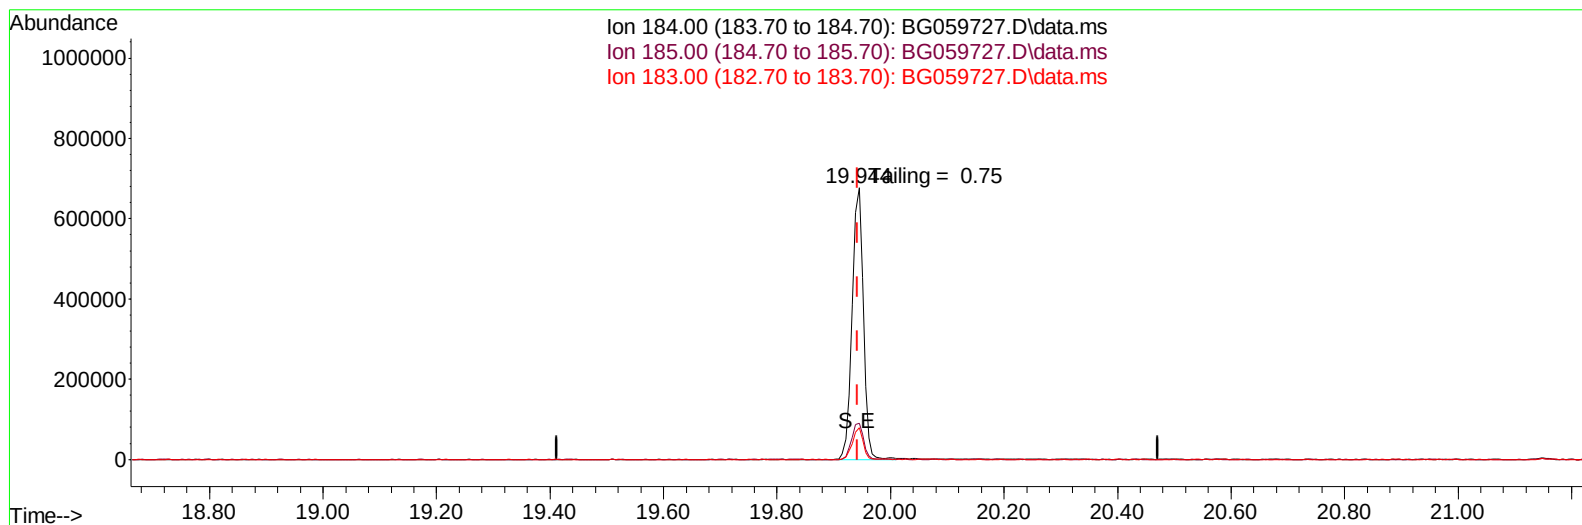

TIC: BG059727.D\data.ms

(77) Benzidine**19.944min (+ 0.003) 236651.43 ng****response 922995**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	13.41
183.00	11.00	11.74
0.00	0.00	0.00