
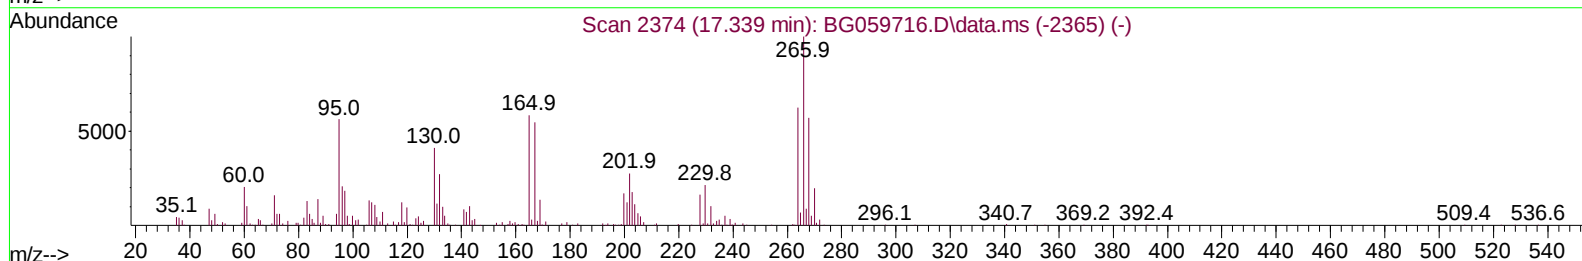
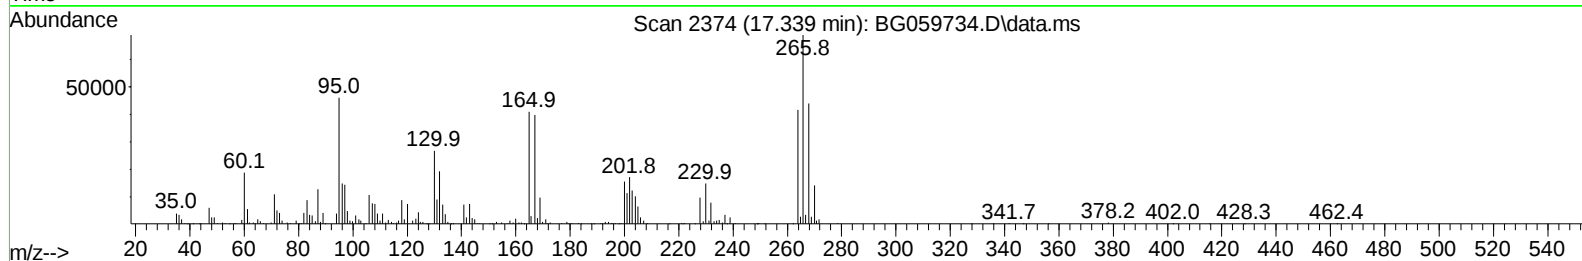


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111723\
Data File : BG059734.D
Acq On : 17 Nov 2023 16:46
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 17 17:32:27 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 17 01:51:38 2023
Response via : Initial Calibration

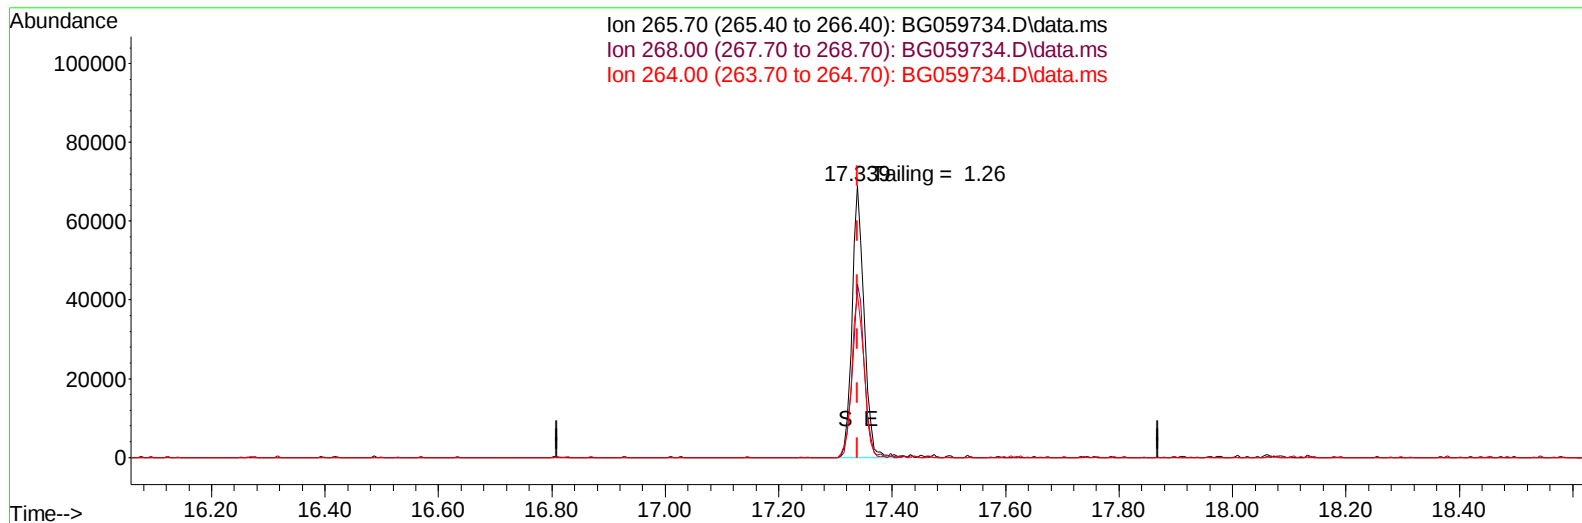

TIC: BG059734.D\data.ms

(70) Pentachlorophenol (C)




17.339min (-0.000) 95398.24 ng

response 101437

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	57.10	63.85
264.00	62.30	60.32
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111723\
Data File : BG059734.D
Acq On : 17 Nov 2023 16:46
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 17 17:32:27 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 17 01:51:38 2023
Response via : Initial Calibration

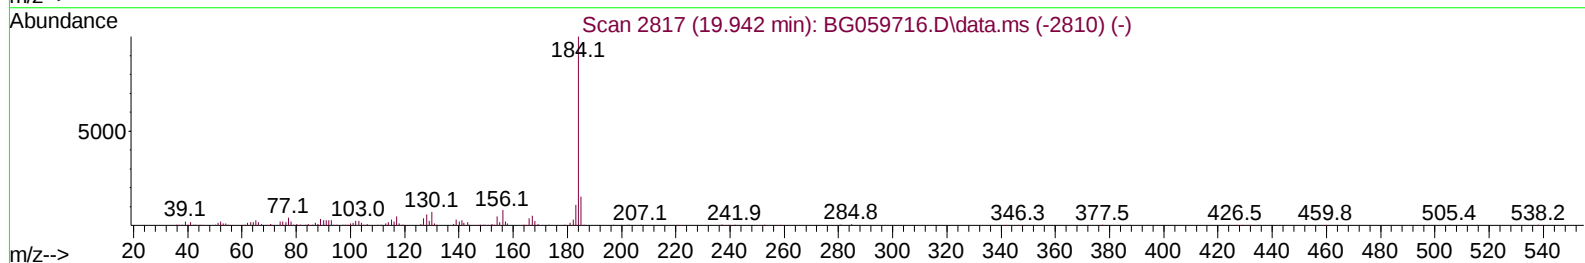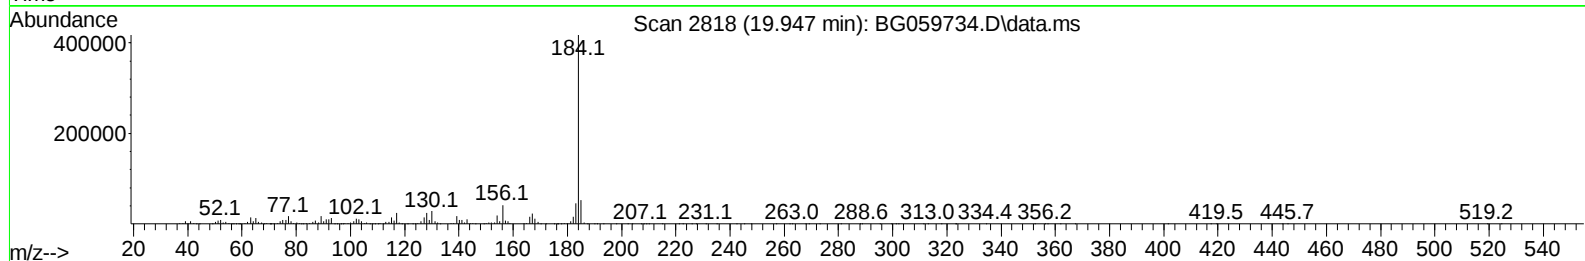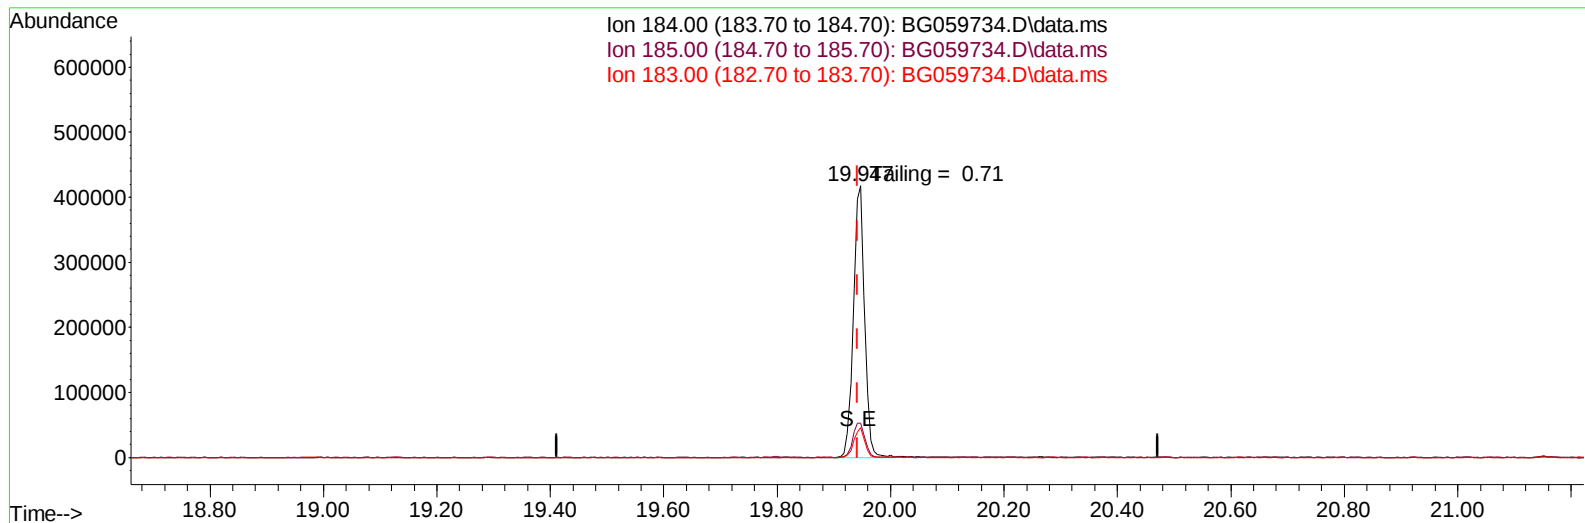

TIC: BG059734.D\data.ms

(77) Benzidine**19.947min (+ 0.006) 385881.36 ng****response 577510**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	12.55
183.00	11.00	11.01
0.00	0.00	0.00