
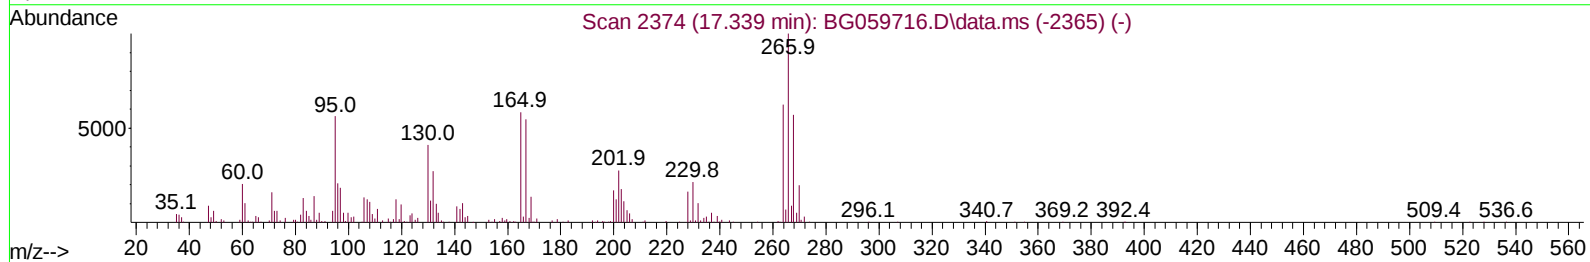
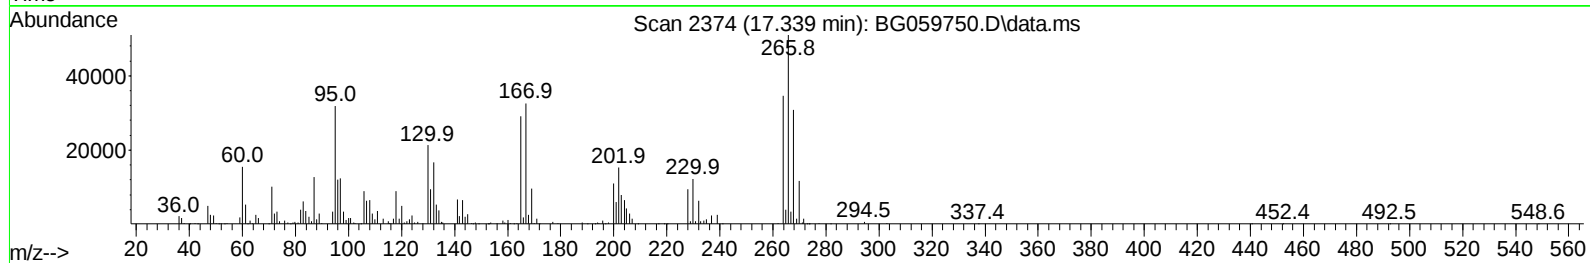


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111723\
Data File : BG059750.D
Acq On : 18 Nov 2023 5:08
Operator : MA/JU
Sample : DFTTP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 20 07:51:54 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 17 01:51:38 2023
Response via : Initial Calibration

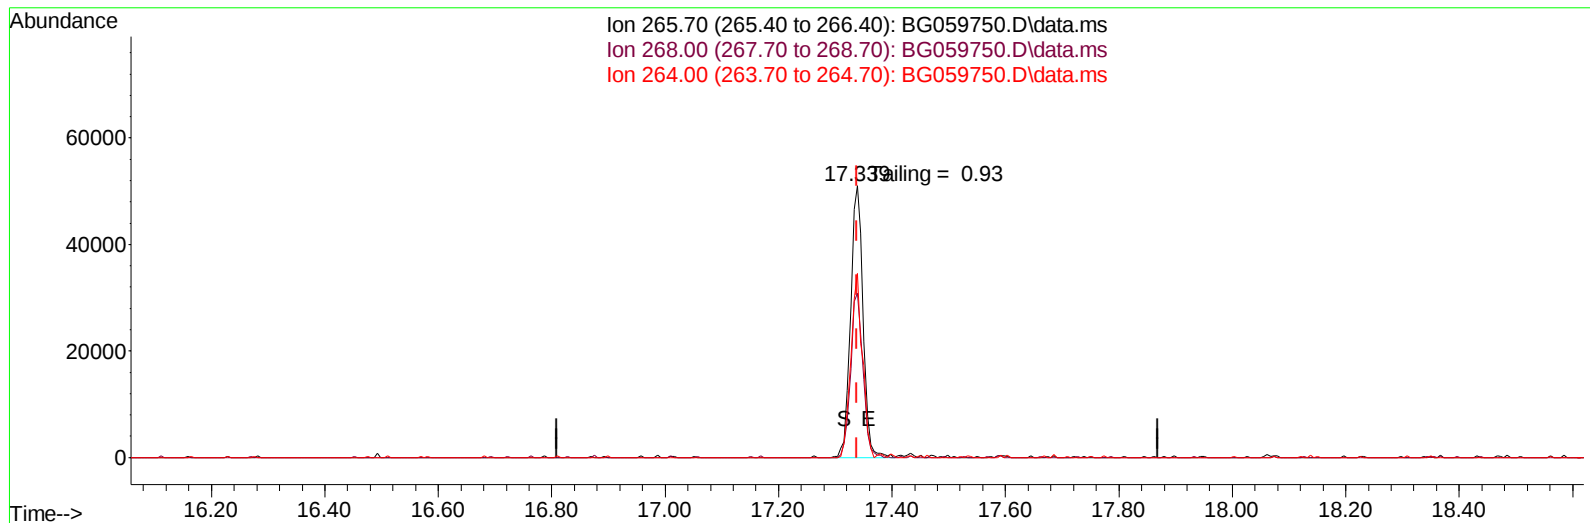

TIC: BG059750.D\data.ms

(70) Pentachlorophenol (C)




17.339min (+ 0.000) 157125.46 ng

response 78127

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	57.10	60.47
264.00	62.30	67.89
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111723\
Data File : BG059750.D
Acq On : 18 Nov 2023 5:08
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 20 07:51:54 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 17 01:51:38 2023
Response via : Initial Calibration

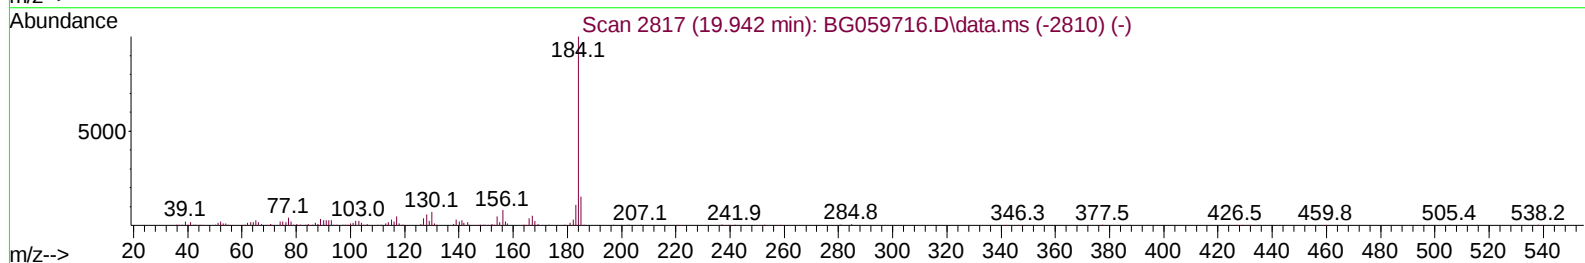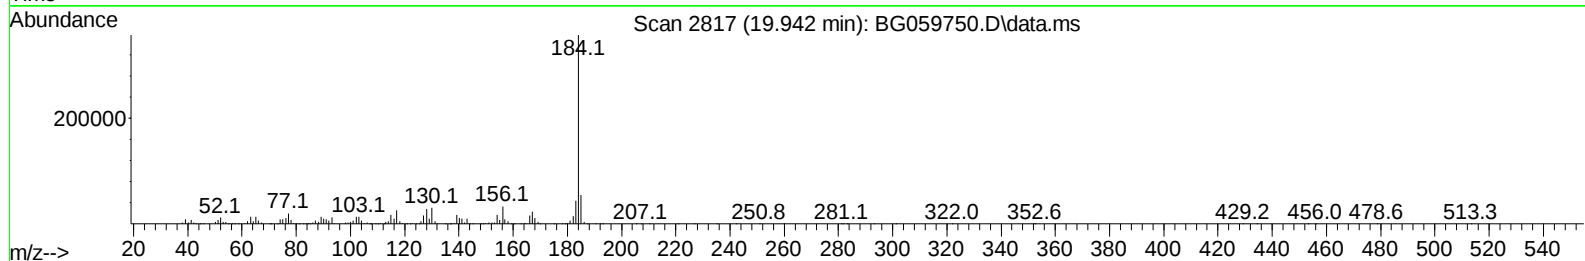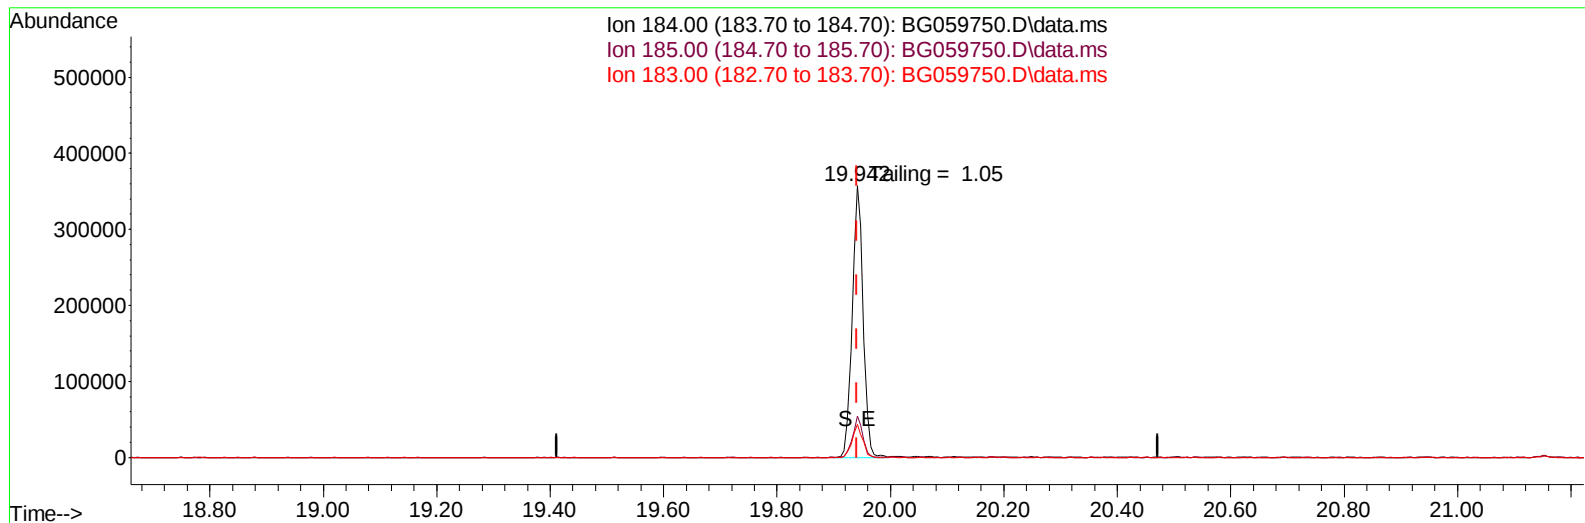

TIC: BG059750.D\data.ms

(77) Benzidine**19.942min (+ 0.000) 69956.37 ng****response 480653**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	15.16
183.00	11.00	12.24
0.00	0.00	0.00